
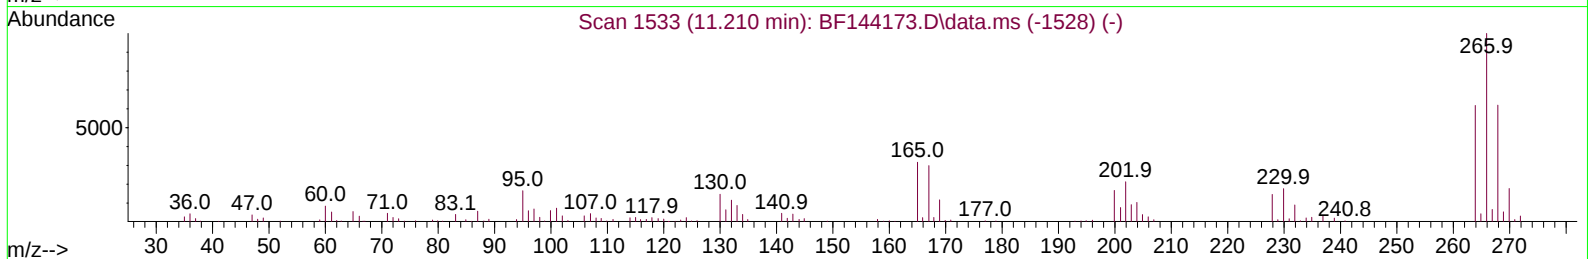
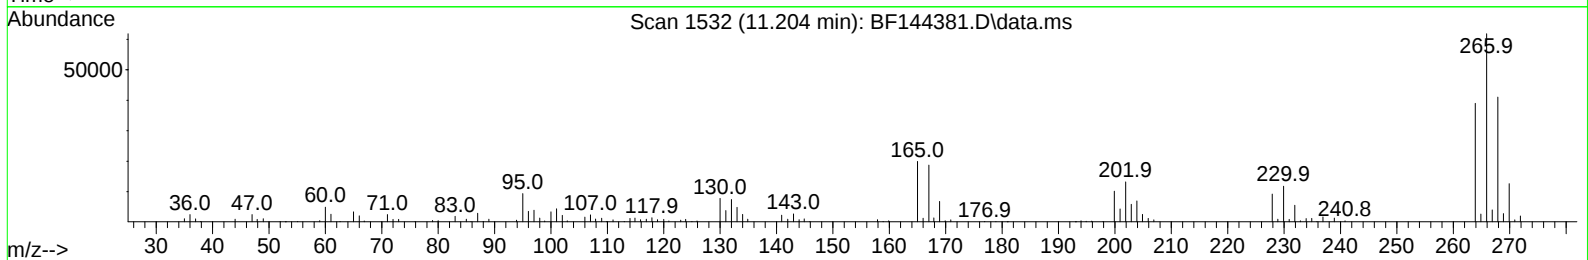


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120125\
Data File : BF144381.D
Acq On : 01 Dec 2025 12:12
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 01 13:16:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

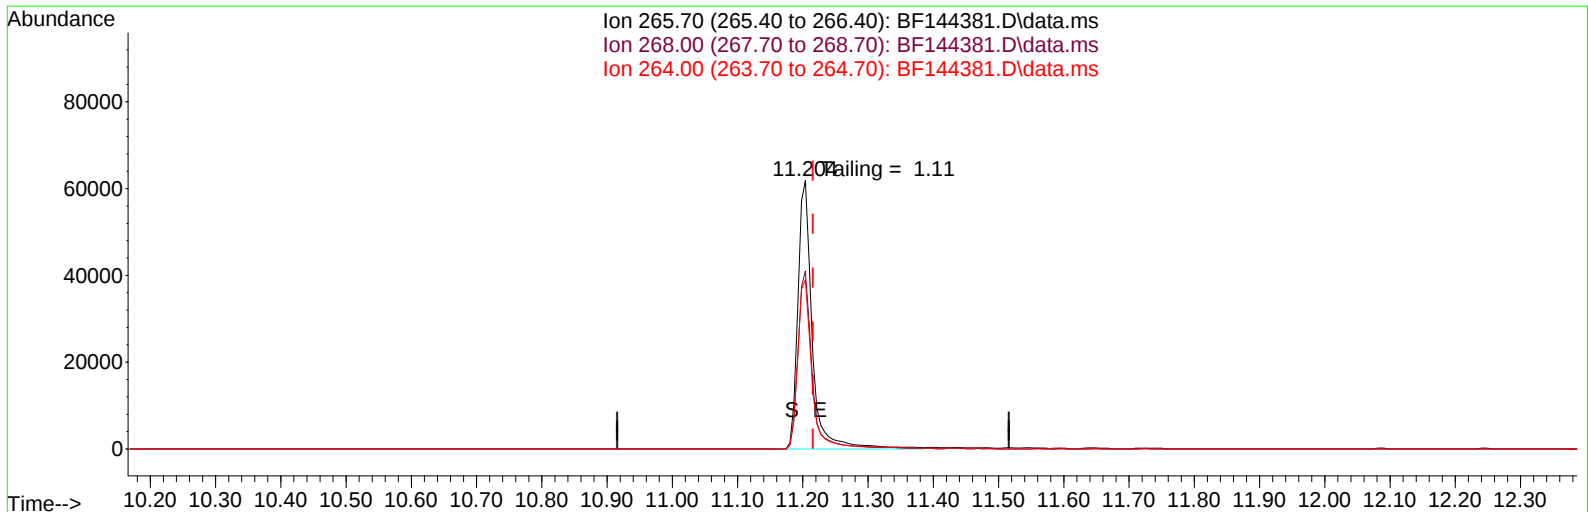

TIC: BF144381.D\data.ms

(70) Pentachlorophenol (C)




11.204min (-0.012) 40255.49 ng

response 94933

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	66.35
264.00	61.80	63.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120125\
Data File : BF144381.D
Acq On : 01 Dec 2025 12:12
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 01 13:16:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

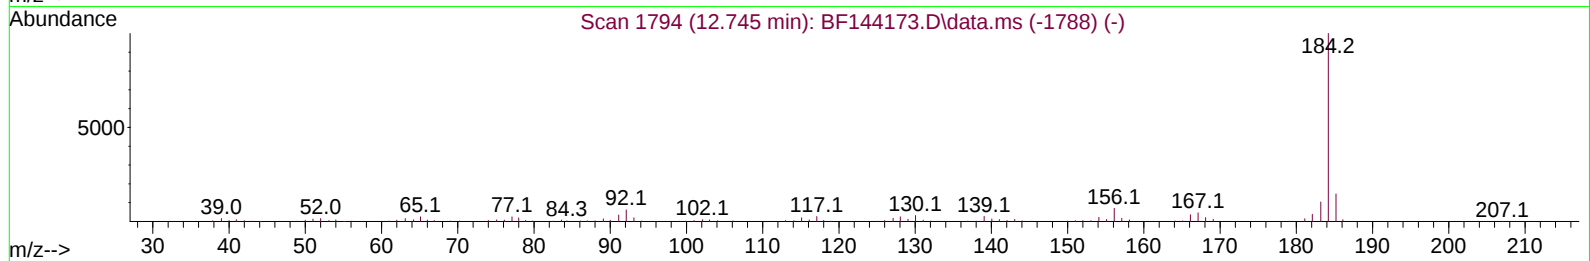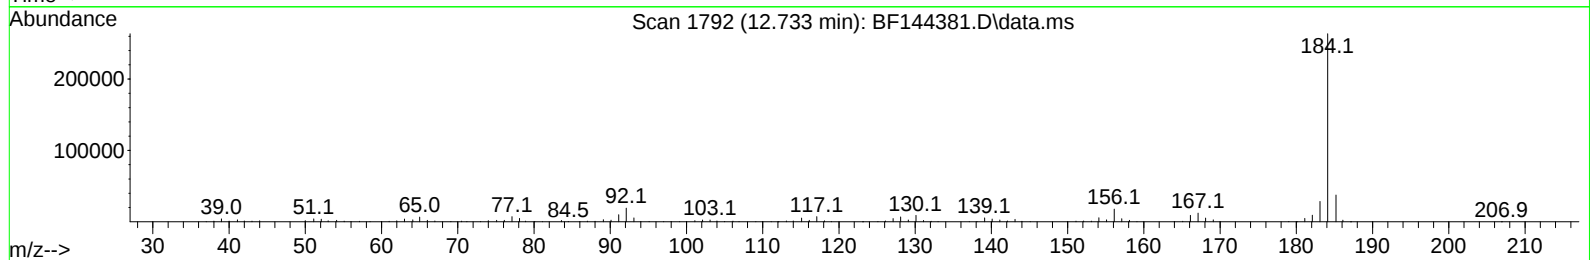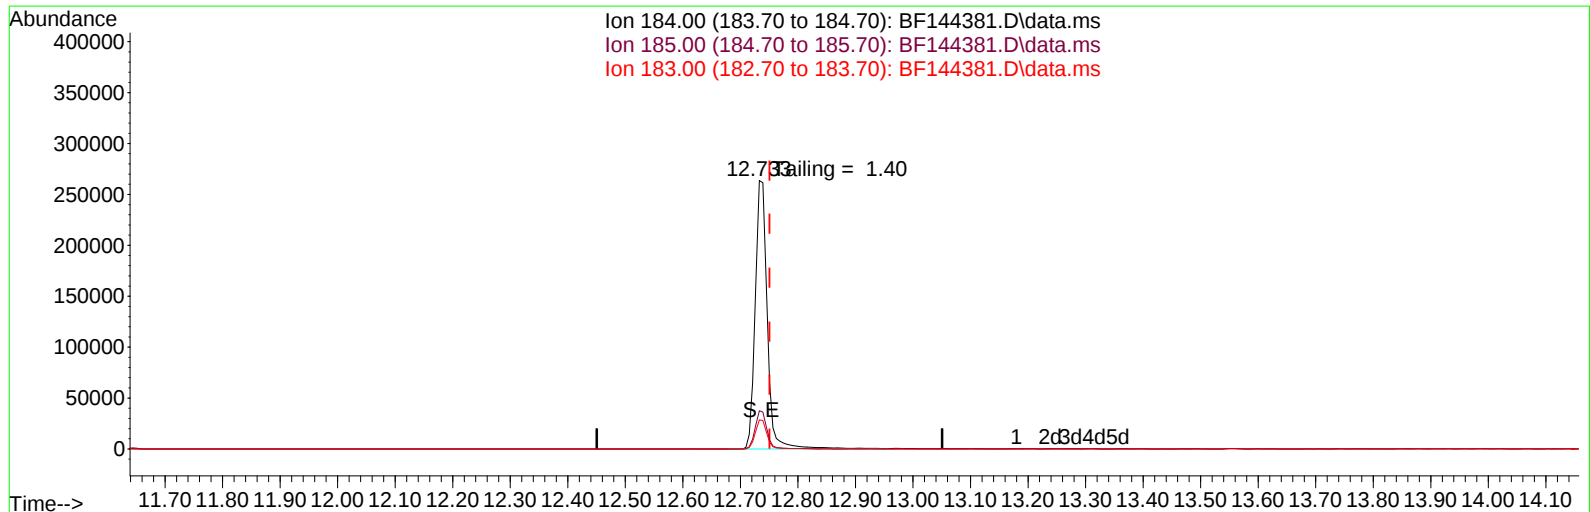

TIC: BF144381.D\data.ms

(77) Benzidine

12.733min (-0.018) 33019.21 ng m

response 387744

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.21
183.00	10.40	10.81
0.00	0.00	0.00