
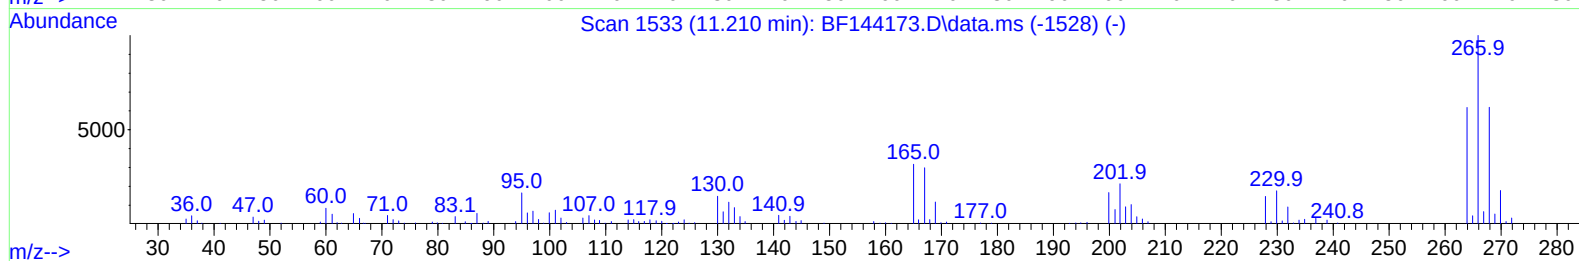
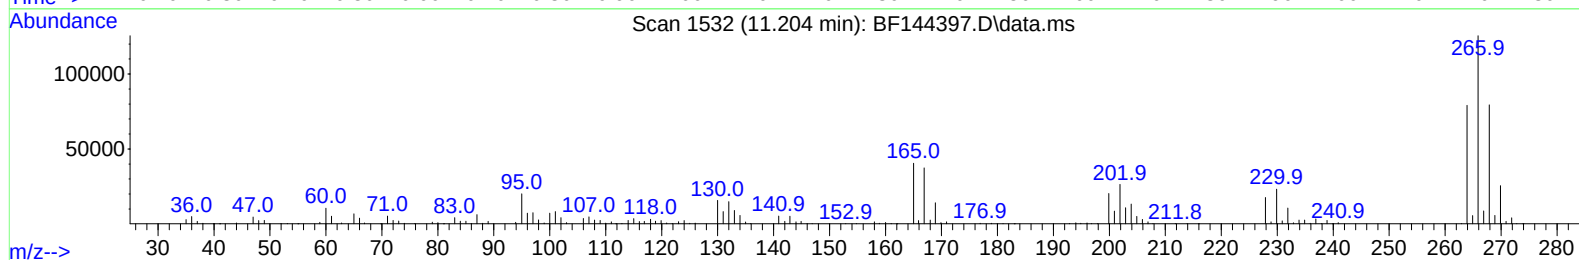


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120225\
Data File : BF144397.D
Acq On : 02 Dec 2025 10:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 02 10:51:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

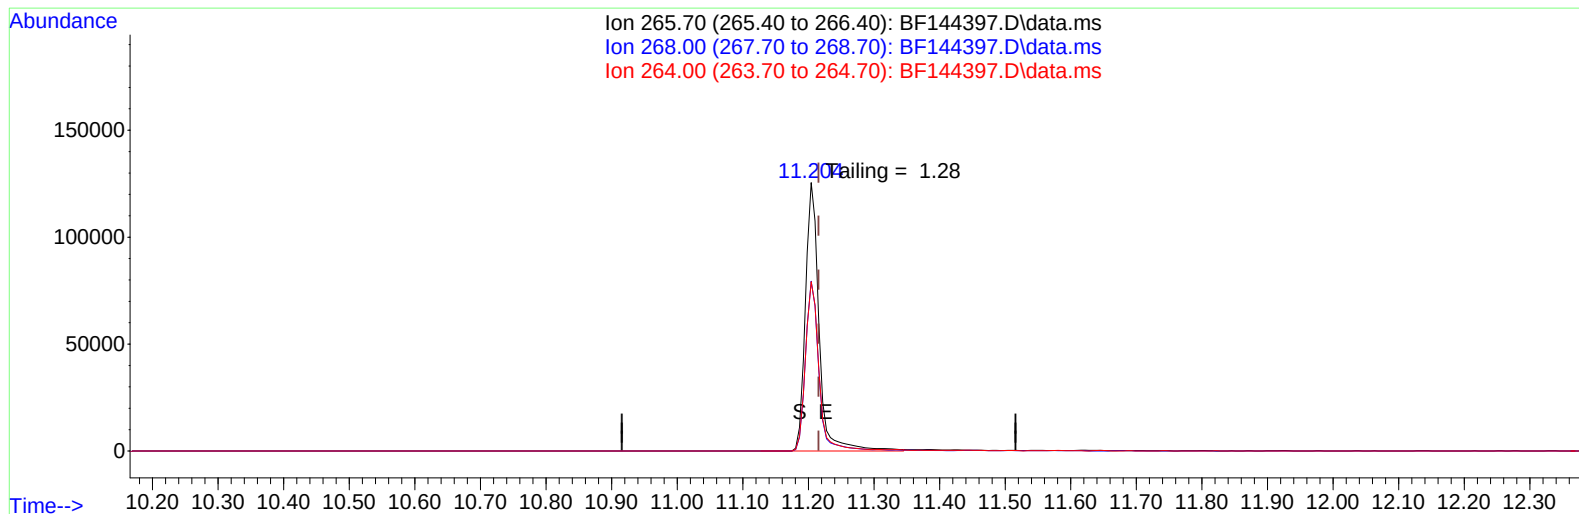

TIC: BF144397.D\data.ms

(70) Pentachlorophenol (C)




11.204min (-0.012) 36284.74 ng

response 183362

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	63.26
264.00	61.80	63.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120225\
Data File : BF144397.D
Acq On : 02 Dec 2025 10:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 02 10:51:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

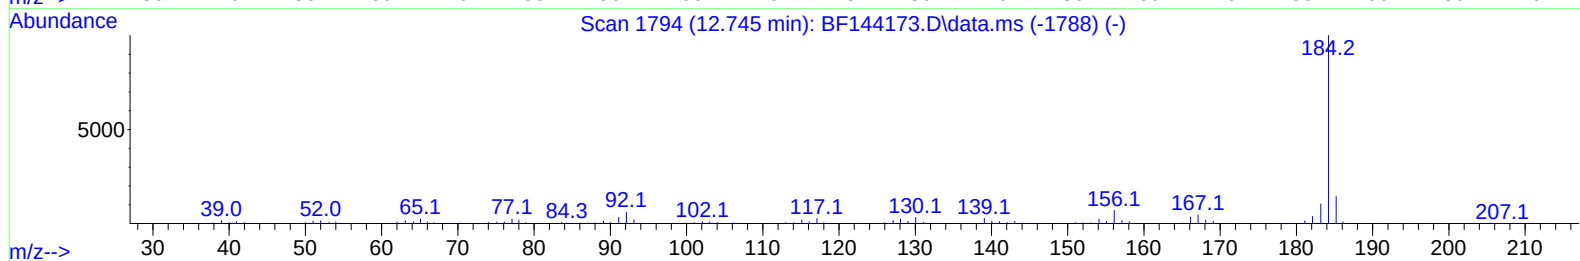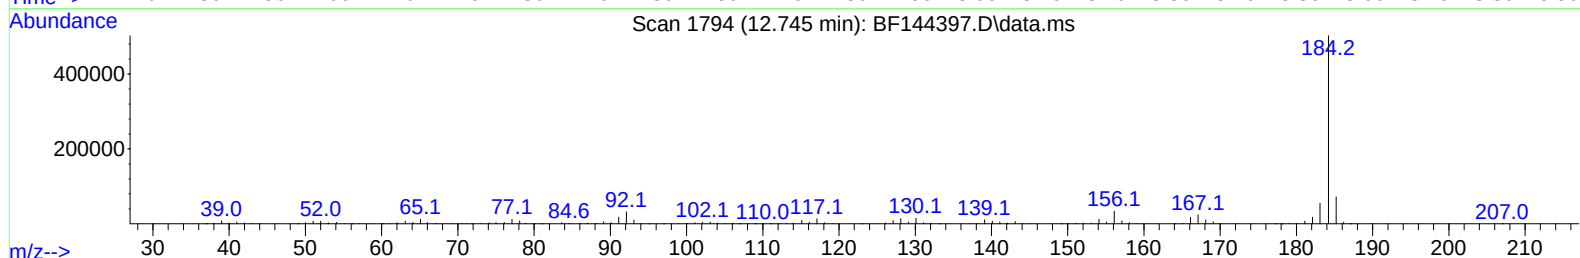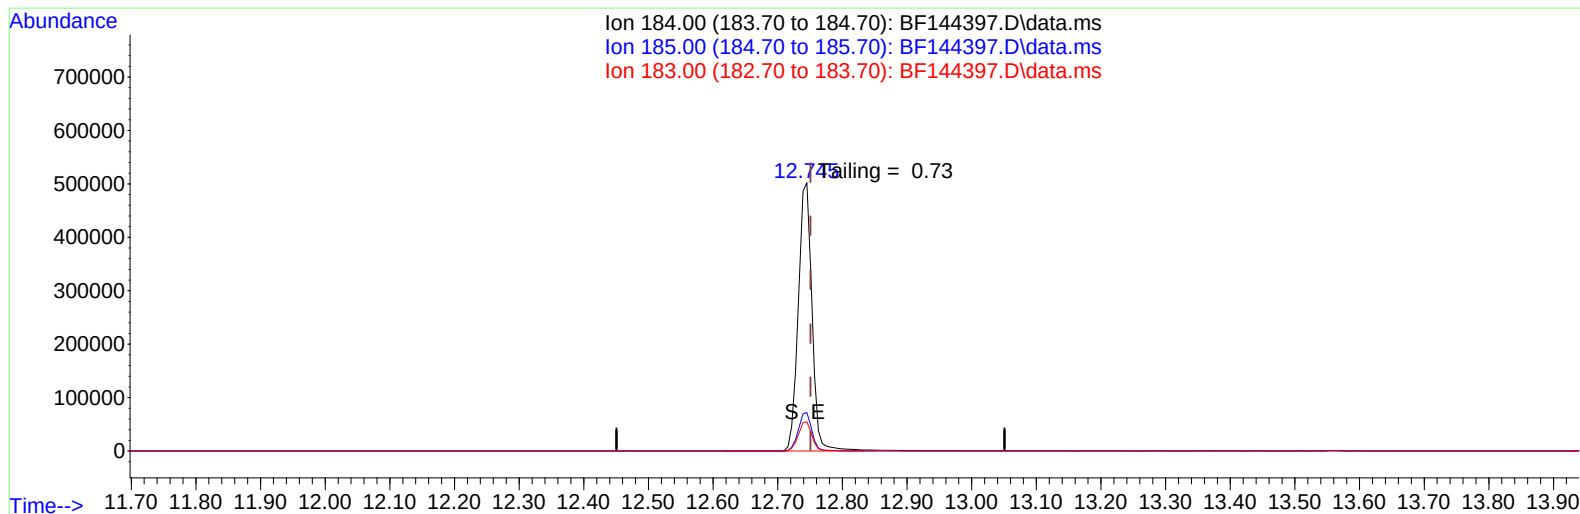

TIC: BF144397.D\data.ms

(77) Benzidine

12.745min (-0.006) 20356.93 ng

response 746056

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.33
183.00	10.40	10.92
0.00	0.00	0.00