
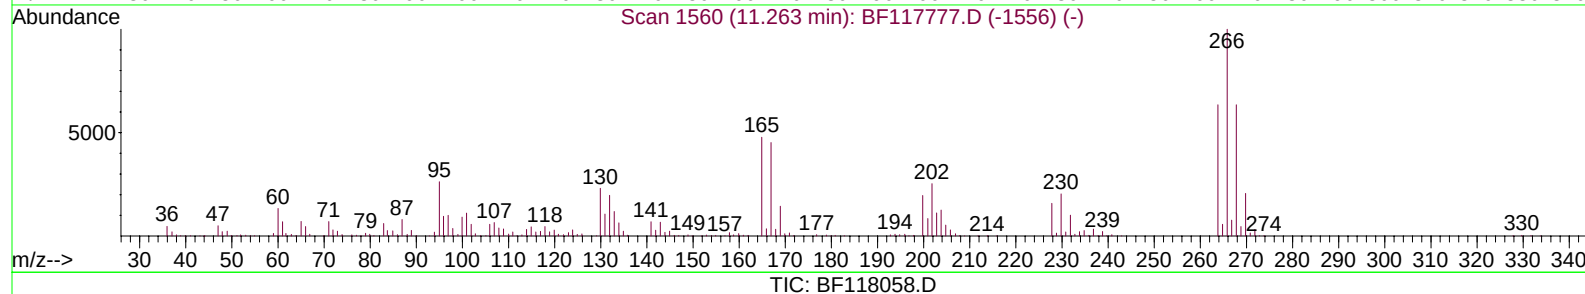
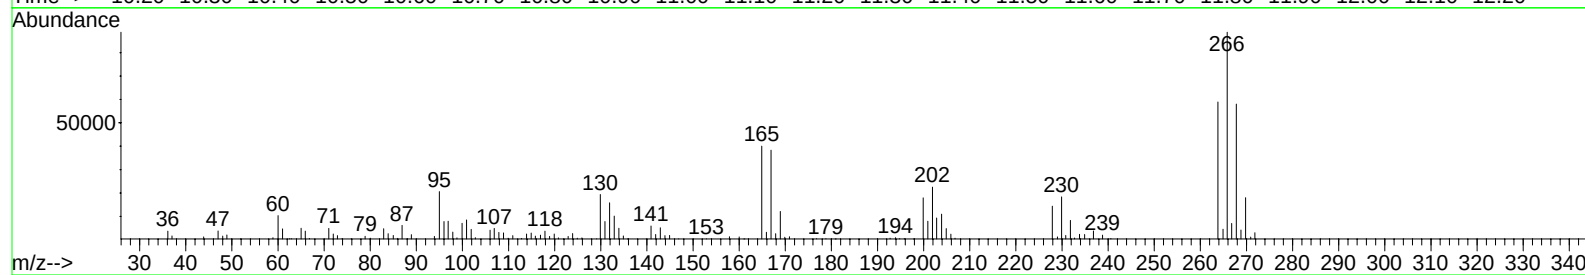


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF120319\
Data File : BF118058.D
Acq On : 3 Dec 2019 12:46
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 03 16:35:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 03 15:16:53 2019
Response via : Initial Calibration

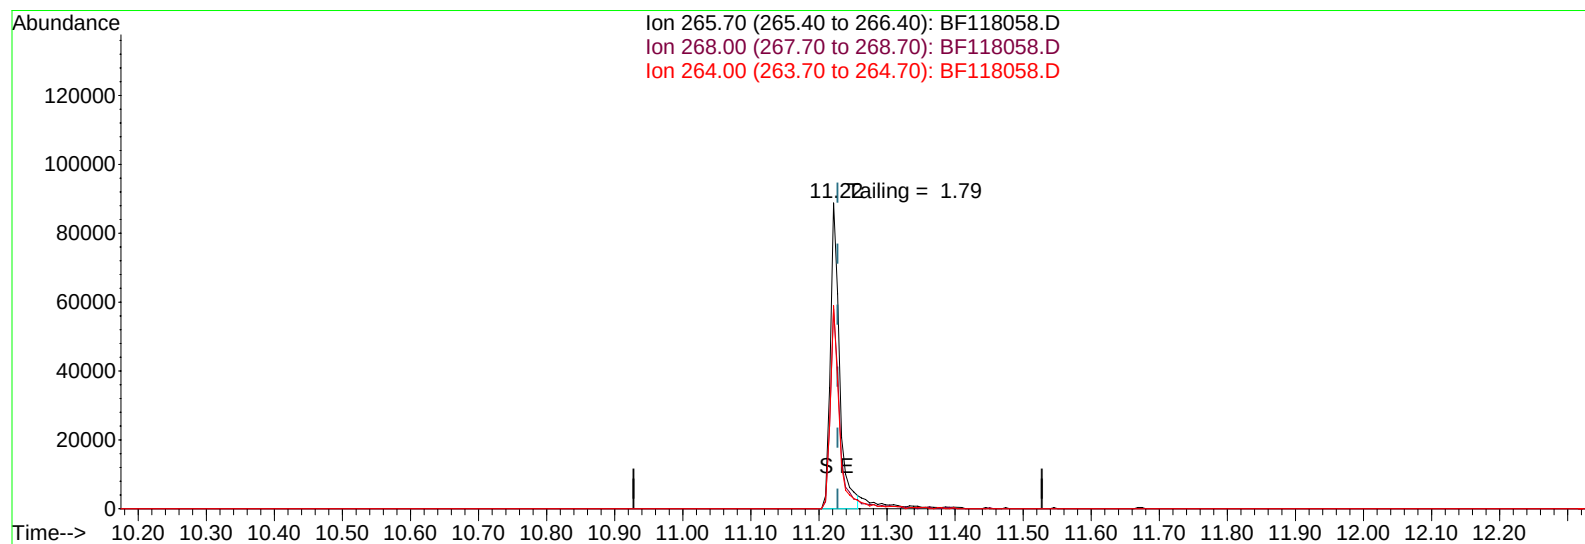

(70) Pentachlorophenol (C)

11.222min (-0.006) 33770.10ng

response 89362




Ion	Exp%	Act%
265.70	100	100
268.00	62.90	65.39
264.00	62.90	66.38
0.00	0.00	0.00

```

Data Path  : Z:\svoasrv\HPCHEM1\BNA F\Data\BF120319\
Data File  : BF118058.D
Acq On     : 3 Dec 2019 12:46
Operator   : JU
Sample     : DFTPP
Misc       :
ALS Vial   : 1      Sample Multiplier: 1

```

Quant Time: Dec 03 16:35:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 03 15:16:53 2019
Response via : Initial Calibration

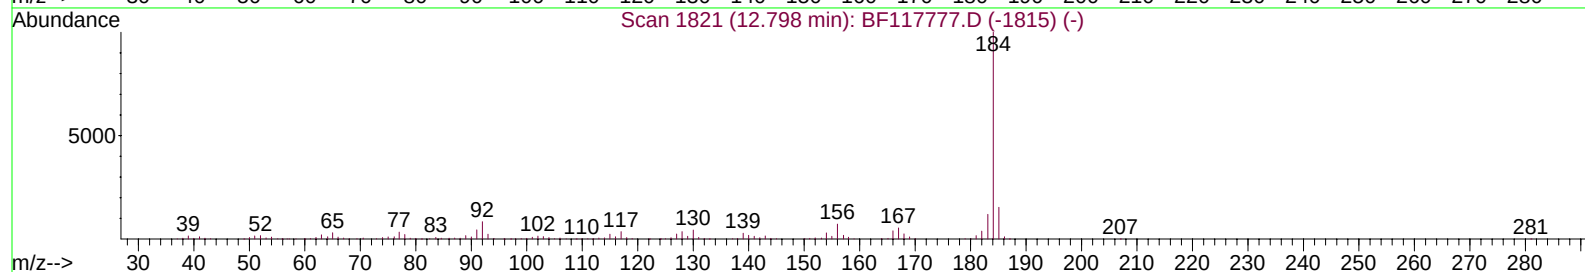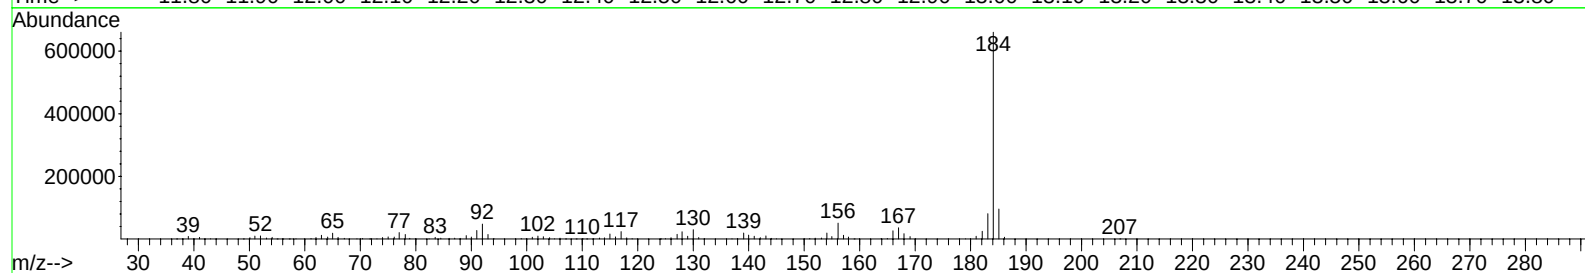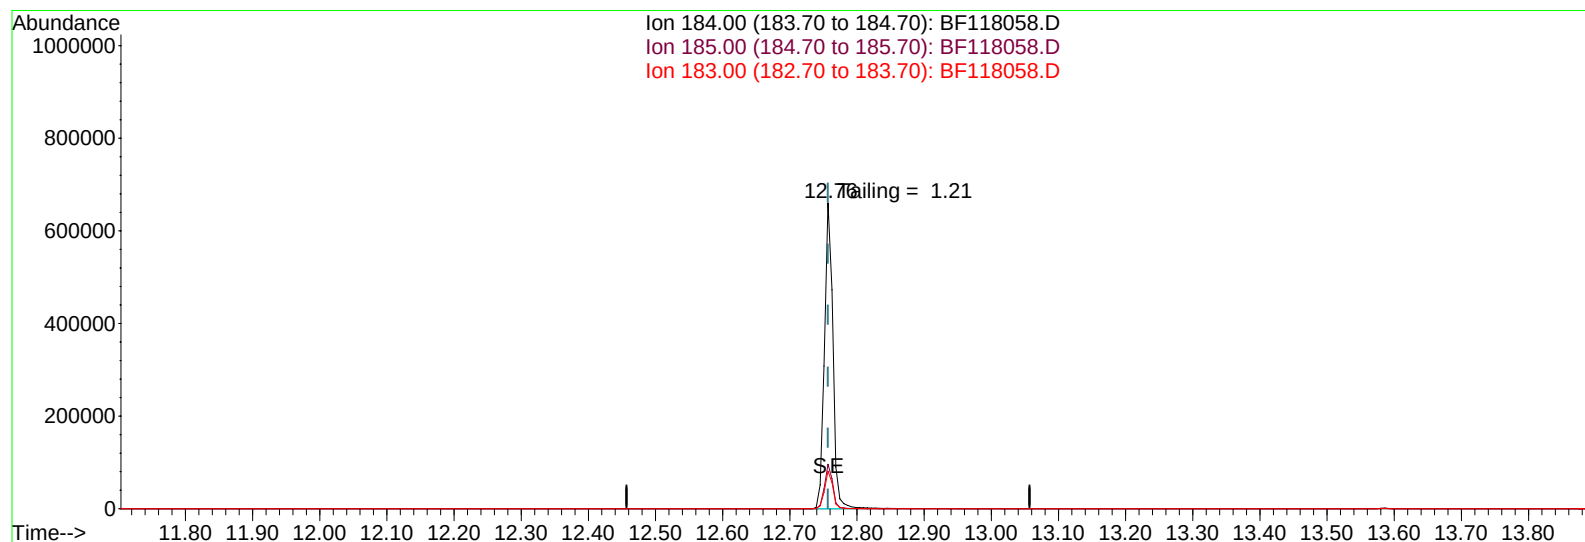

TIC: BF118058.D

(77) Benzidine

12.757min (0.000) 0.00ng

response 581558

Ion	Exp%	Act%
184.00	100	100
185.00	14.50	14.53
183.00	12.10	12.30
0.00	0.00	0.00