


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF120319\
 Data File : BF118058.D
 Acq On : 3 Dec 2019 12:46
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF111319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 03 15:16:53 2019

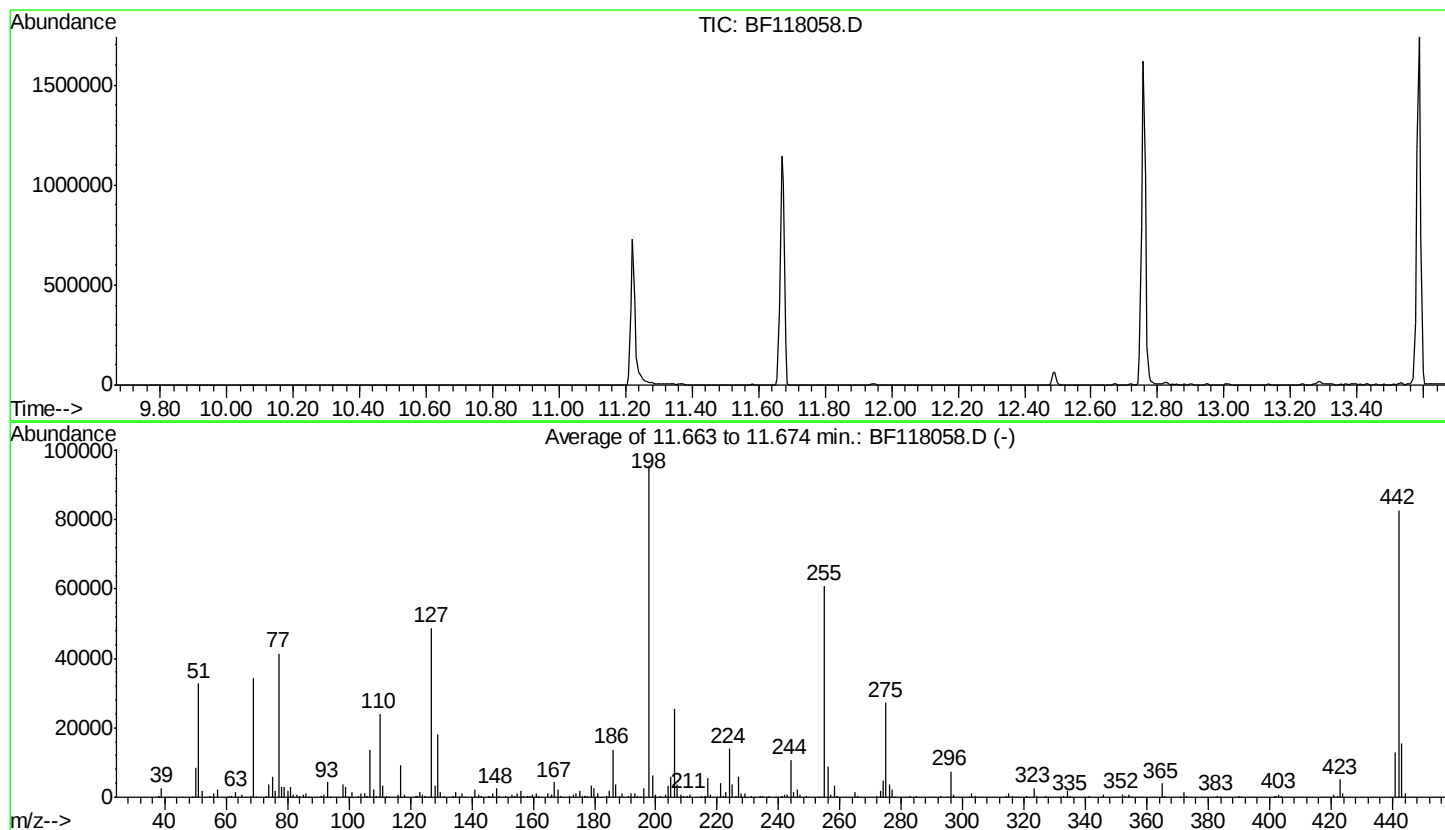

AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1623

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	32701	PASS
68	69	0.00	2	1.2	416	PASS
69	198	0.00	100	36.0	34370	PASS
70	69	0.00	2	0.4	129	PASS
127	198	10	80	51.0	48770	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	95549	PASS
199	198	5	9	6.8	6456	PASS
275	198	10	60	28.5	27215	PASS
365	198	1	100	4.2	4002	PASS
441	198	0.01	100	13.5	12924	PASS
442	198	50	100	86.6	82780	PASS
443	442	15	24	18.9	15634	PASS