
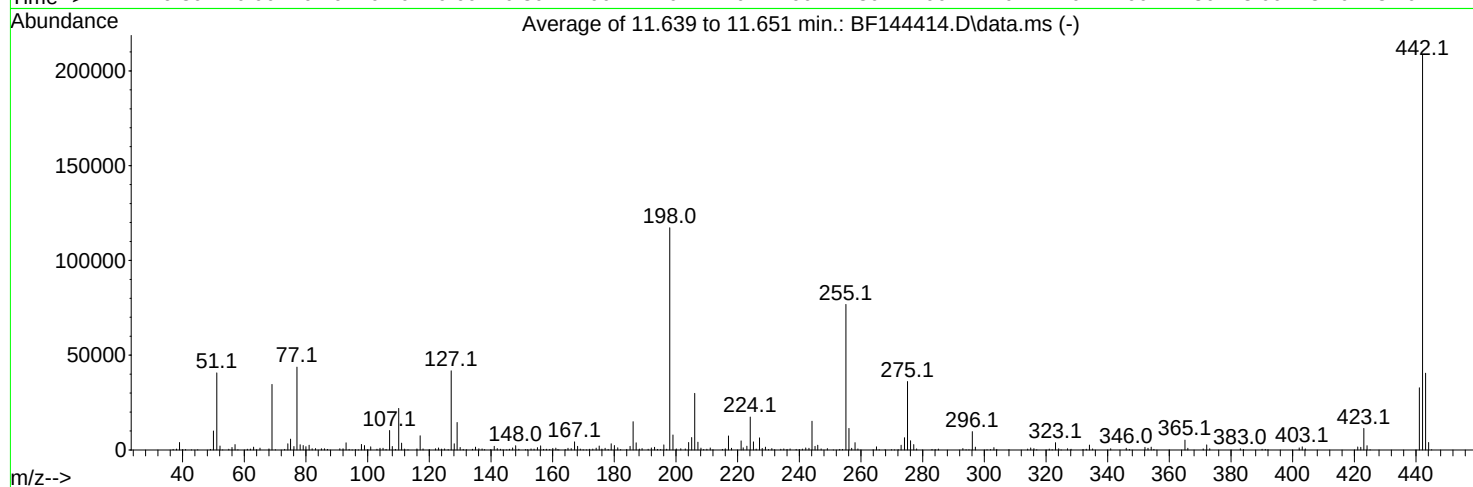


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120325\
Data File : BF144414.D
Acq On : 03 Dec 2025 11:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 05 18:37:33 2025

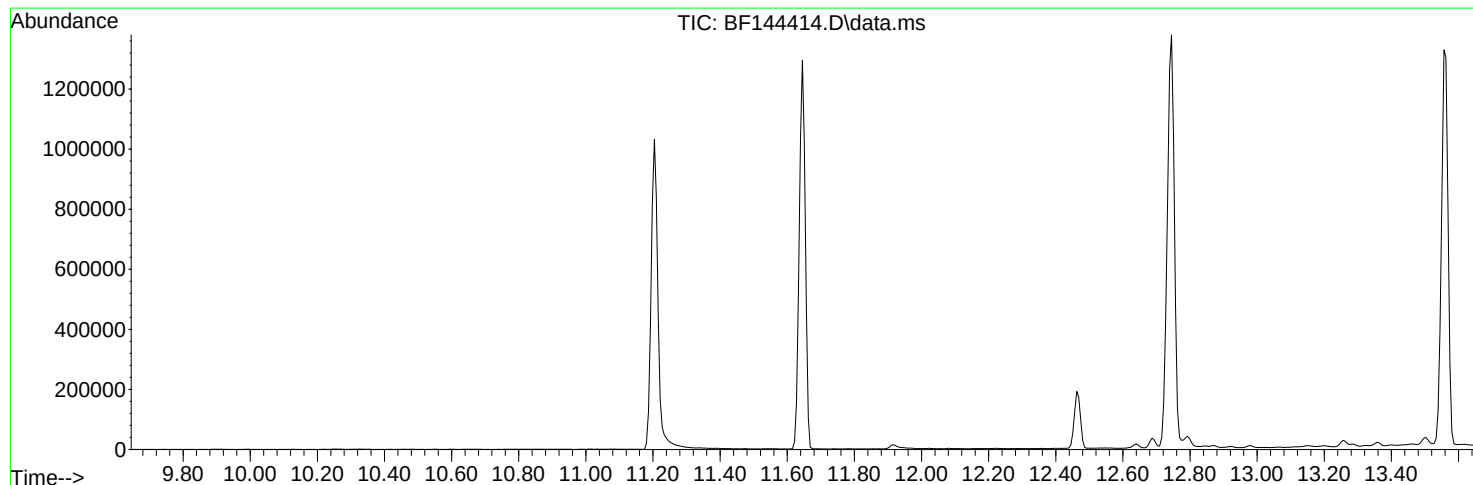




AutoFind: Scans 1606, 1607, 1608; Background Corrected with Scan 1599

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	589	PASS
69	69	100	100	100.0	34621	PASS
70	69	0.00	2	0.4	137	PASS
197	198	0.00	2	0.3	356	PASS
198	198	100	100	100.0	117253	PASS
199	198	5	9	6.8	7917	PASS
365	198	1	100	4.4	5188	PASS
441	443	0.01	150	81.0	32803	PASS
442	442	100	100	100.0	208341	PASS
443	442	15	24	19.4	40475	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120325\
Data File : BF144414.D
Acq On : 03 Dec 2025 11:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 03 12:18:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

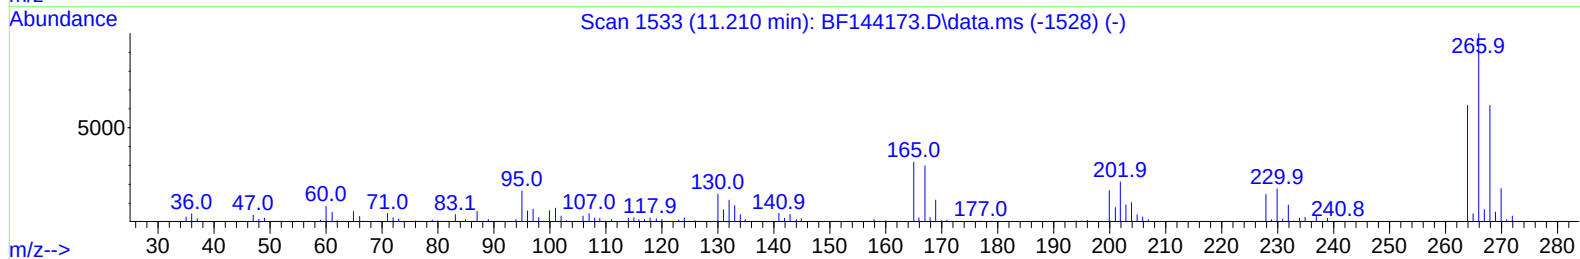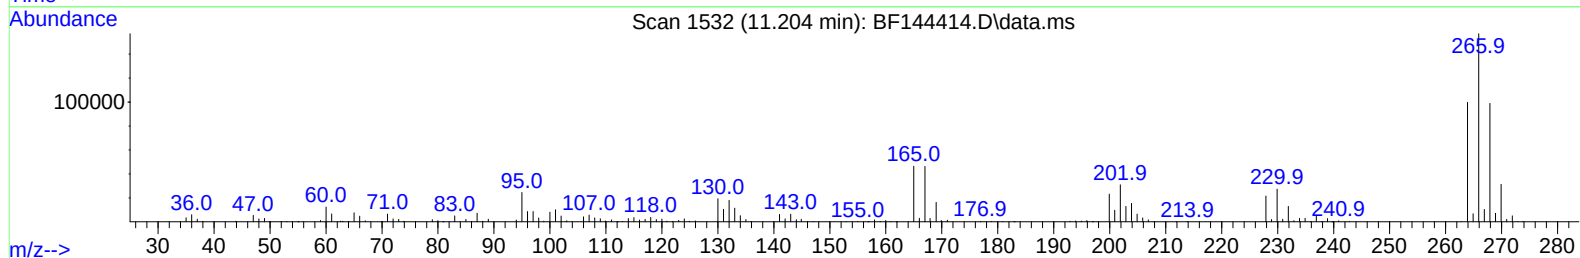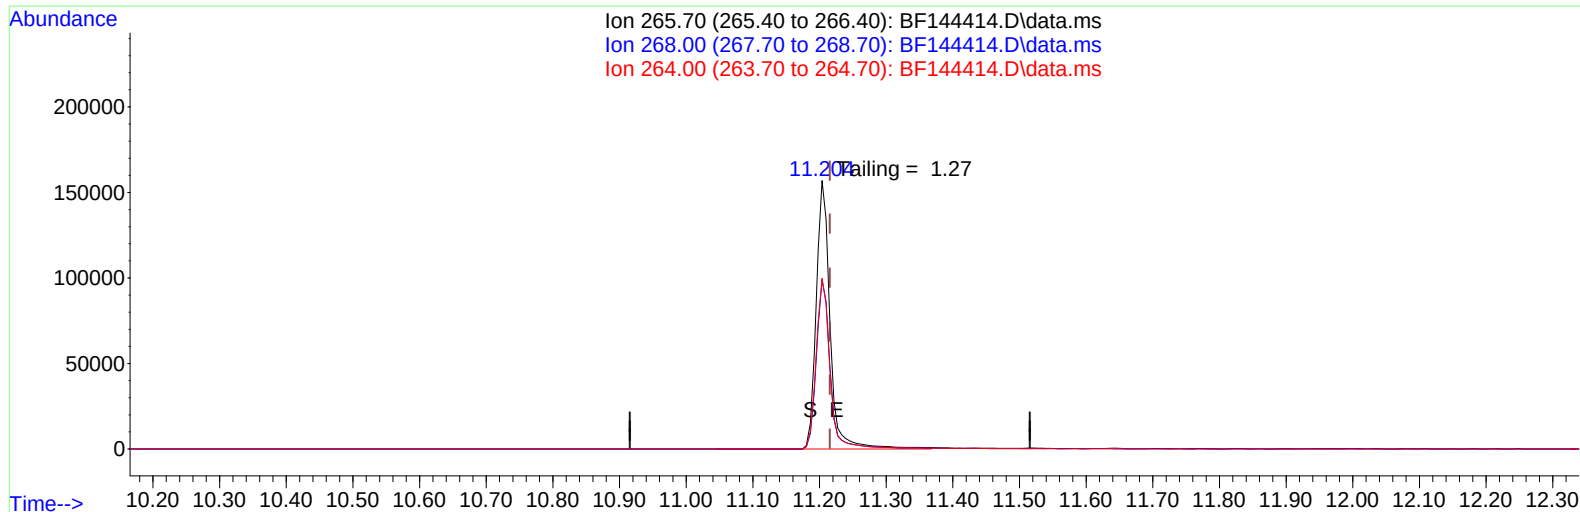

TIC: BF144414.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.012) 45959.22 ng




response 226746

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	63.03
264.00	61.80	63.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120325\
Data File : BF144414.D
Acq On : 03 Dec 2025 11:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 03 12:18:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

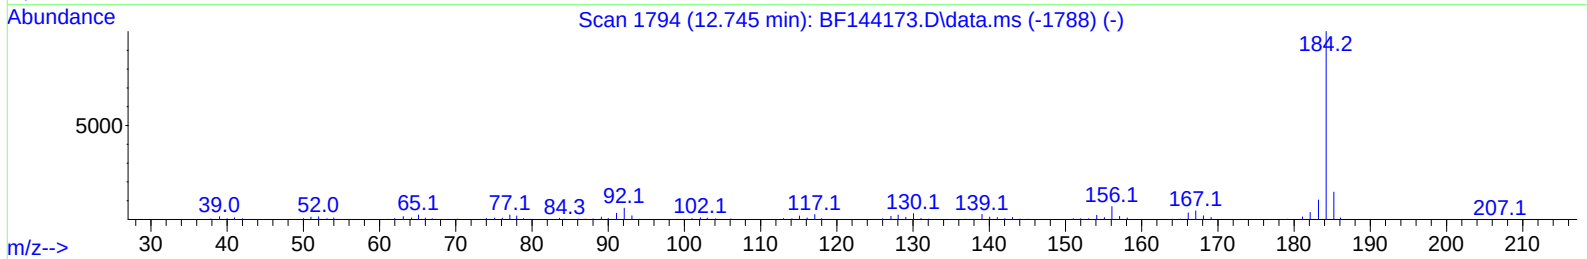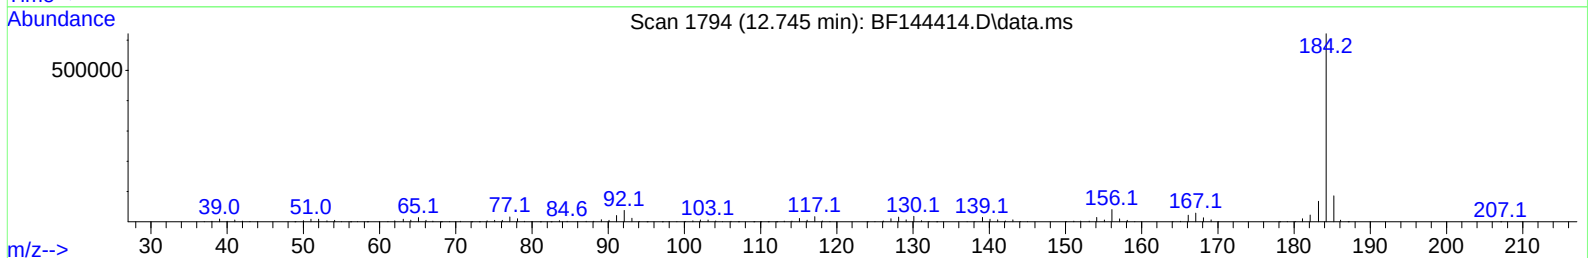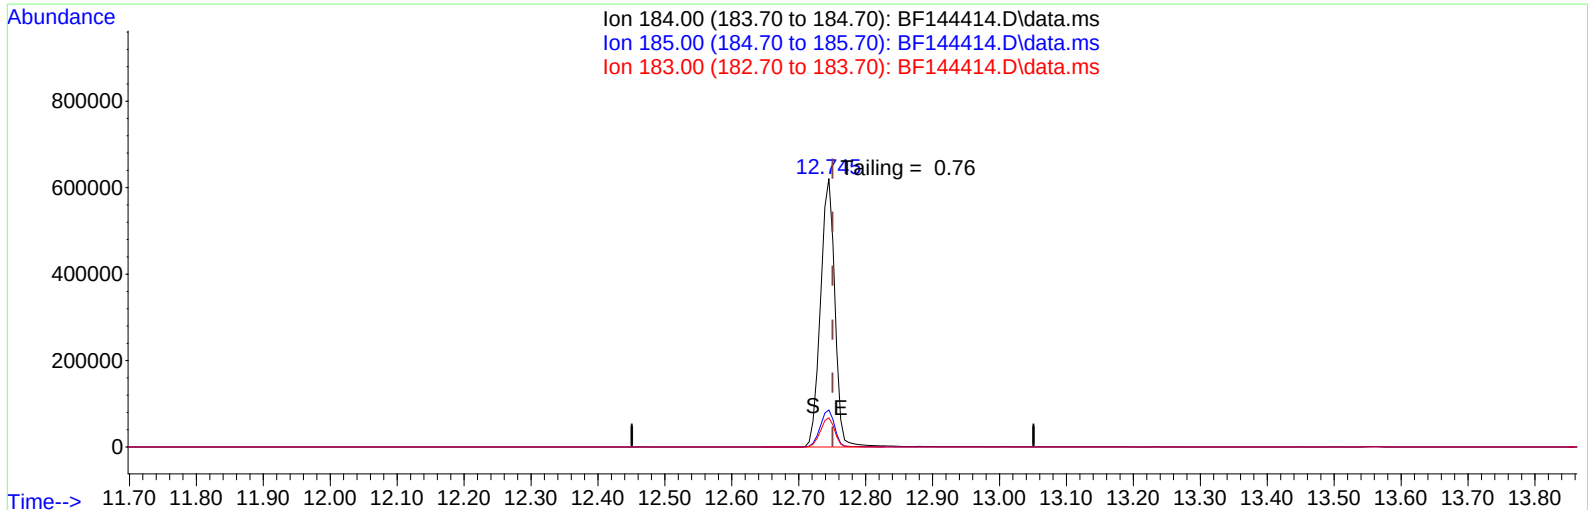

TIC: BF144414.D\data.ms

(77) Benzidine

12.745min (-0.006) 26690.04 ng m

response 925262

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.84
183.00	10.40	10.90
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/3/2025	BNA_F	<u>BF144414.D</u>
Compound Name	Response	Retention Time
DDT	394746	13.563
DDD	9602	13.257
DDE	998	12.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10600	405346	2.62

Instrument :
BNA_F
ClientSampleId :
DFTPP