
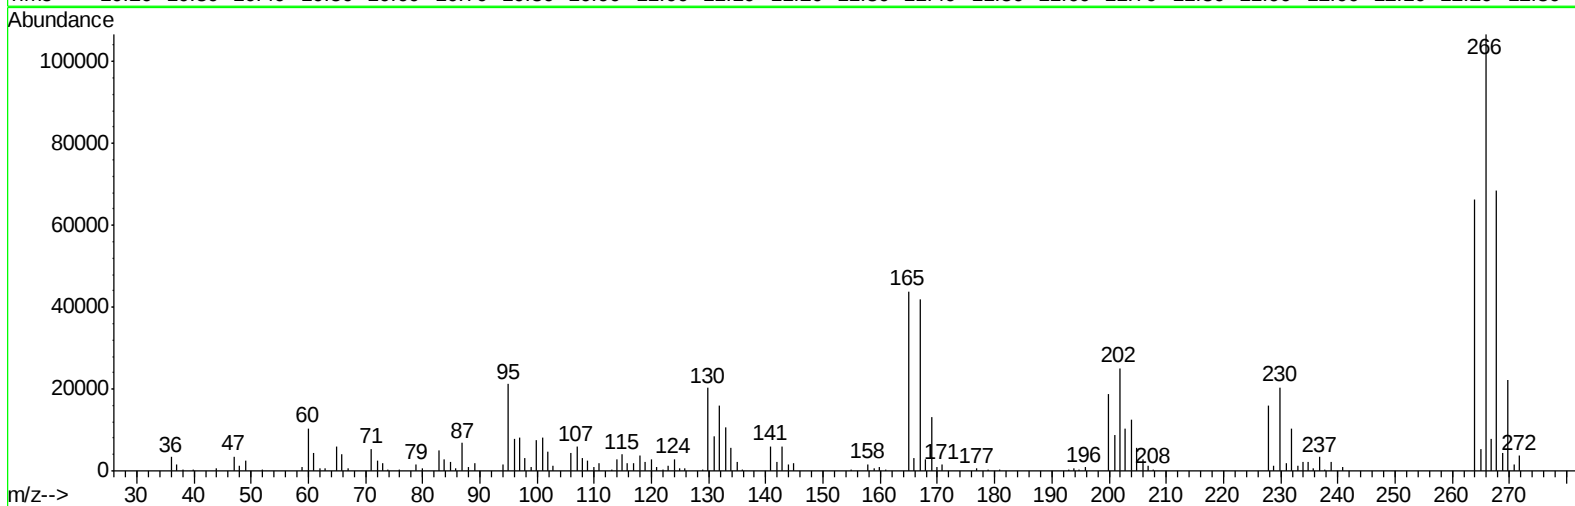


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF120419\
Data File : BF118082.D
Acq On : 4 Dec 2019 12:37
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 05 05:05:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 03 15:16:53 2019
Response via : Initial Calibration

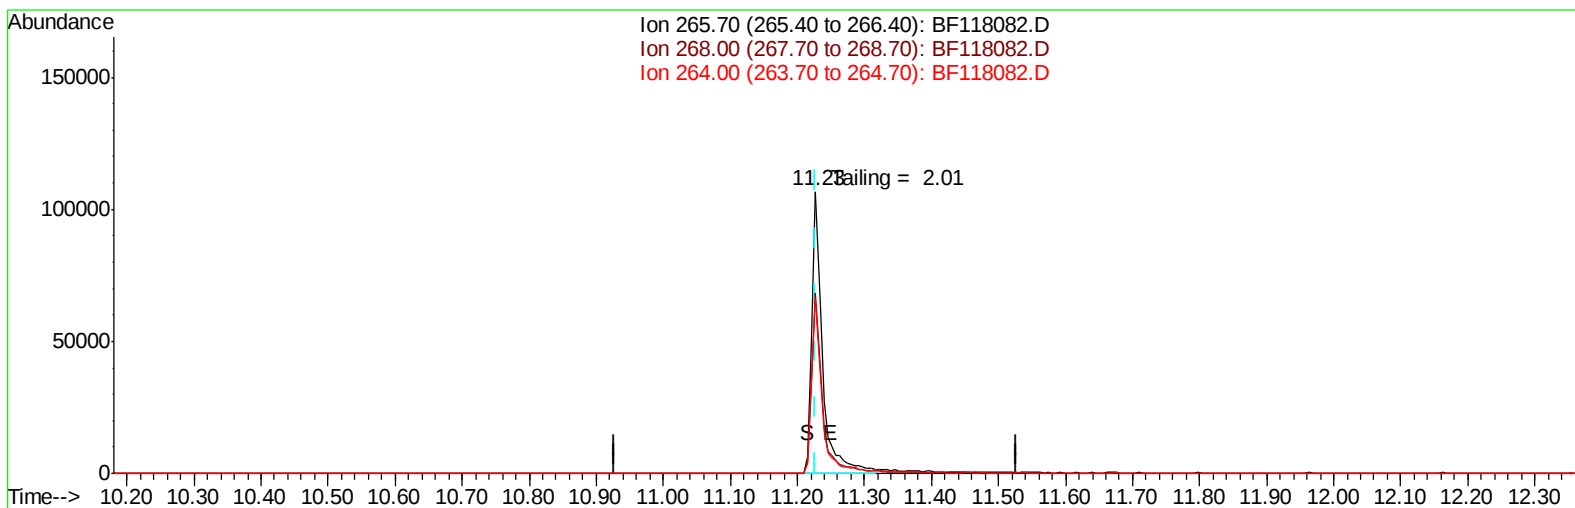

TIC: BF118082.D

(70) Pentachlorophenol (C)



11.227min (-0.000) 33800.98ng

response 115283

Ion	Exp%	Act%
265.70	100	100
268.00	62.90	64.20
264.00	62.90	62.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF120419\
 Data File : BF118082.D
 Acq On : 4 Dec 2019 12:37
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 05 05:05:57 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 03 15:16:53 2019
 Response via : Initial Calibration

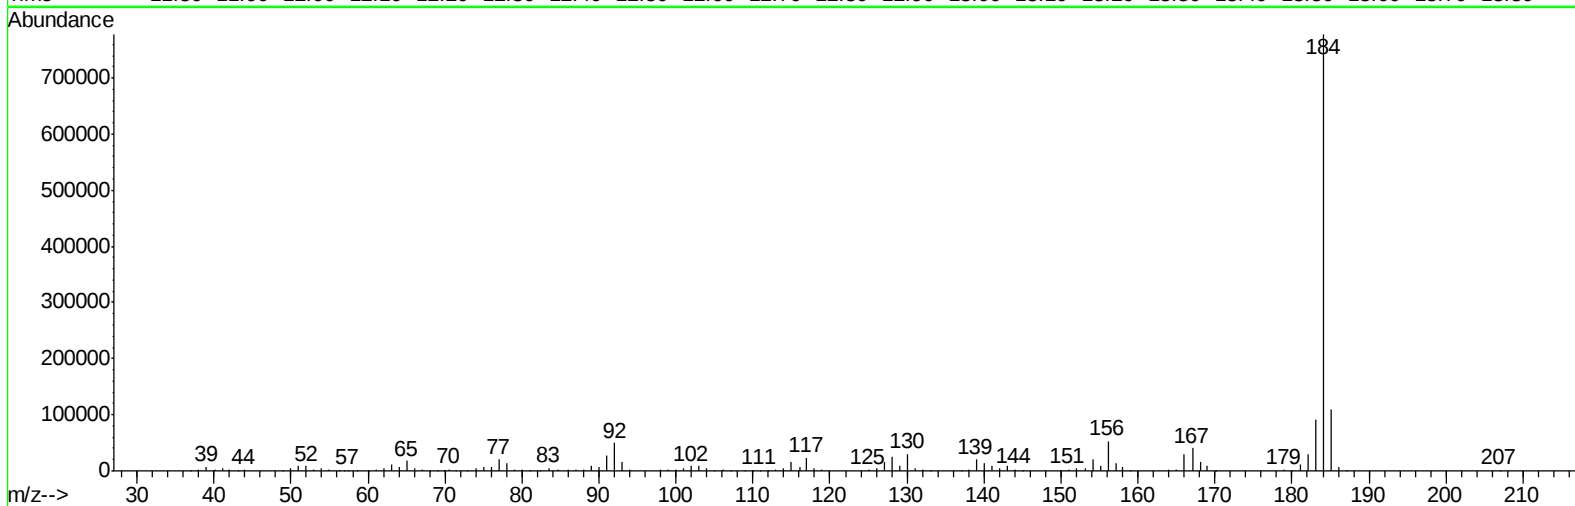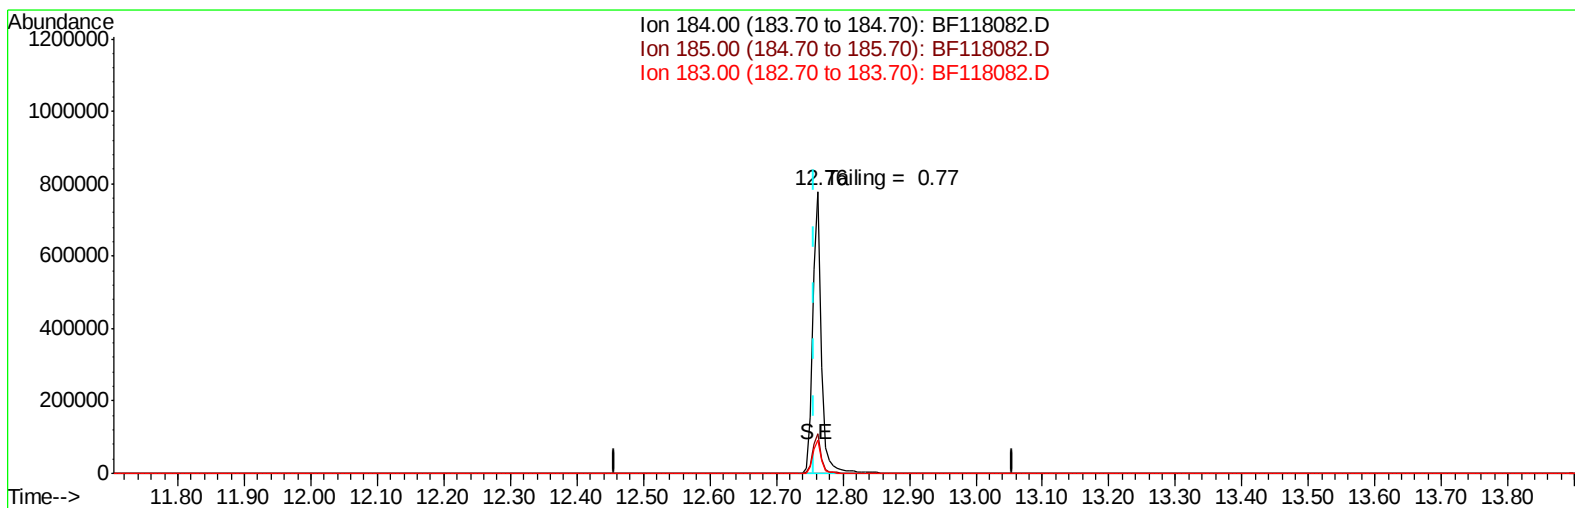

TIC: BF118082.D

(77) Benzidine

12.763min (+0.006) 0.00ng

response 707219

Ion	Exp%	Act%
184.00	100	100
185.00	14.50	14.00
183.00	12.10	11.65
0.00	0.00	0.00