


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF120419\
 Data File : BF118082.D
 Acq On : 4 Dec 2019 12:37
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF111319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 03 15:16:53 2019

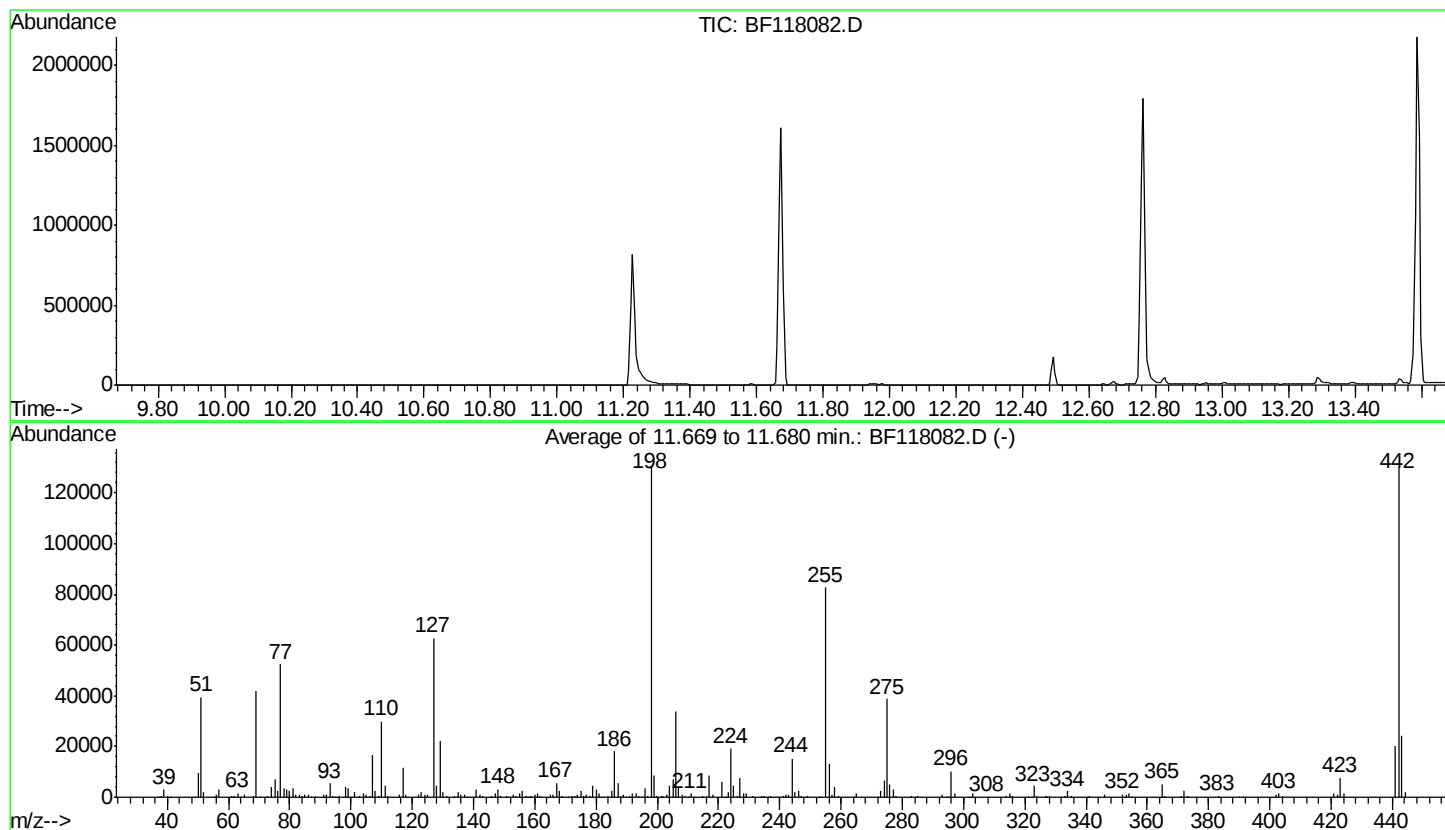

AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.3	39596	PASS
68	69	0.00	2	1.6	689	PASS
69	198	0.00	100	32.2	42134	PASS
70	69	0.00	2	0.5	210	PASS
127	198	10	80	47.9	62613	PASS
197	198	0.00	2	0.3	363	PASS
198	198	100	100	100.0	130749	PASS
199	198	5	9	6.5	8538	PASS
275	198	10	60	29.7	38850	PASS
365	198	1	100	4.1	5307	PASS
441	198	0.01	100	15.5	20317	PASS
442	198	50	100	99.4	129992	PASS
443	442	15	24	18.6	24146	PASS