

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120423\
 Data File : BF136393.D
 Acq On : 04 Dec 2023 21:08
 Operator : CG\JU
 Sample : 05587-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WE-MR-CON

Quant Time: Dec 05 00:37:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 04 13:30:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.804	152	101694	20.000	ng	0.00
21) Naphthalene-d8	8.081	136	384743	20.000	ng	0.00
39) Acenaphthene-d10	9.833	164	176841	20.000	ng	0.00
64) Phenanthrene-d10	11.327	188	286042	20.000	ng	0.00
76) Chrysene-d12	13.980	240	245779	20.000	ng	0.00
86) Perylene-d12	15.462	264	194150	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.434	112	404890	55.416	ng	0.00
7) Phenol-d6	6.434	99	539311	59.034	ng	-0.01
23) Nitrobenzene-d5	7.363	82	340276	46.736	ng	0.00
42) 2,4,6-Tribromophenol	10.627	330	102393	47.360	ng	0.00
45) 2-Fluorobiphenyl	9.157	172	721319	52.100	ng	0.00
79) Terphenyl-d14	12.921	244	750027	35.200	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120423\
Data File : BF136393.D
Acq On : 04 Dec 2023 21:08
Operator : CG\JU
Sample : 05587-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WE-MR-CON

Quant Time: Dec 05 00:37:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 04 13:30:53 2023
Response via : Initial Calibration




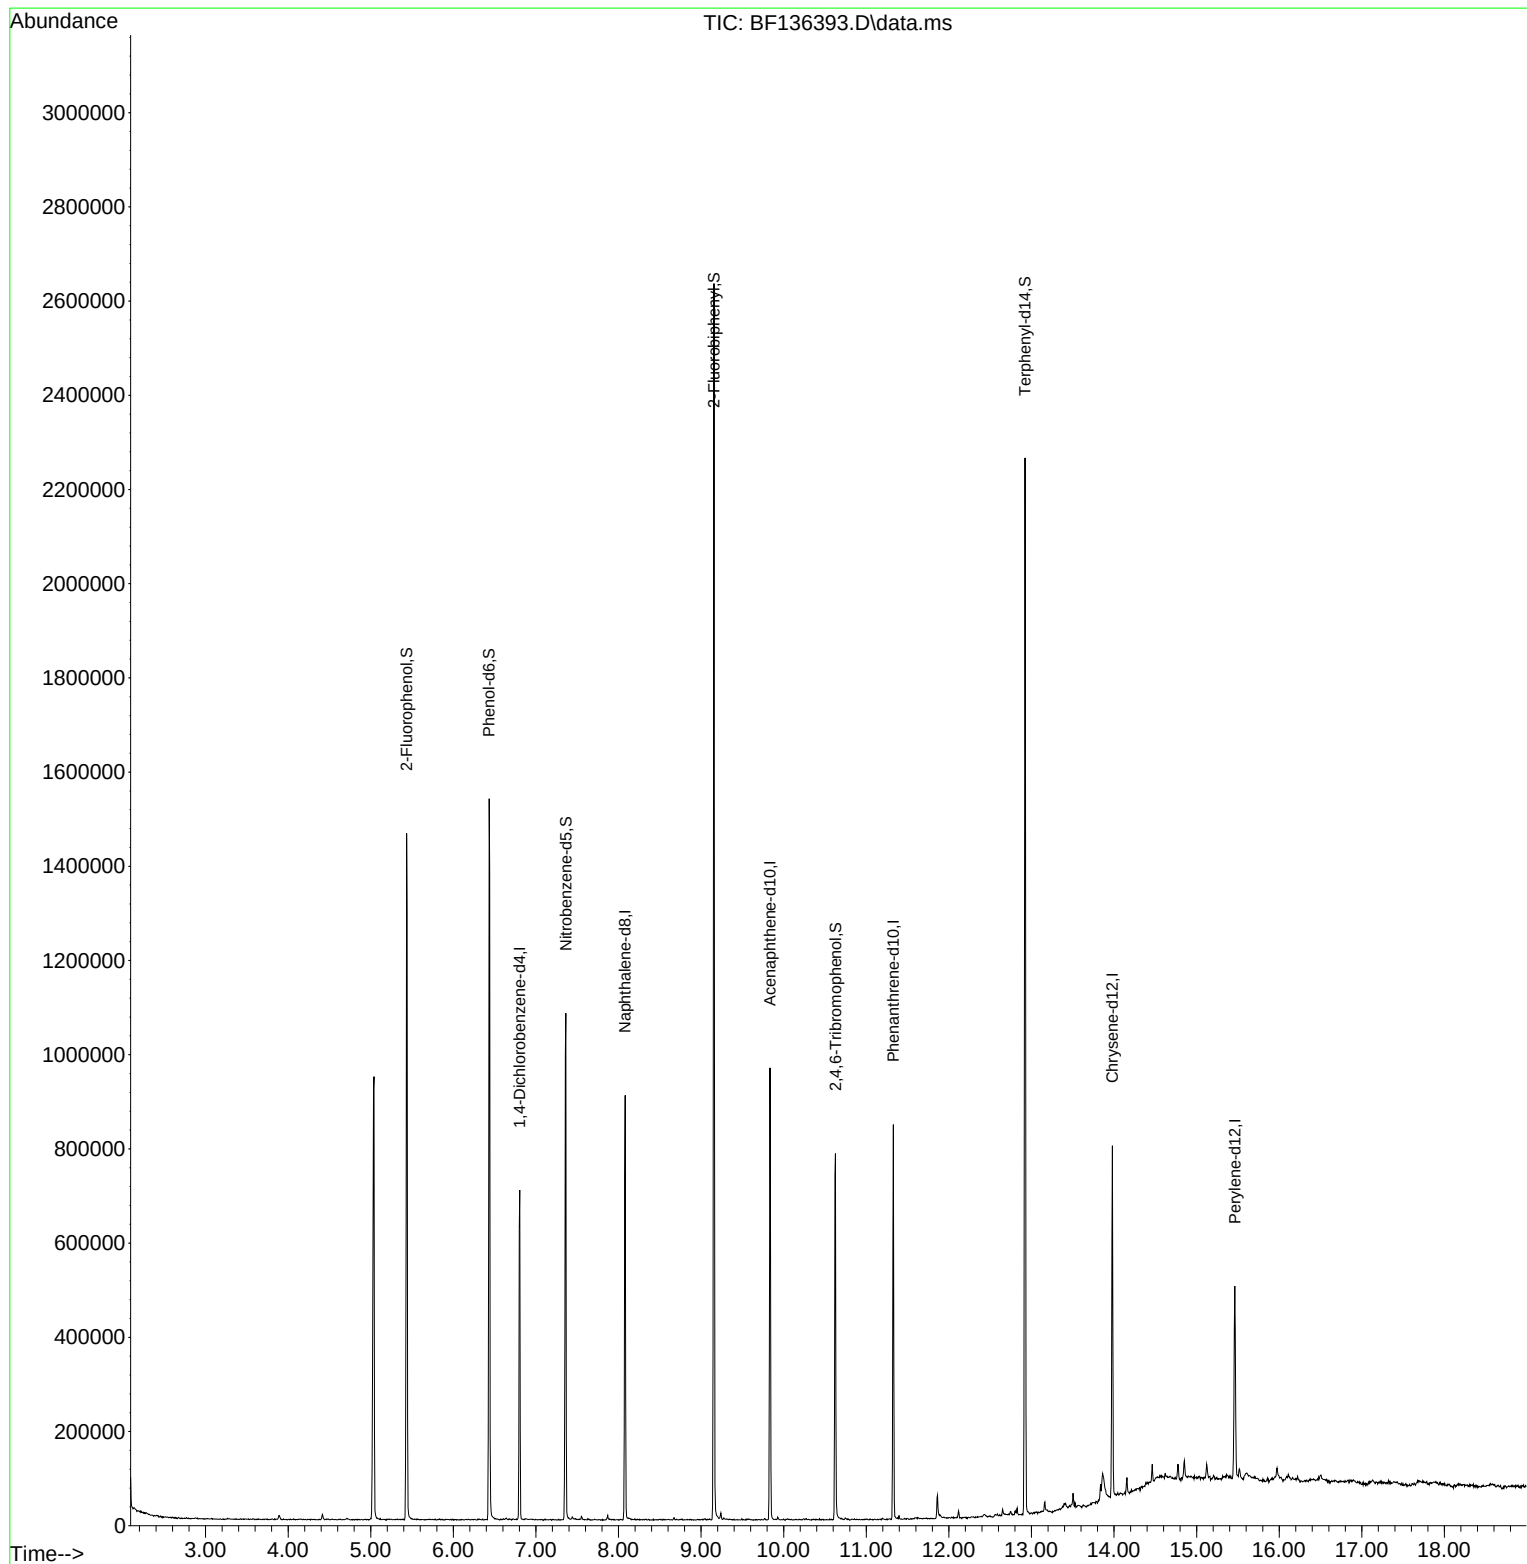


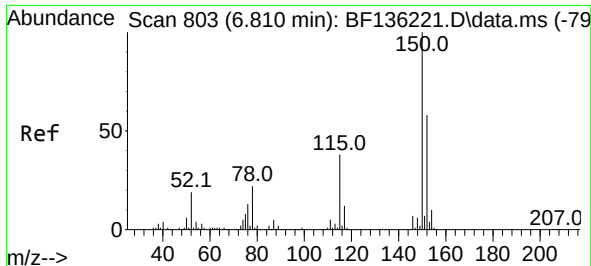

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.804 min Scan# 803
Delta R.T. 0.000 min
Lab File: BF136393.D
Acq: 04 Dec 2023 21:08




Instrument :
BNA_F
ClientSampleId :
WE-MR-CON


Tgt Ion:152 Resp: 101694
Ion Ratio Lower Upper
152 100
150 157.4 137.8 206.8
115 59.9 52.7 79.1

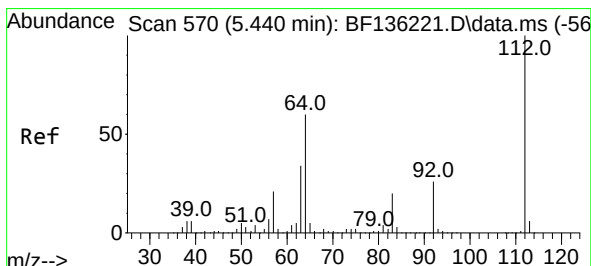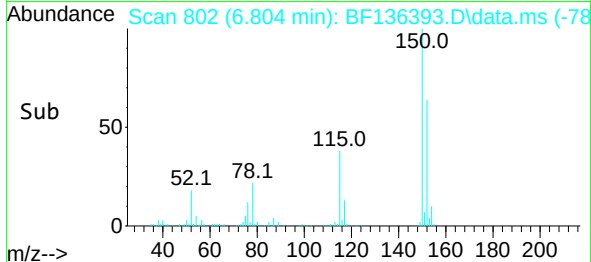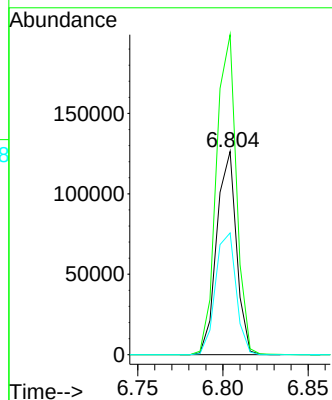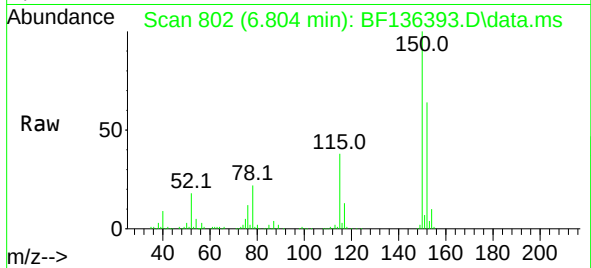

#5
2-Fluorophenol
Concen: 55.416 ng
RT: 5.434 min Scan# 569
Delta R.T. -0.006 min
Lab File: BF136393.D
Acq: 04 Dec 2023 21:08

Tgt Ion:112 Resp: 404890
Ion Ratio Lower Upper
112 100
64 58.4 48.2 72.4
63 30.6 27.0 40.6


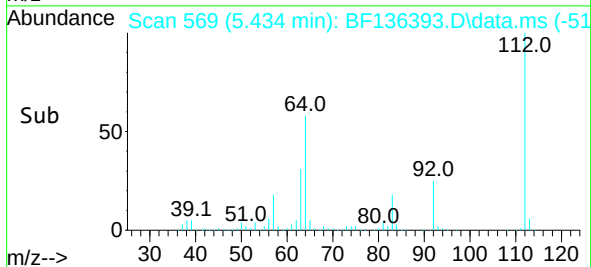
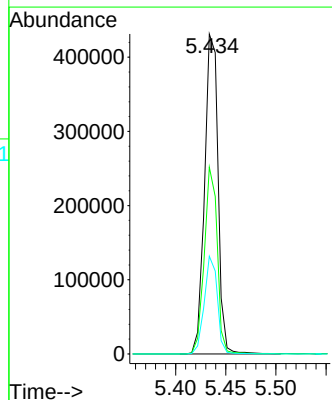
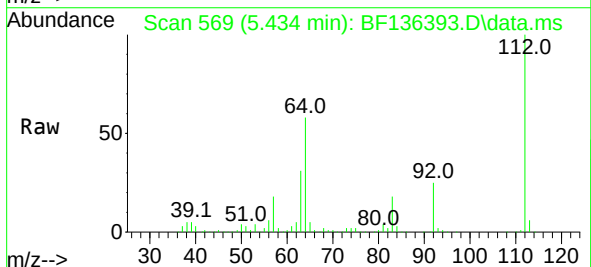


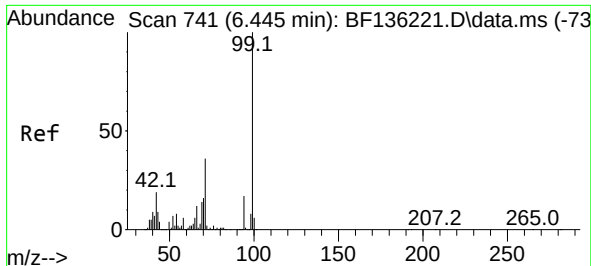

#7
Phenol-d6
Concen: 59.034 ng
RT: 6.434 min Scan# 71
Delta R.T. -0.012 min
Lab File: BF136393.D
Acq: 04 Dec 2023 21:08




Instrument :
BNA_F
ClientSampleId :
WE-MR-CON


Tgt Ion: 99 Resp: 539311
Ion Ratio Lower Upper
99 100
42 16.6 15.0 22.6
71 33.7 28.9 43.3

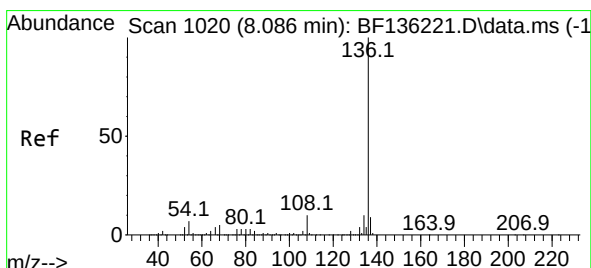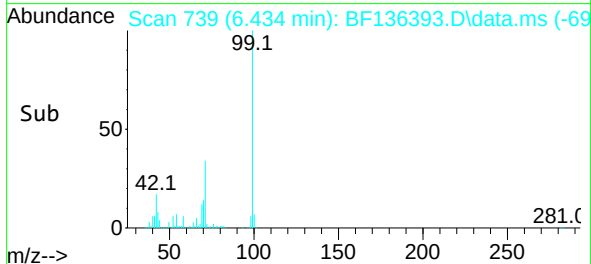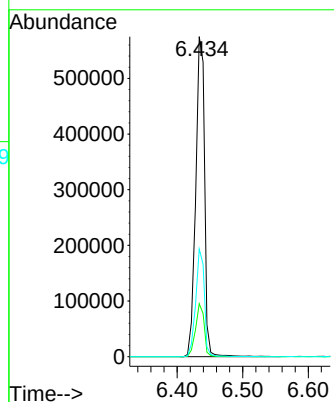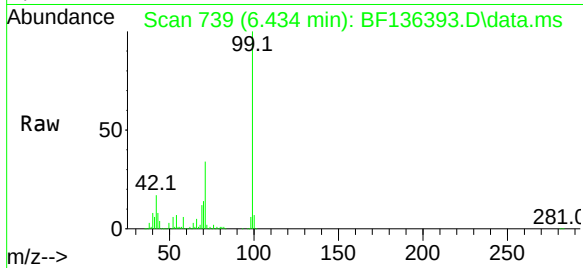

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.081 min Scan# 1019
Delta R.T. 0.000 min
Lab File: BF136393.D
Acq: 04 Dec 2023 21:08

Tgt Ion: 136 Resp: 384743
Ion Ratio Lower Upper
136 100
137 10.2 7.4 11.2
54 6.7 5.5 8.3
68 4.7 3.7 5.5

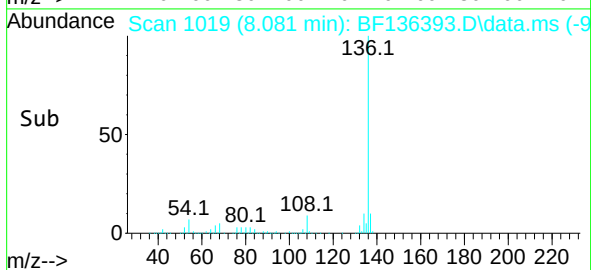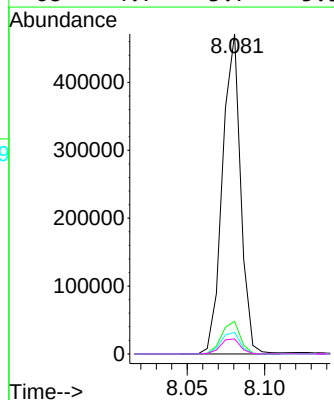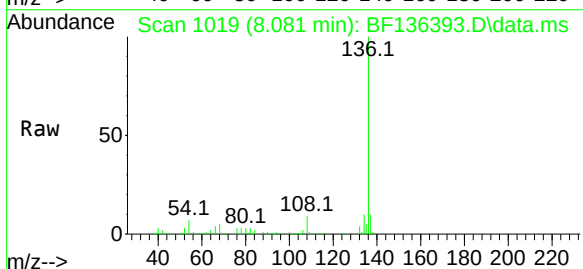

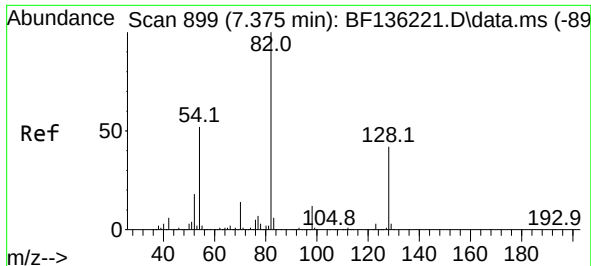

#23

Nitrobenzene-d5

Concen: 46.736 ng

RT: 7.363 min Scan# 89

Delta R.T. -0.006 min

Lab File: BF136393.D

Acq: 04 Dec 2023 21:08

Instrument :

BNA_F

ClientSampleId :

WE-MR-CON





Tgt Ion: 82 Resp: 340276

Ion Ratio Lower Upper

82 100

128 47.4 33.4 50.2

54 47.9 41.7 62.5

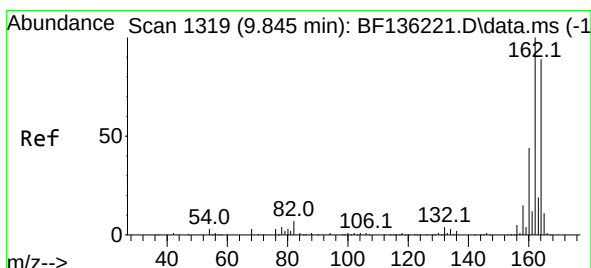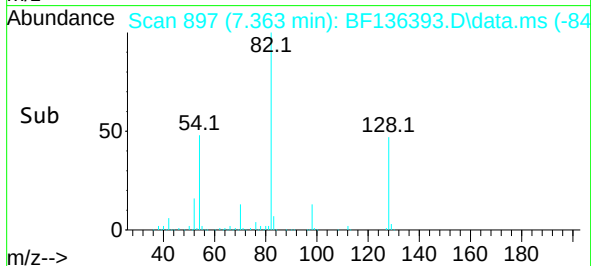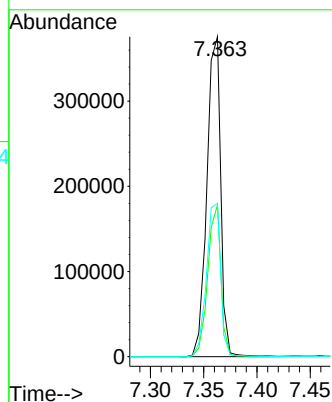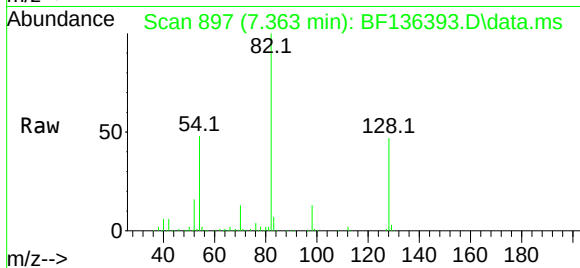

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.833 min Scan# 1317

Delta R.T. -0.006 min

Lab File: BF136393.D

Acq: 04 Dec 2023 21:08




Tgt Ion: 164 Resp: 176841


Ion Ratio Lower Upper

164 100

162 104.9 89.5 134.3

160 49.4 39.6 59.4

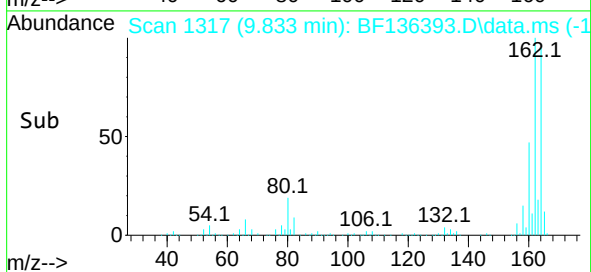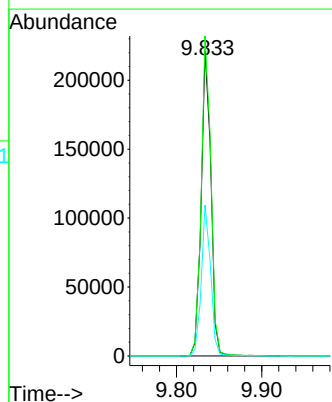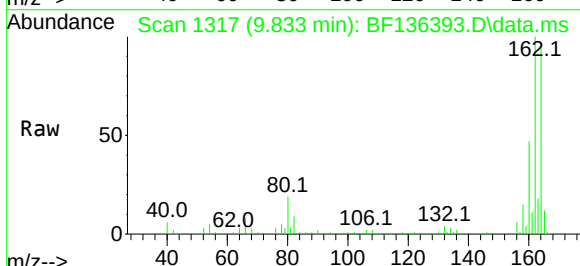

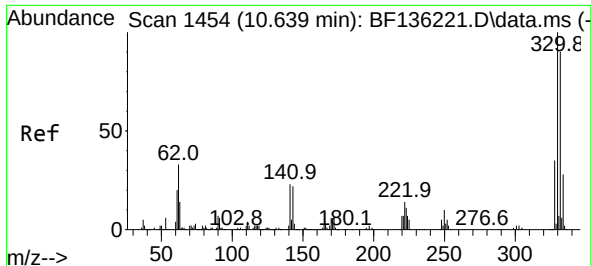

#42

2,4,6-Tribromophenol

Concen: 47.360 ng

RT: 10.627 min Scan# 1454

Delta R.T. -0.006 min

Lab File: BF136393.D

Acq: 04 Dec 2023 21:08

Instrument :

BNA_F

ClientSampleId :

WE-MR-CON





Tgt Ion:330 Resp: 102393

Ion Ratio Lower Upper

330 100

332 95.8 73.0 109.6

141 29.3 24.2 36.2

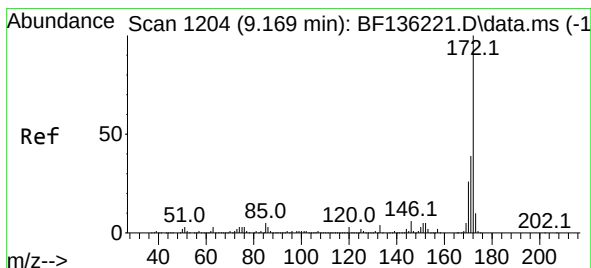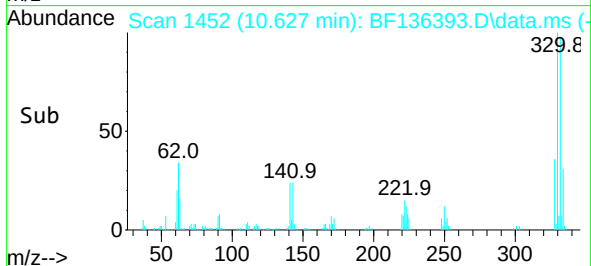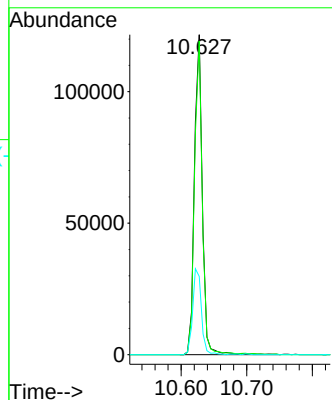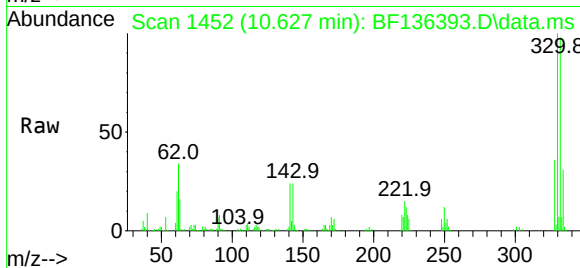

#45

2-Fluorobiphenyl

Concen: 52.100 ng

RT: 9.157 min Scan# 1202

Delta R.T. -0.006 min

Lab File: BF136393.D

Acq: 04 Dec 2023 21:08




Tgt Ion:172 Resp: 721319


Ion Ratio Lower Upper

172 100

171 37.5 31.5 47.3

170 24.5 20.8 31.2

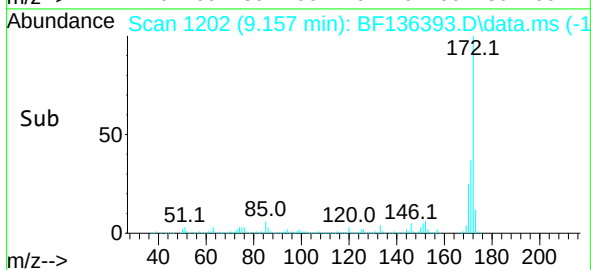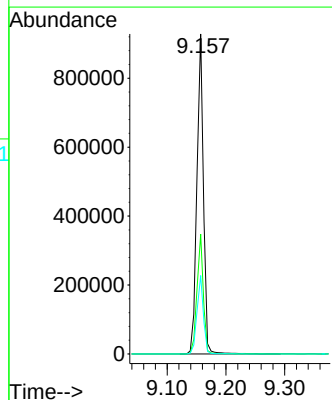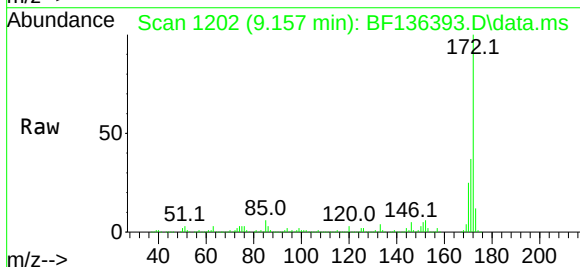

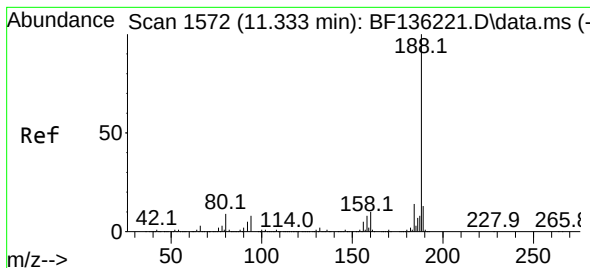

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.327 min Scan# 1

Delta R.T. 0.000 min

Lab File: BF136393.D

Acq: 04 Dec 2023 21:08

Instrument :

BNA_F

ClientSampleId :

WE-MR-CON





Tgt Ion:188 Resp: 286042

Ion Ratio Lower Upper

188 100

94 8.6 6.7 10.1

80 8.6 7.2 10.8

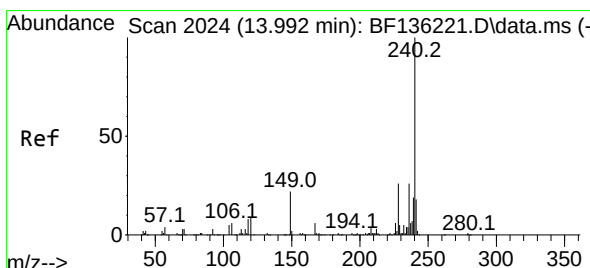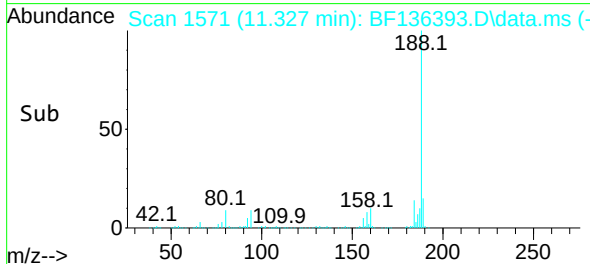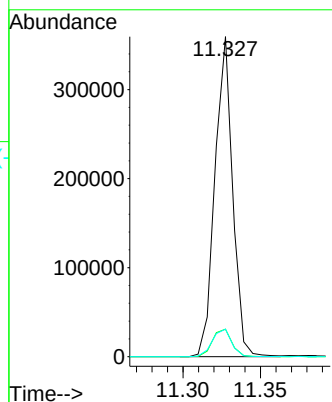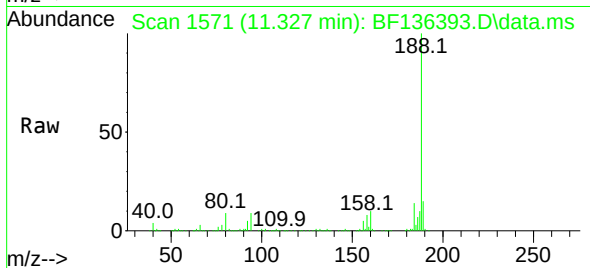

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.980 min Scan# 2022

Delta R.T. 0.000 min

Lab File: BF136393.D

Acq: 04 Dec 2023 21:08




Tgt Ion:240 Resp: 245779


Ion Ratio Lower Upper

240 100

120 10.0 7.4 11.2


236 25.2 21.1 31.7

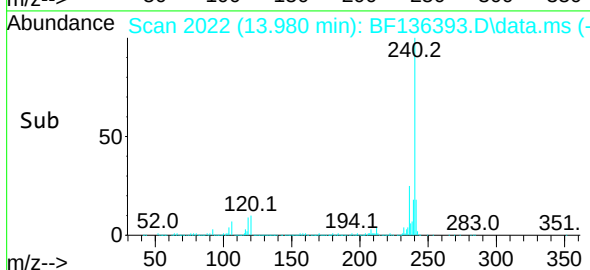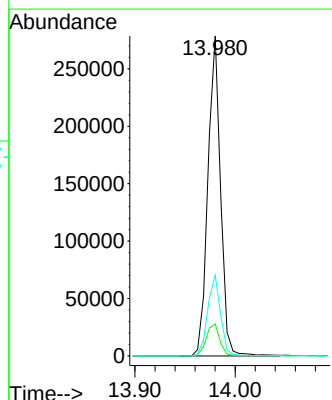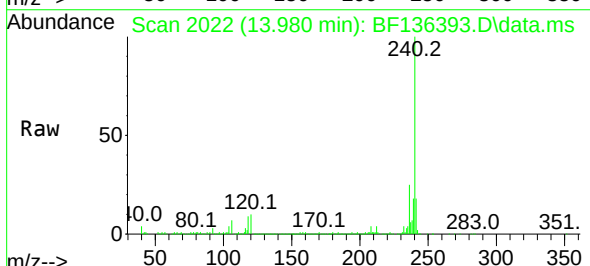



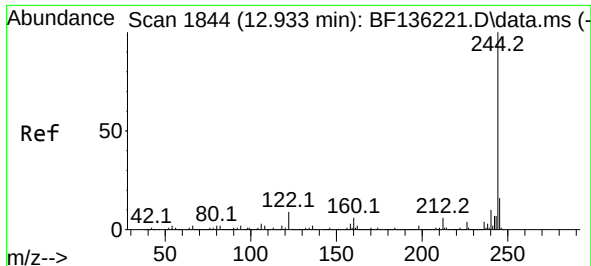


#79
 Terphenyl-d14
 Concen: 35.200 ng
 RT: 12.921 min Scan# 1842
 Delta R.T. -0.006 min
 Lab File: BF136393.D
 Acq: 04 Dec 2023 21:08

Instrument :
 BNA_F
 ClientSampleId :
 WE-MR-CON

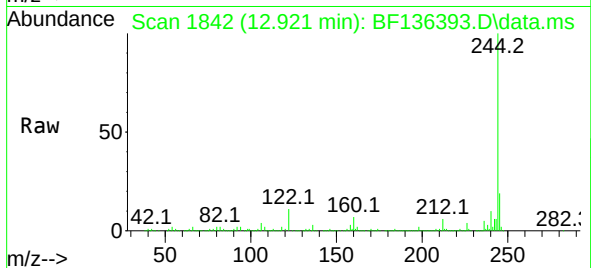

Tgt Ion:244 Resp: 750027
 Ion Ratio Lower Upper
 244 100
 212 6.1 4.6 7.0
 122 10.6 7.3 10.9

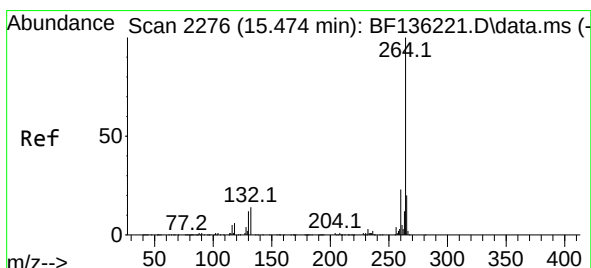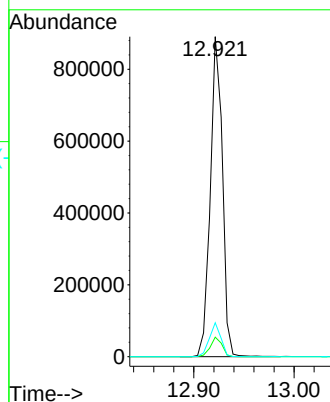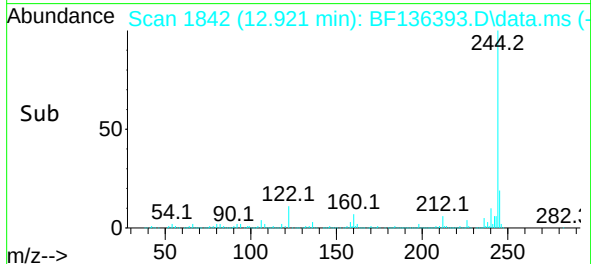

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.462 min Scan# 2274
 Delta R.T. 0.006 min
 Lab File: BF136393.D
 Acq: 04 Dec 2023 21:08

Tgt Ion:264 Resp: 194150
 Ion Ratio Lower Upper
 264 100
 260 23.5 18.6 27.8
 265 21.1 15.7 23.5

