
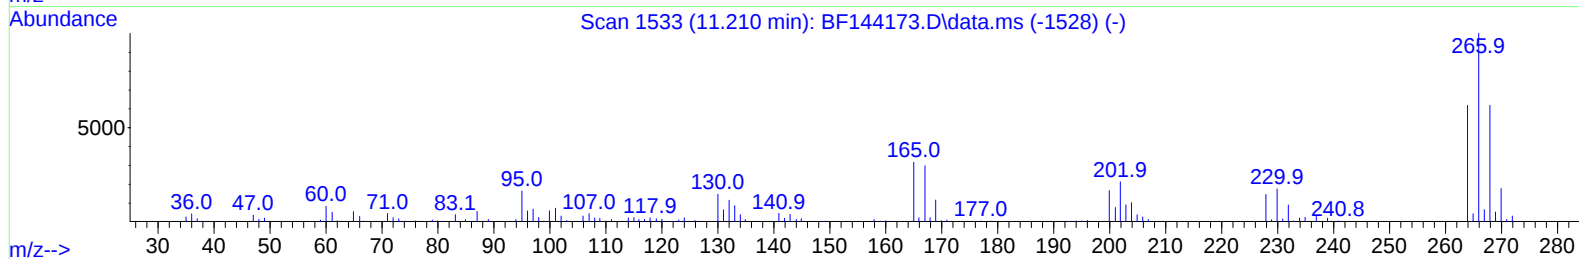
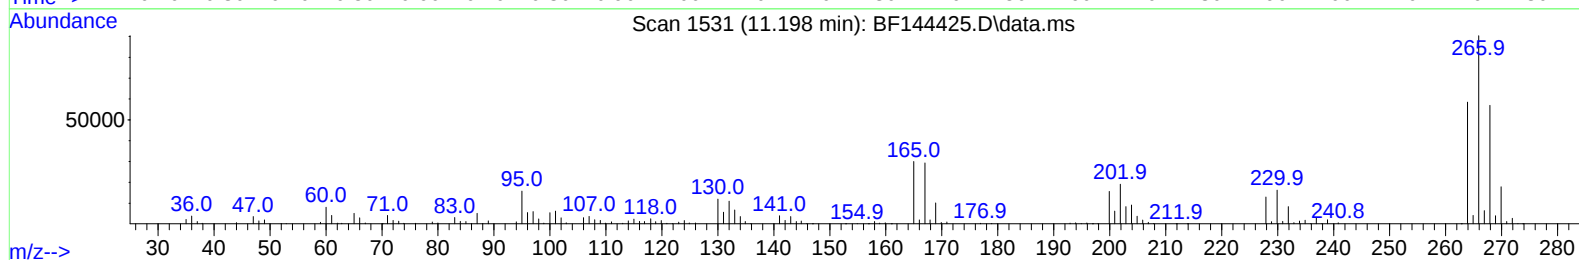


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120425\
Data File : BF144425.D
Acq On : 04 Dec 2025 12:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 04 12:52:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

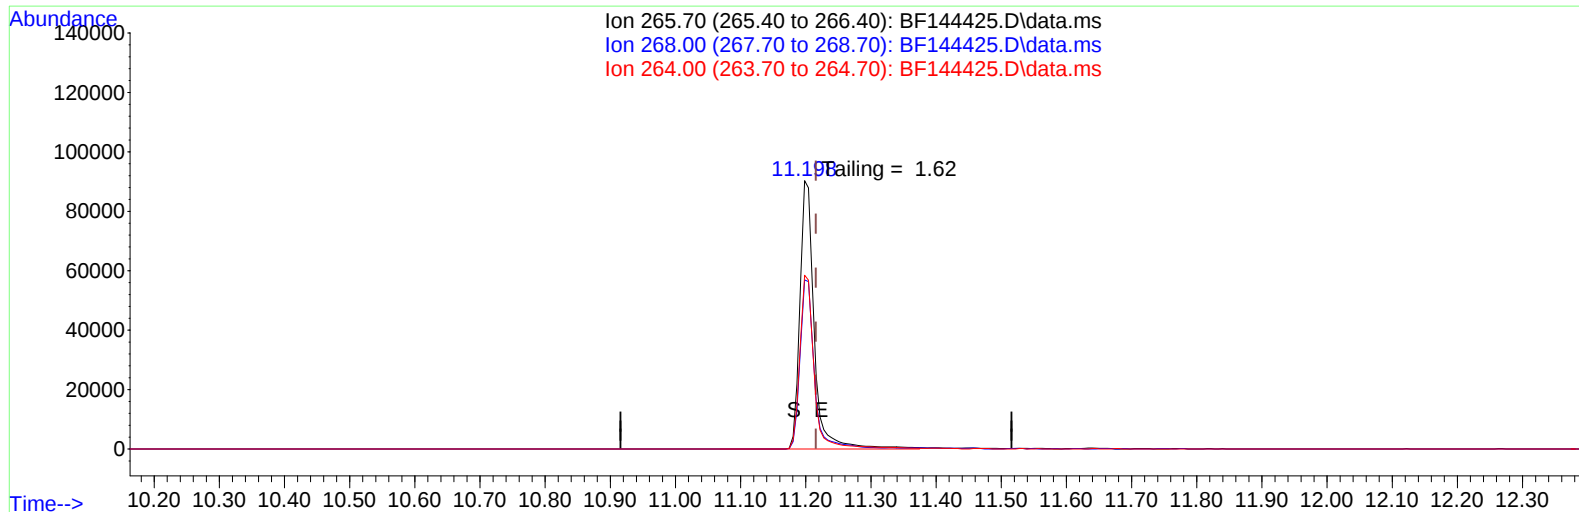

TIC: BF144425.D\data.ms

(70) Pentachlorophenol (C)




11.198min (-0.018) 54055.10 ng

response 139212

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	63.01
264.00	61.80	64.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120425\
Data File : BF144425.D
Acq On : 04 Dec 2025 12:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 04 12:52:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

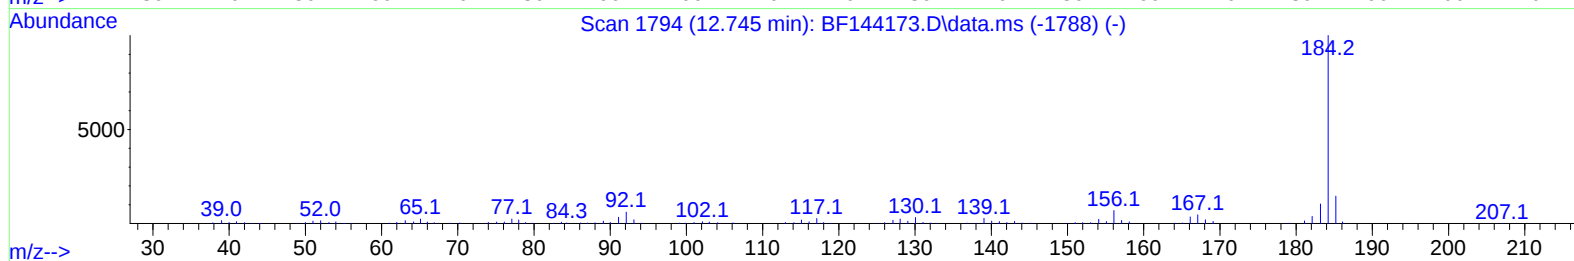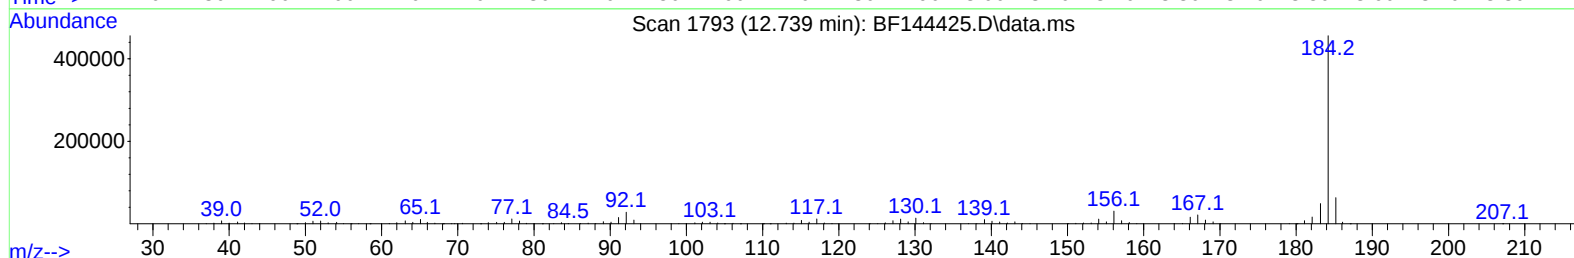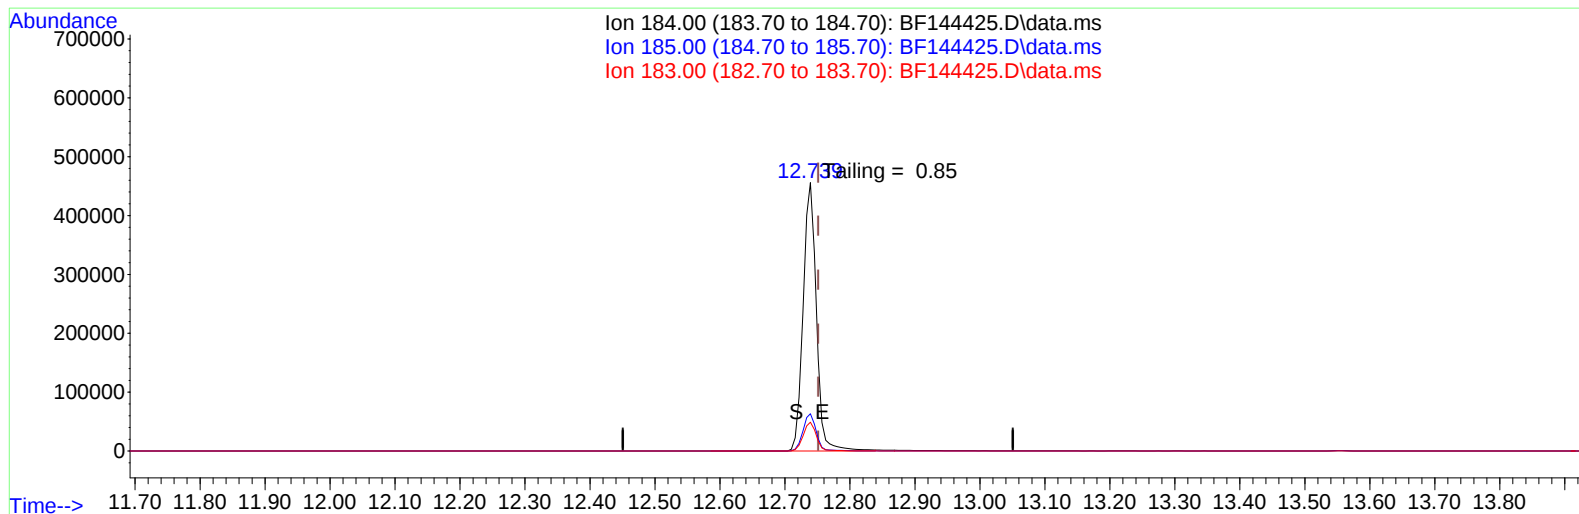

TIC: BF144425.D\data.ms

(77) Benzidine

12.739min (-0.012) 22803.06 ng

response 650891

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.91
183.00	10.40	10.76
0.00	0.00	0.00