


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120425\
Data File : BF144425.D
Acq On : 04 Dec 2025 12:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 05 18:37:33 2025

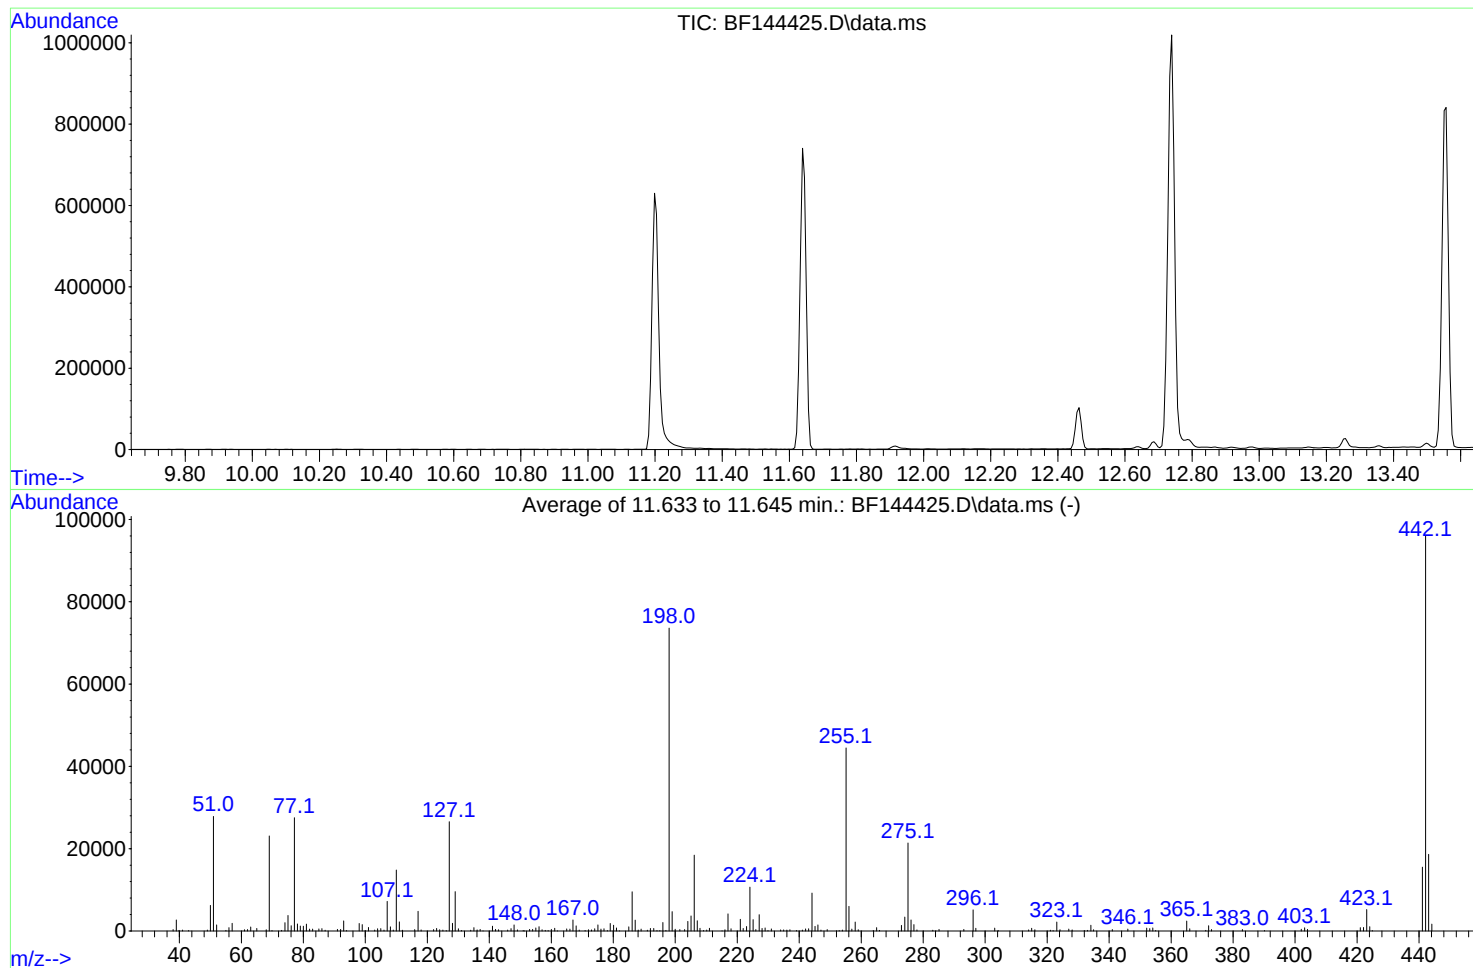

AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.4	318	PASS
69	69	100	100	100.0	23099	PASS
70	69	0.00	2	0.6	129	PASS
197	198	0.00	2	0.2	150	PASS
198	198	100	100	100.0	73608	PASS
199	198	5	9	6.4	4722	PASS
365	198	1	100	3.3	2421	PASS
441	443	0.01	150	83.2	15506	PASS
442	442	100	100	100.0	95944	PASS
443	442	15	24	19.4	18638	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/4/2025	BNA_F	<u>BF144425.D</u>
Compound Name	Response	Retention Time
DDT	244998	13.557
DDD	9866	13.257
DDE	989	12.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10855	255853	4.24

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120425\
Data File : BF144425.D
Acq On : 04 Dec 2025 12:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 04 12:52:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

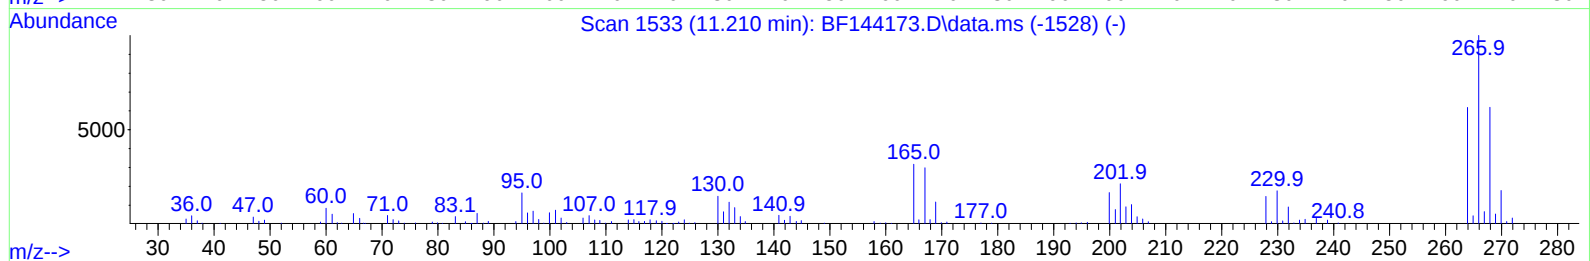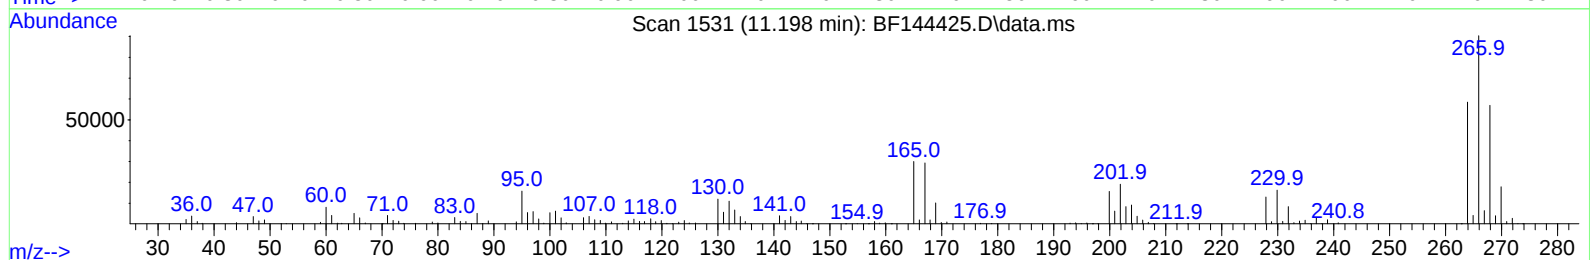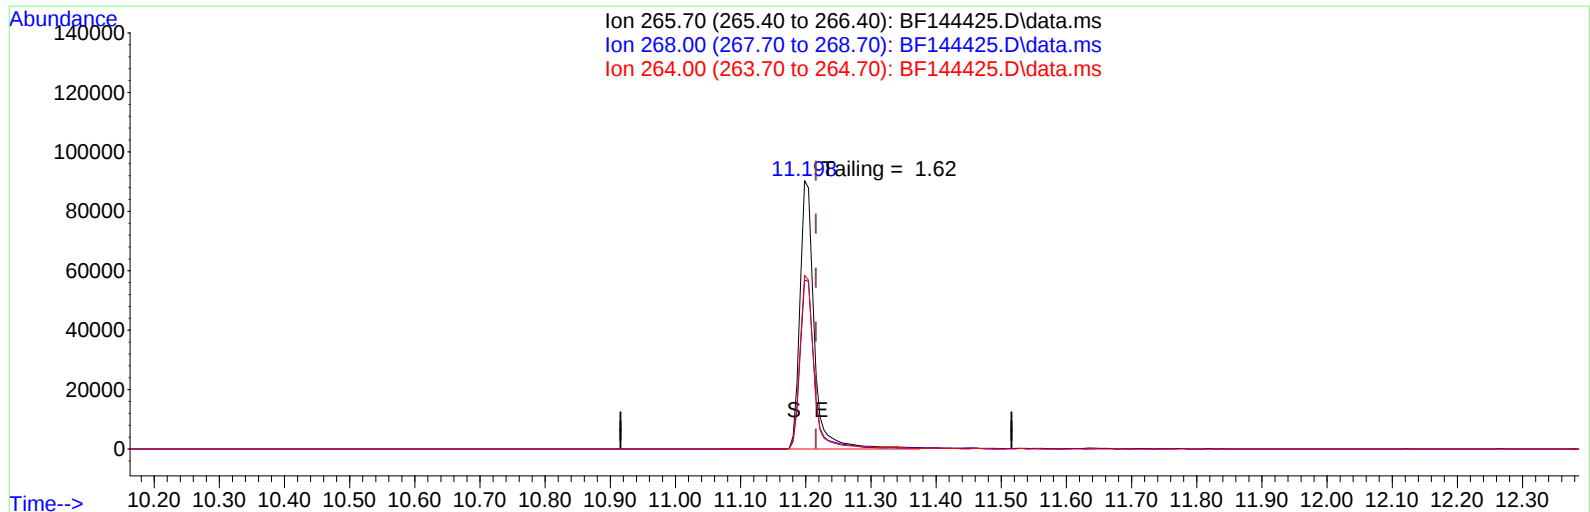

TIC: BF144425.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.018) 54055.10 ng




response 139212

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	63.01
264.00	61.80	64.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120425\
Data File : BF144425.D
Acq On : 04 Dec 2025 12:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 04 12:52:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

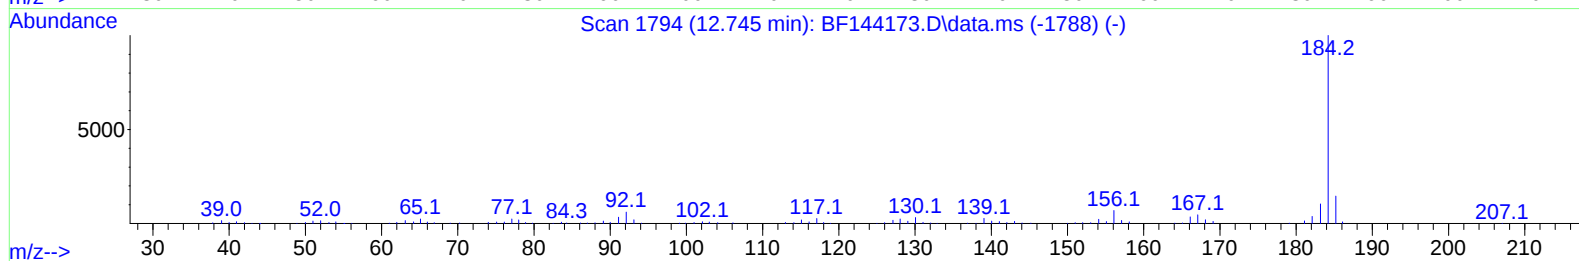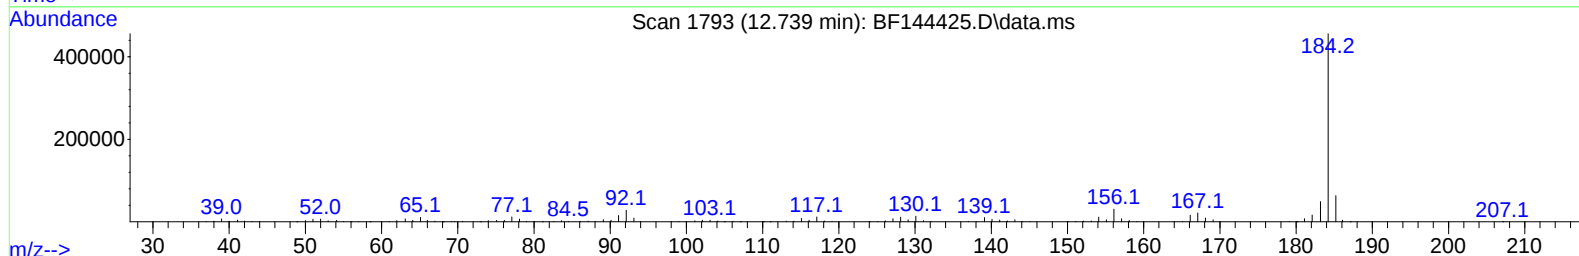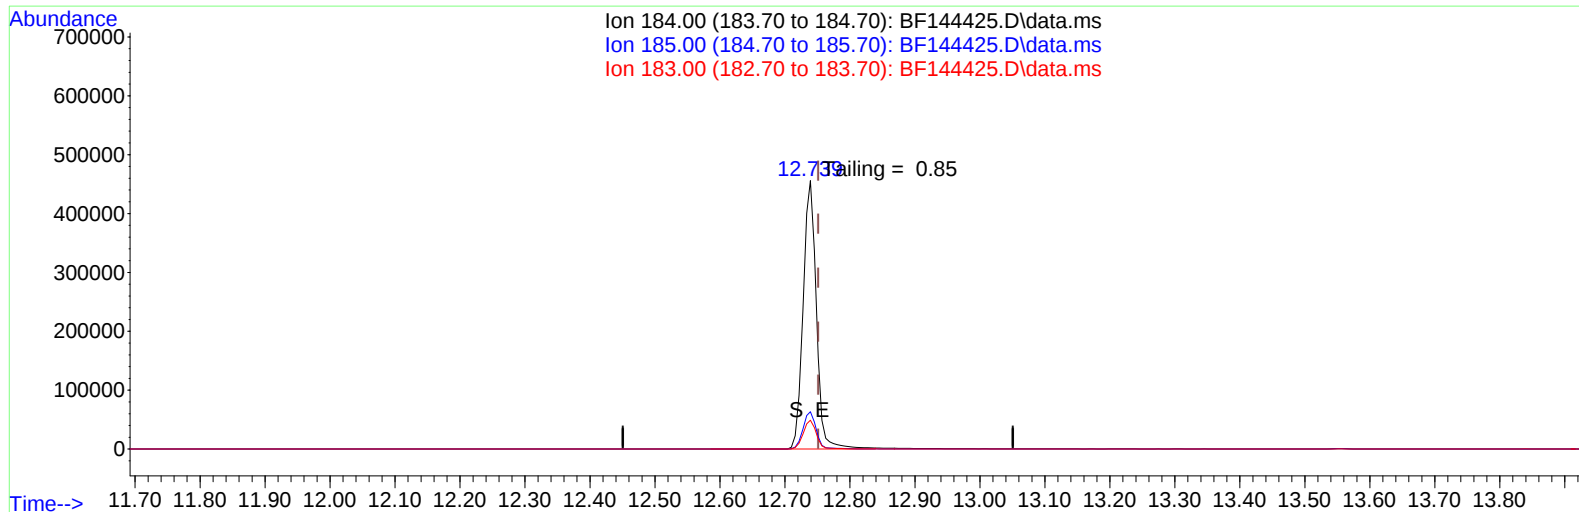

TIC: BF144425.D\data.ms

(77) Benzidine

12.739min (-0.012) 22803.06 ng

response 650891

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.91
183.00	10.40	10.76
0.00	0.00	0.00

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/4/2025	BNA_F	<u>BF144425.D</u>
Compound Name	Response	Retention Time
DDT	244998	13.557
DDD	9866	13.257
DDE	989	12.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10855	255853	4.24

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120425\
Data File : BF144425.D
Acq On : 04 Dec 2025 12:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 04 12:52:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

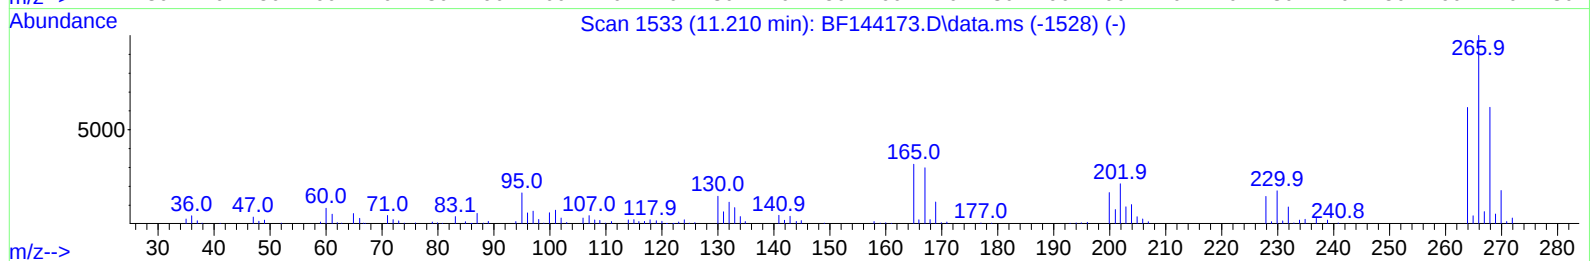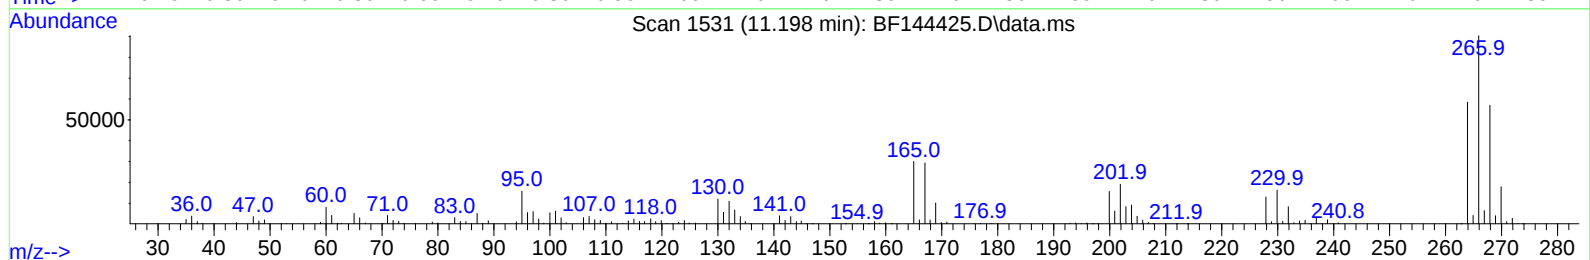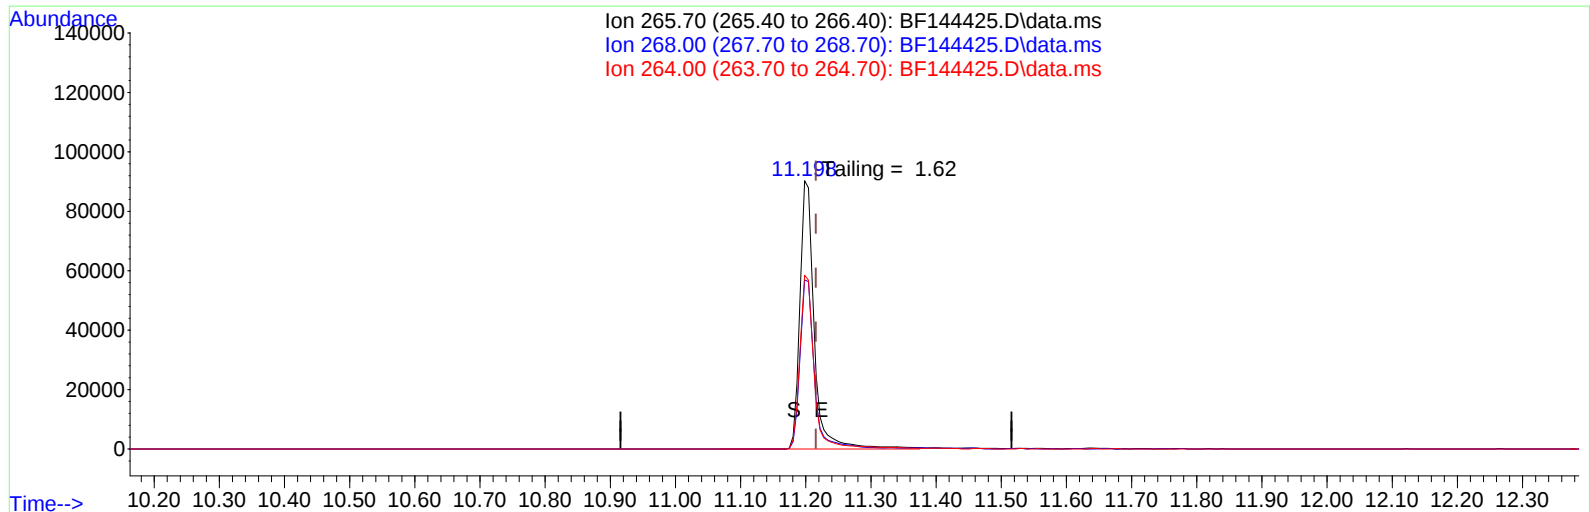

TIC: BF144425.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.018) 54055.10 ng




response 139212

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	63.01
264.00	61.80	64.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120425\
Data File : BF144425.D
Acq On : 04 Dec 2025 12:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 04 12:52:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

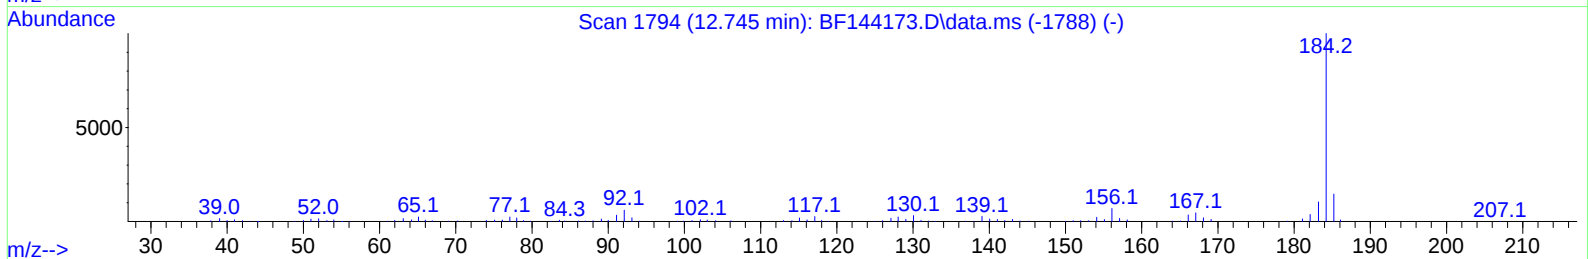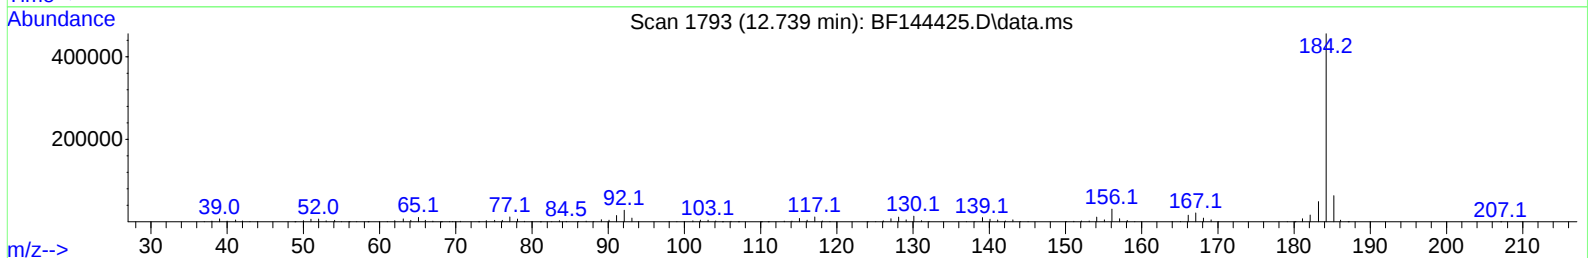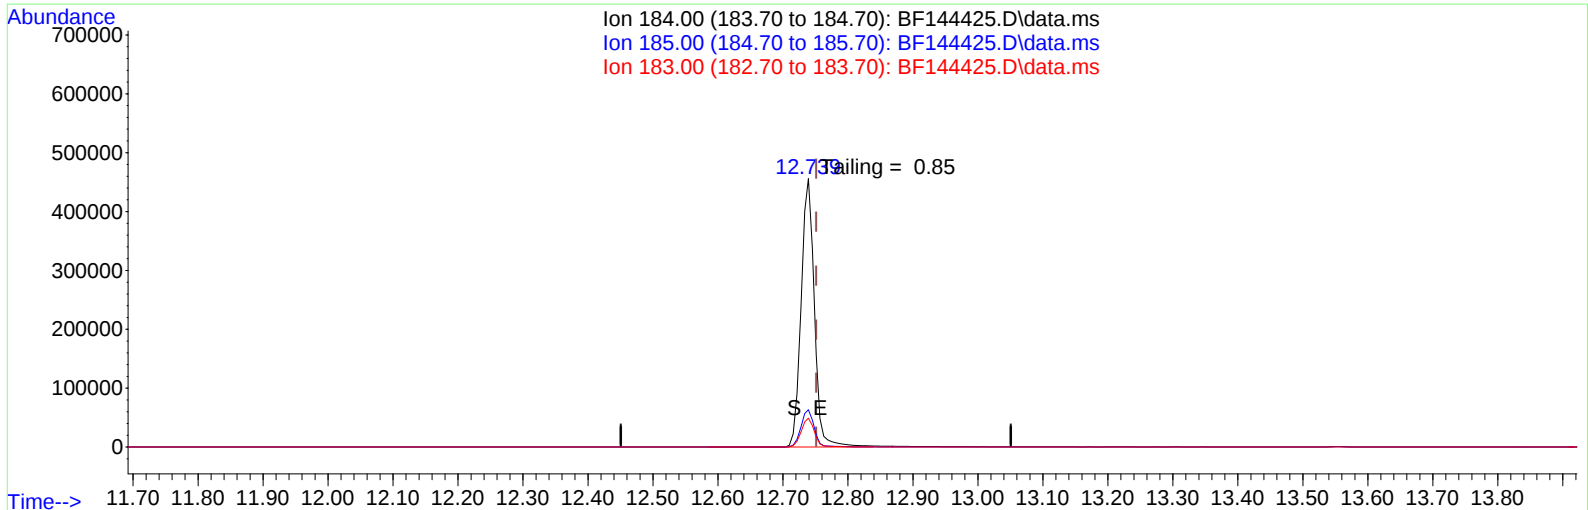

TIC: BF144425.D\data.ms

(77) Benzidine

12.739min (-0.012) 22803.06 ng

response 650891

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.91
183.00	10.40	10.76
0.00	0.00	0.00