
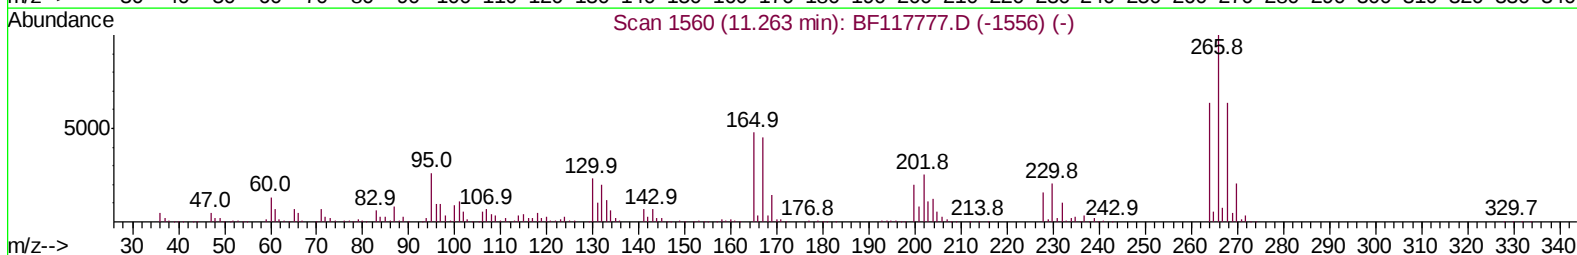
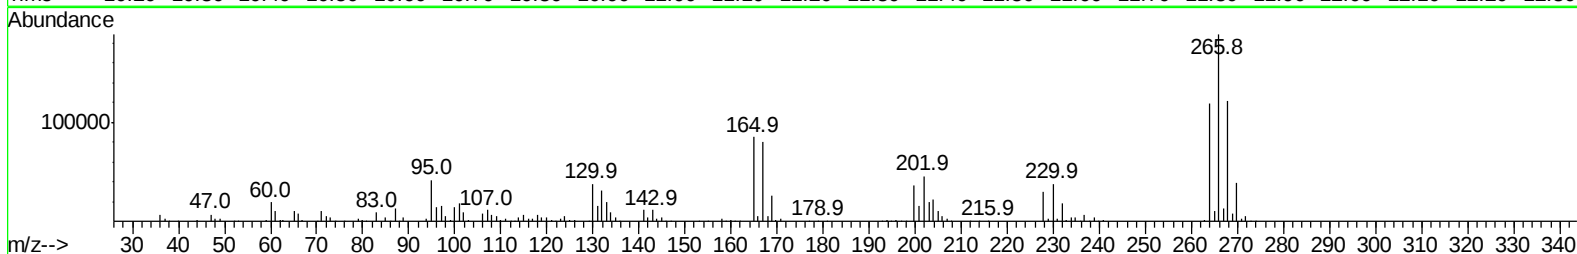


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF120519\
Data File : BF118106.D
Acq On : 5 Dec 2019 15:24
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 06:19:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 03 15:16:53 2019
Response via : Initial Calibration

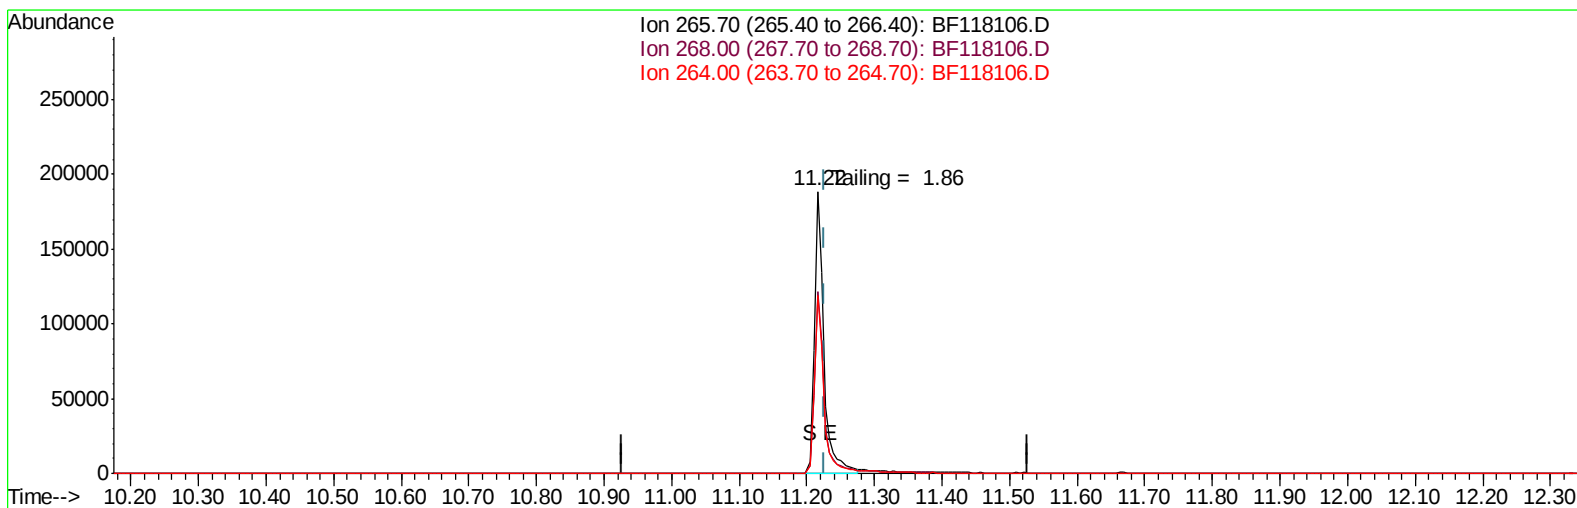

TIC: BF118106.D

(70) Pentachlorophenol (C)




11.216min (-0.012) 35603.54ng

response 193923

Ion	Exp%	Act%
265.70	100	100
268.00	62.90	64.73
264.00	62.90	63.09
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF120519\
Data File : BF118106.D
Acq On : 5 Dec 2019 15:24
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 06:19:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 03 15:16:53 2019
Response via : Initial Calibration

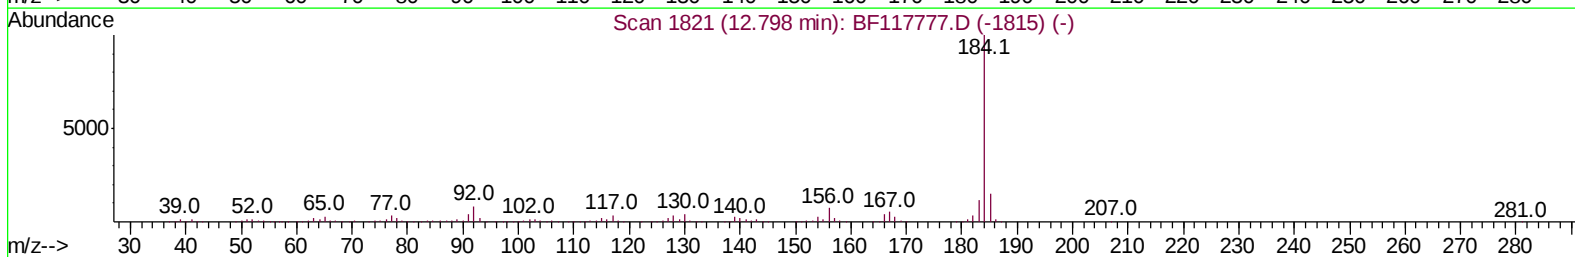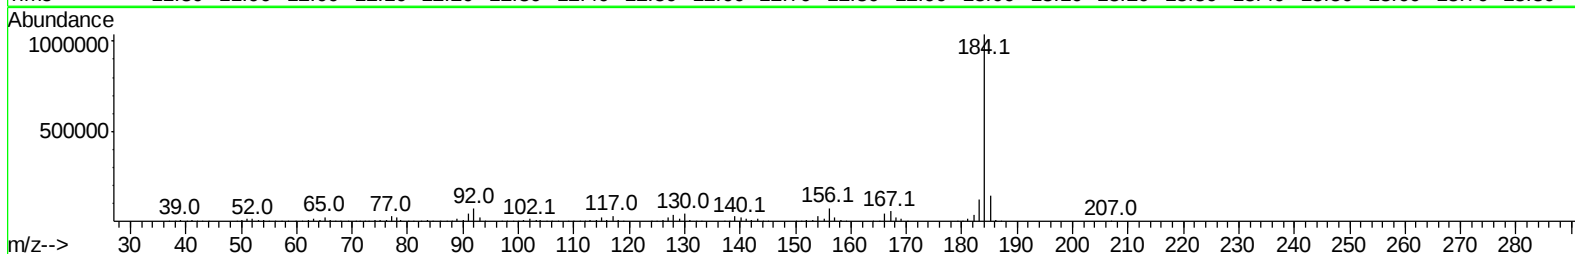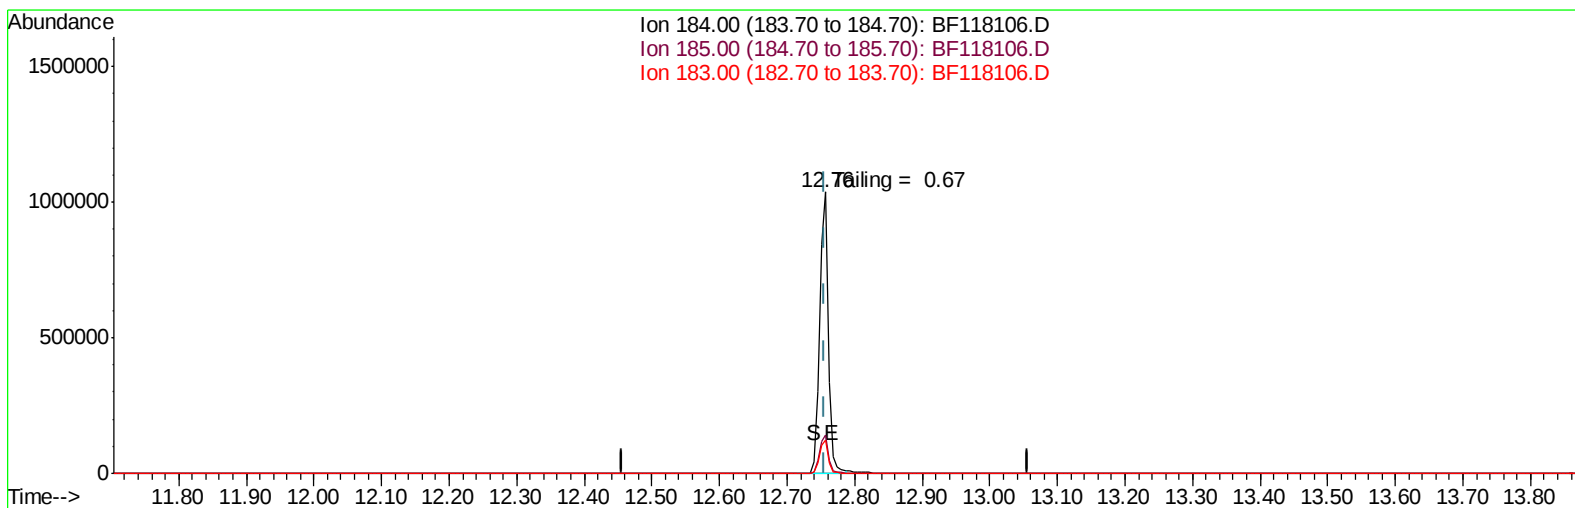

TIC: BF118106.D

(77) Benzidine

12.757min (+0.000) 0.00ng

response 960393

Ion	Exp%	Act%
184.00	100	100
185.00	14.50	13.85
183.00	12.10	11.98
0.00	0.00	0.00