


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120519\
 Data File : BF118106.D
 Acq On : 5 Dec 2019 15:24
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF111319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 03 15:16:53 2019

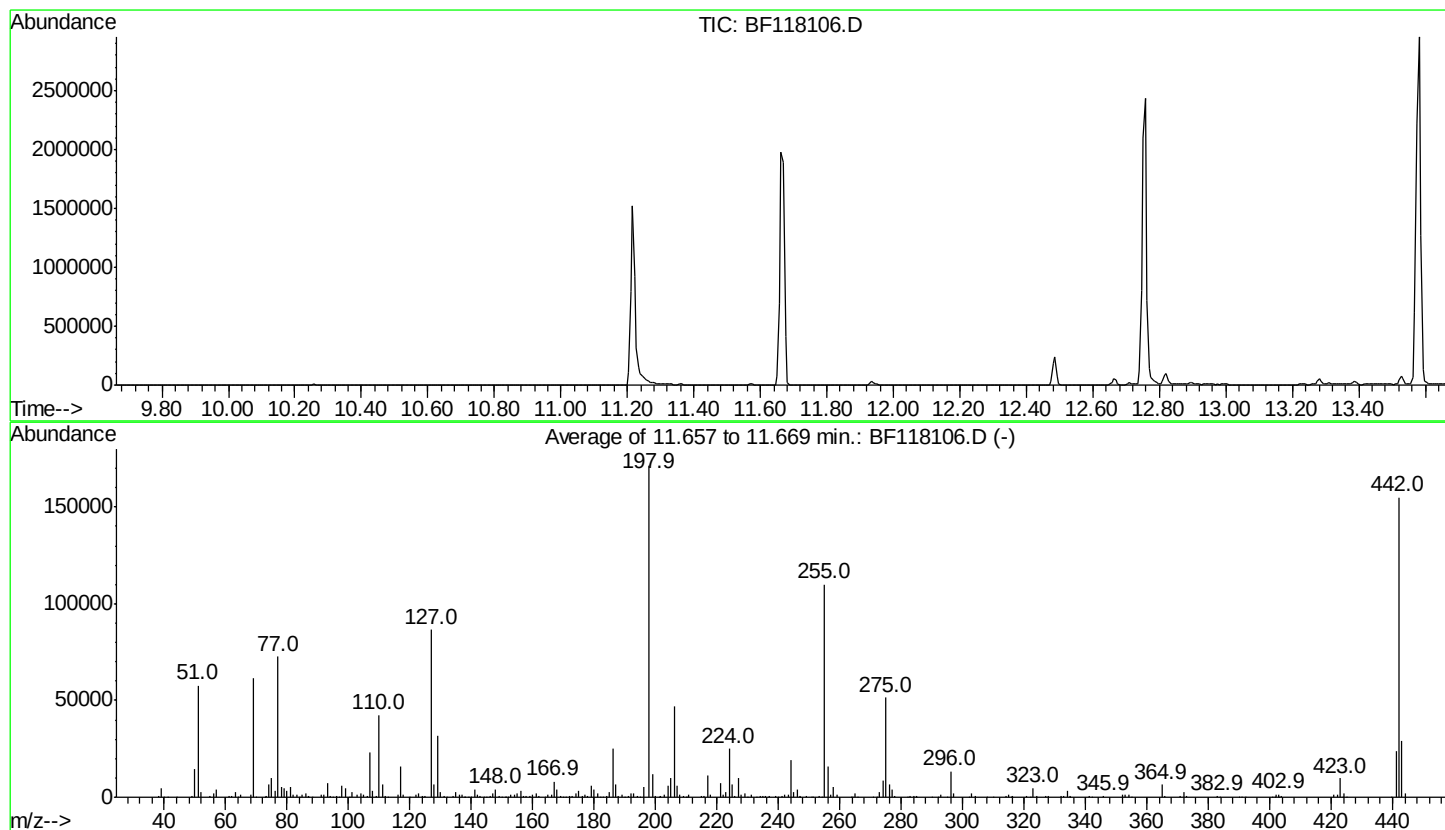

AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	57722	PASS
68	69	0.00	2	1.8	1122	PASS
69	198	0.00	100	36.0	61696	PASS
70	69	0.00	2	0.5	295	PASS
127	198	10	80	50.6	86656	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	171397	PASS
199	198	5	9	6.8	11687	PASS
275	198	10	60	30.0	51469	PASS
365	198	1	100	3.8	6586	PASS
441	198	0.01	100	13.8	23687	PASS
442	198	50	100	90.3	154848	PASS
443	442	15	24	18.7	29023	PASS