


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120522\
Data File : BF131502.D
Acq On : 05 Dec 2022 14:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120522.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Dec 06 01:30:30 2022

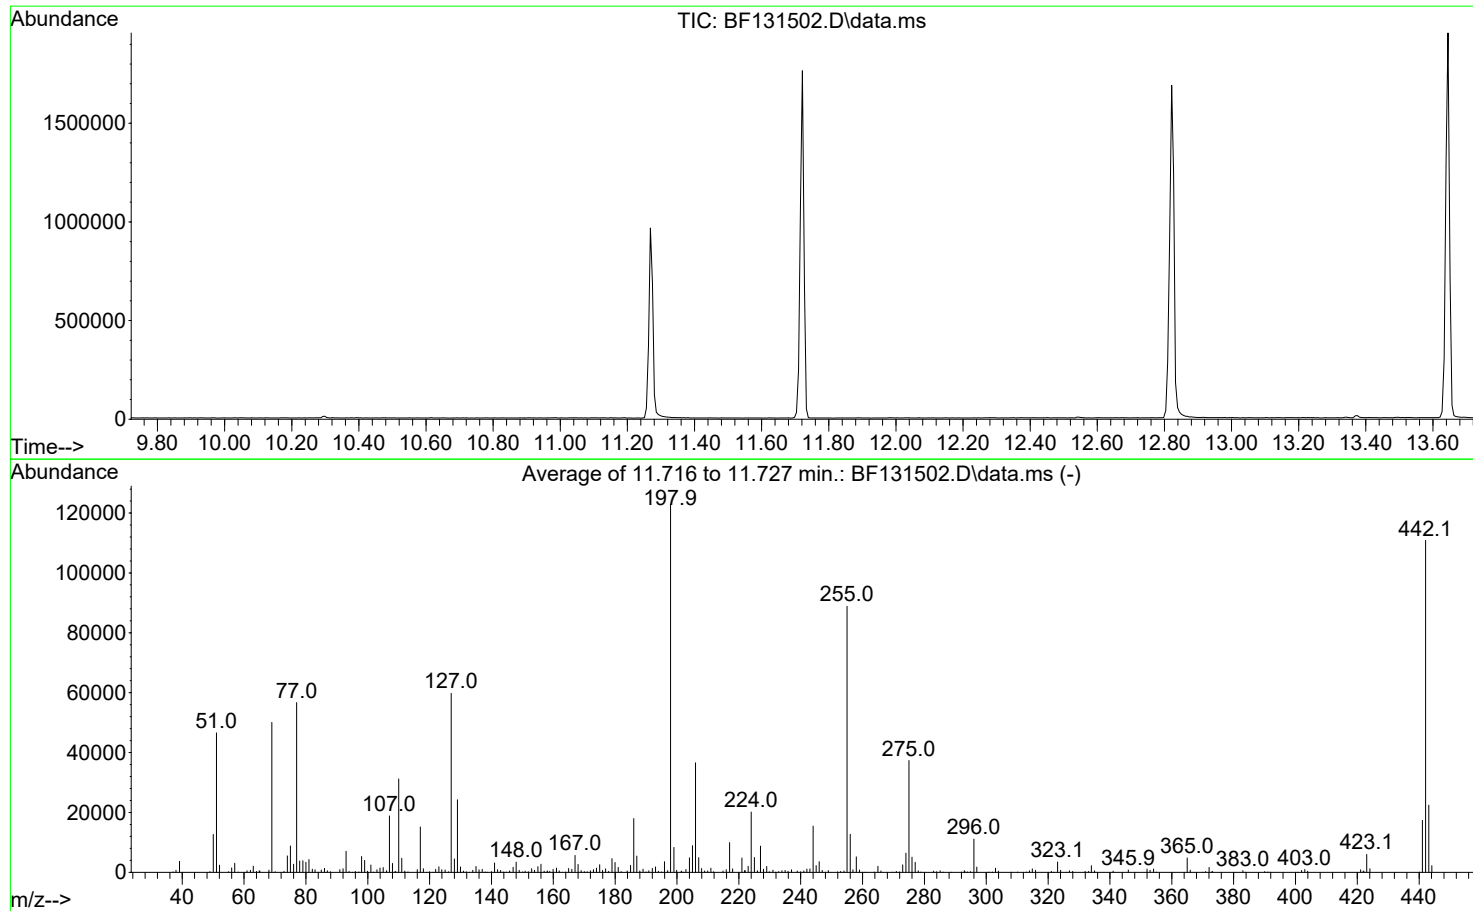


AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	46616	PASS
68	69	0.00	2	1.5	742	PASS
69	198	0.00	100	40.8	50075	PASS
70	69	0.00	2	0.4	222	PASS
127	198	10	80	48.7	59821	PASS
197	198	0.00	2	0.5	594	PASS
198	198	100	100	100.0	122851	PASS
199	198	5	9	6.8	8337	PASS
275	198	10	60	30.4	37344	PASS
365	198	1	100	3.9	4794	PASS
441	198	0.01	100	14.1	17347	PASS
442	442	50	100	100.0	110864	PASS
443	442	15	24	20.2	22438	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120522\
 Data File : BF131502.D
 Acq On : 05 Dec 2022 14:28
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Dec 06 06:00:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 06 01:30:30 2022
 Response via : Initial Calibration

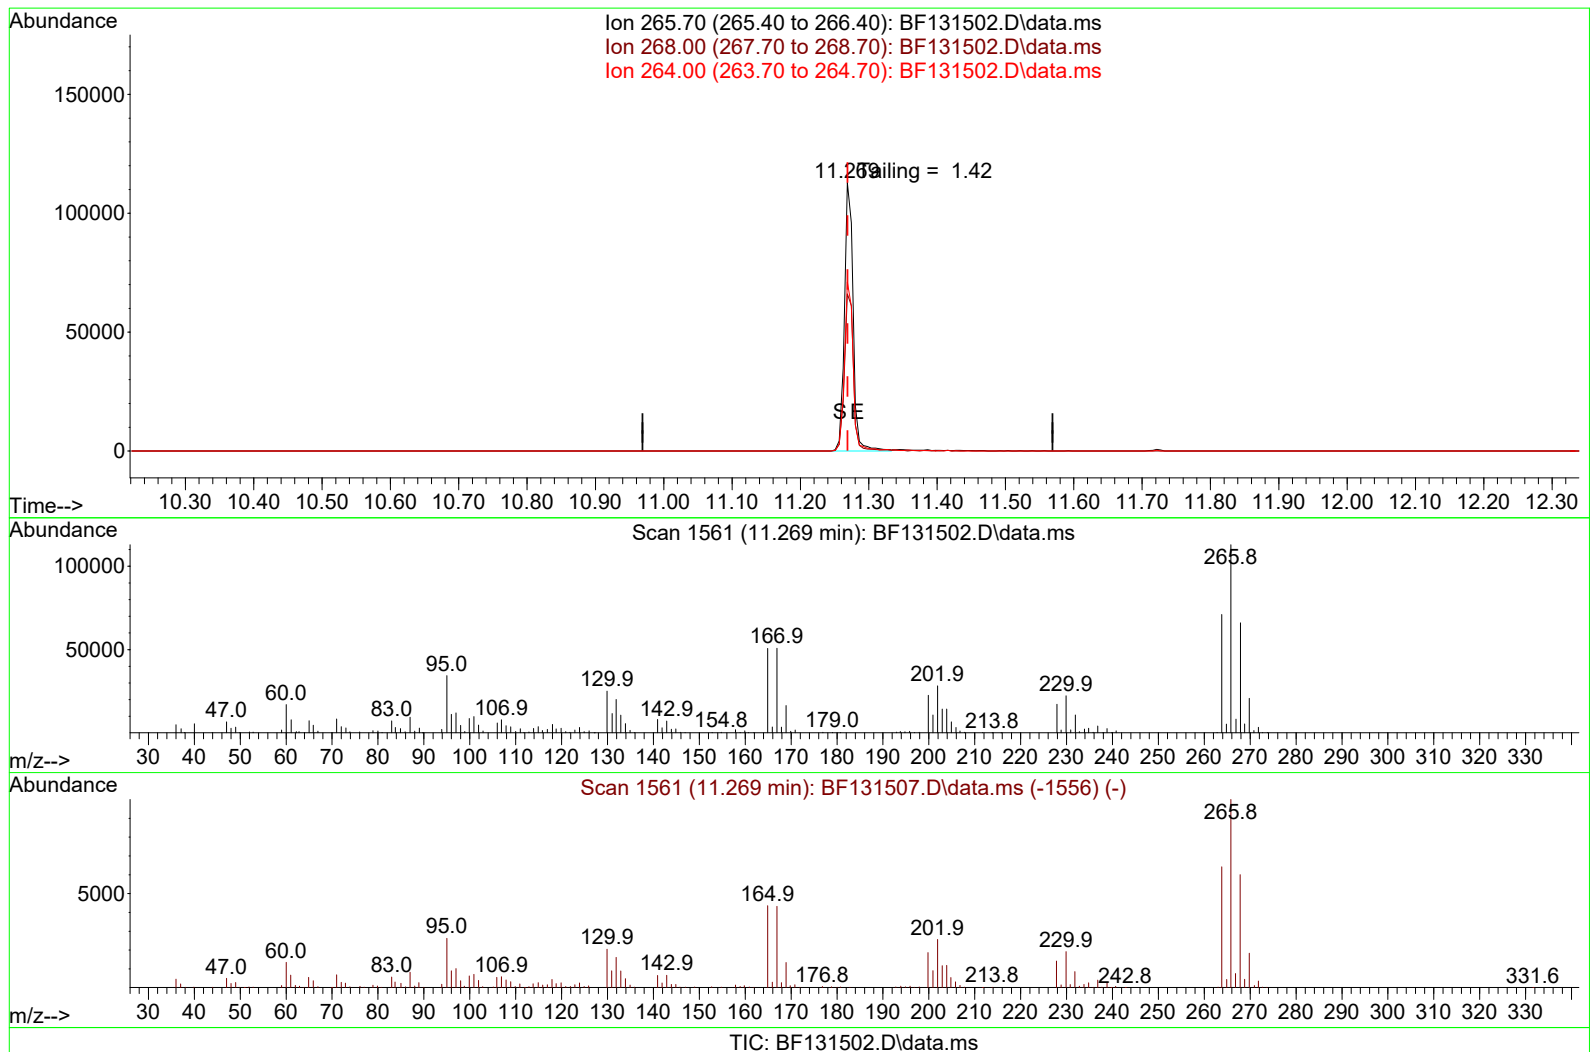

TIC: BF131502.D\data.ms

(70) Pentachlorophenol (C)

11.269min (-0.000) 26131.93 ng




response 99334

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.00	58.54
264.00	64.20	62.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120522\
Data File : BF131502.D
Acq On : 05 Dec 2022 14:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 06 06:00:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 06 01:30:30 2022
Response via : Initial Calibration

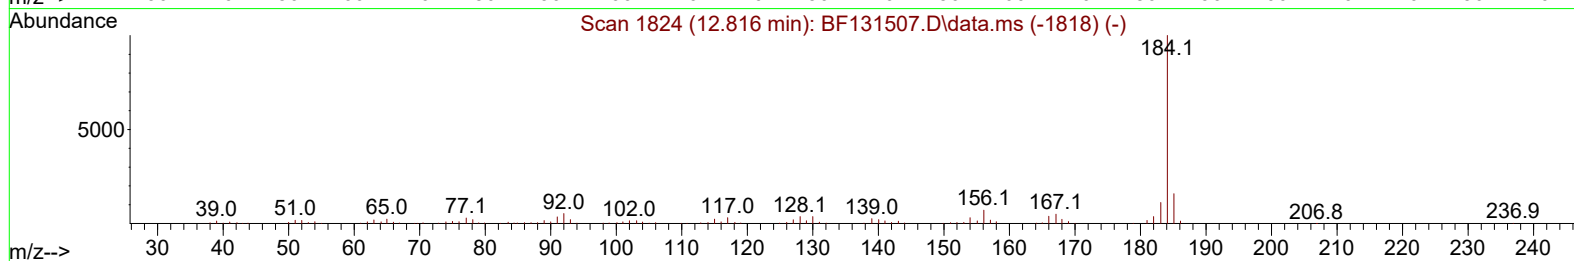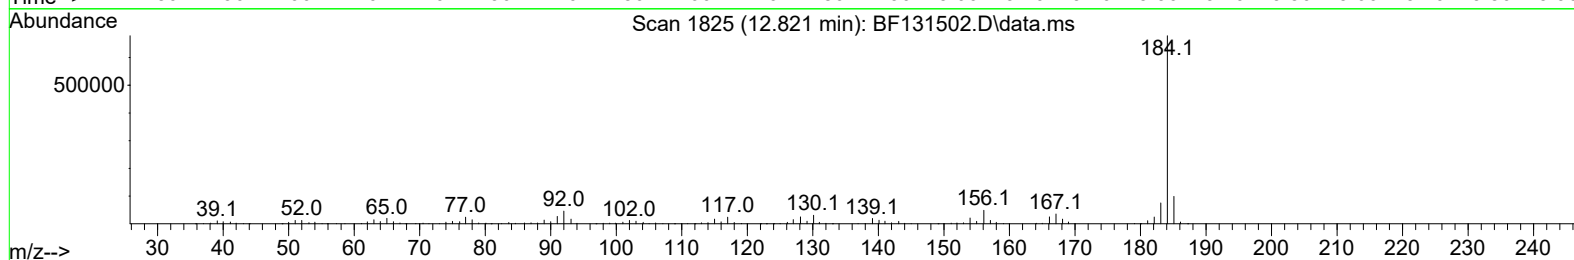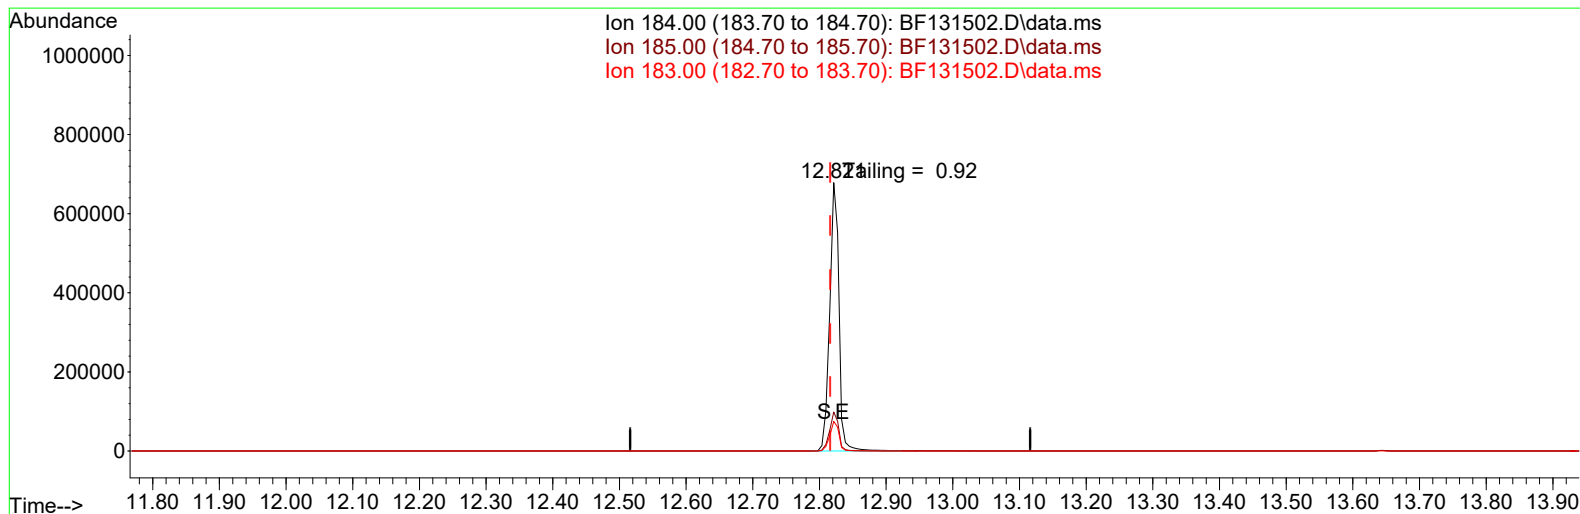

TIC: BF131502.D\data.ms

(77) Benzidine

12.821min (+ 0.005) 0.00 ng

response 654519

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.80	14.54
183.00	11.20	11.06
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/5/2022	BNA_F	<u>BF131502.D</u>
Compound Name	Response	Retention Time
DDT	272588	13.645
DDD	2806	13.374
DDE	0	13.004
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2806	275394	1.02

Instrument :
BNA_F
ClientSampleId :
DFTPP