
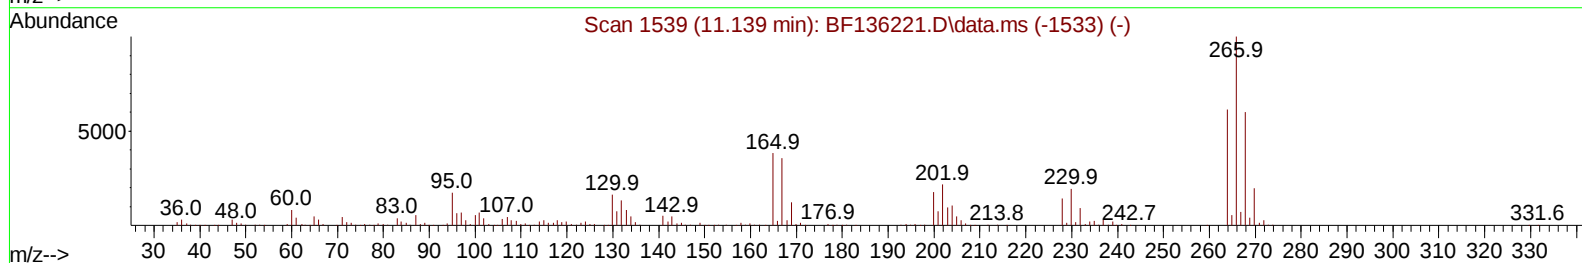
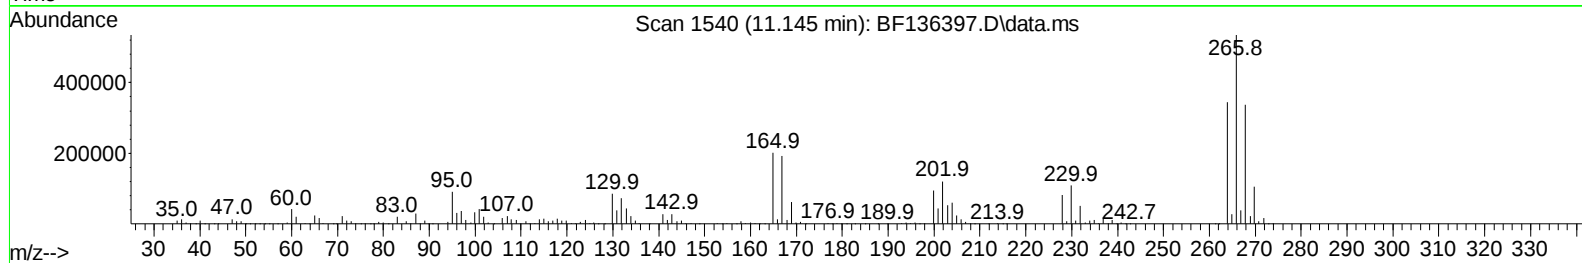


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120523\
 Data File : BF136397.D
 Acq On : 05 Dec 2023 09:33
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 05 10:56:44 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 04 13:30:53 2023
 Response via : Initial Calibration

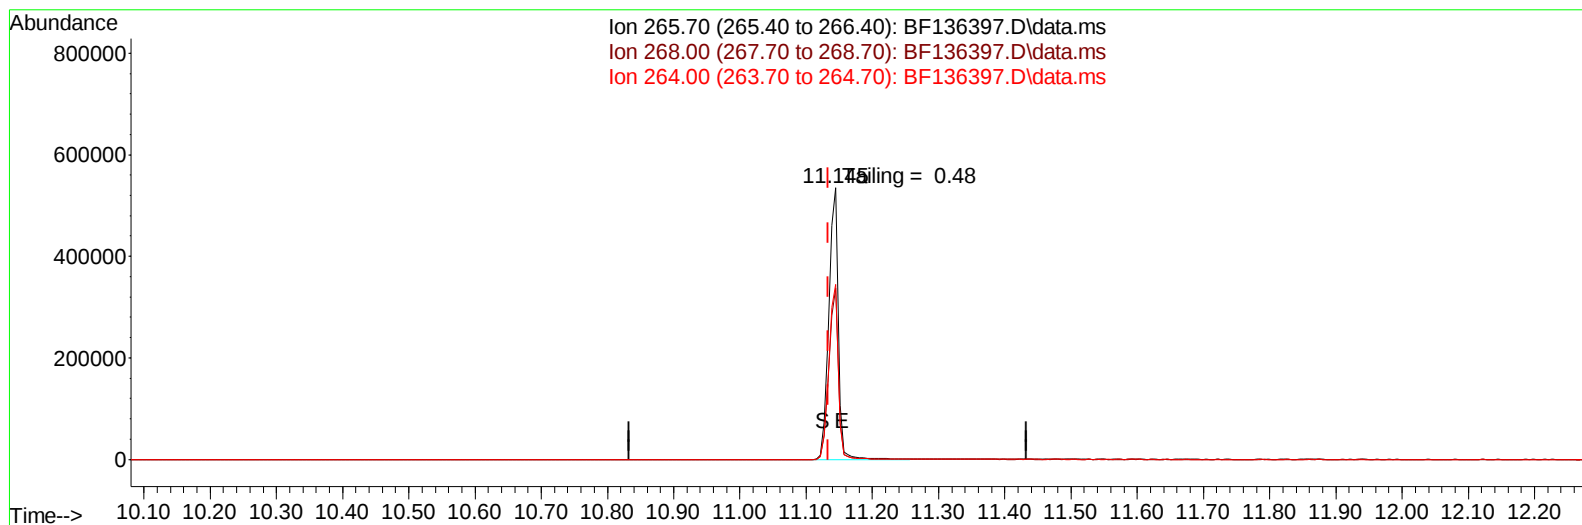

TIC: BF136397.D\data.ms

(70) Pentachlorophenol (C)




11.145min (+ 0.012) 44025.82 ng

response 523524

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.90	63.16
264.00	61.40	64.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120523\
Data File : BF136397.D
Acq On : 05 Dec 2023 09:33
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 05 10:56:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 04 13:30:53 2023
Response via : Initial Calibration

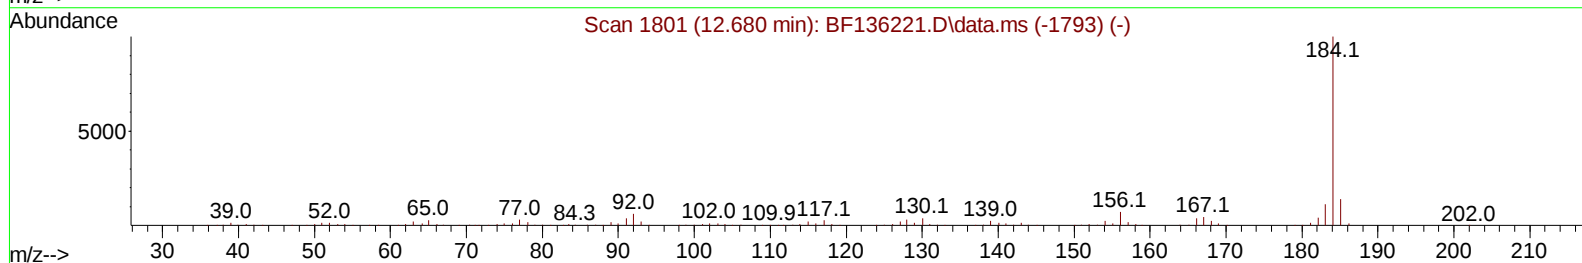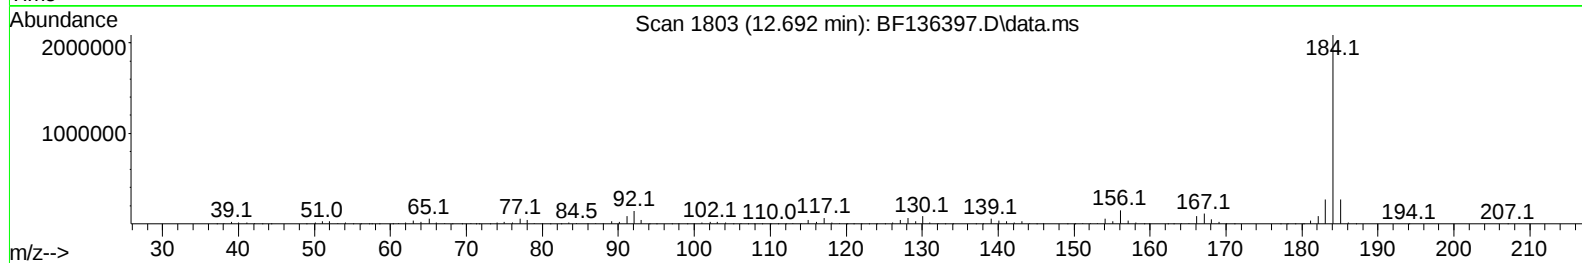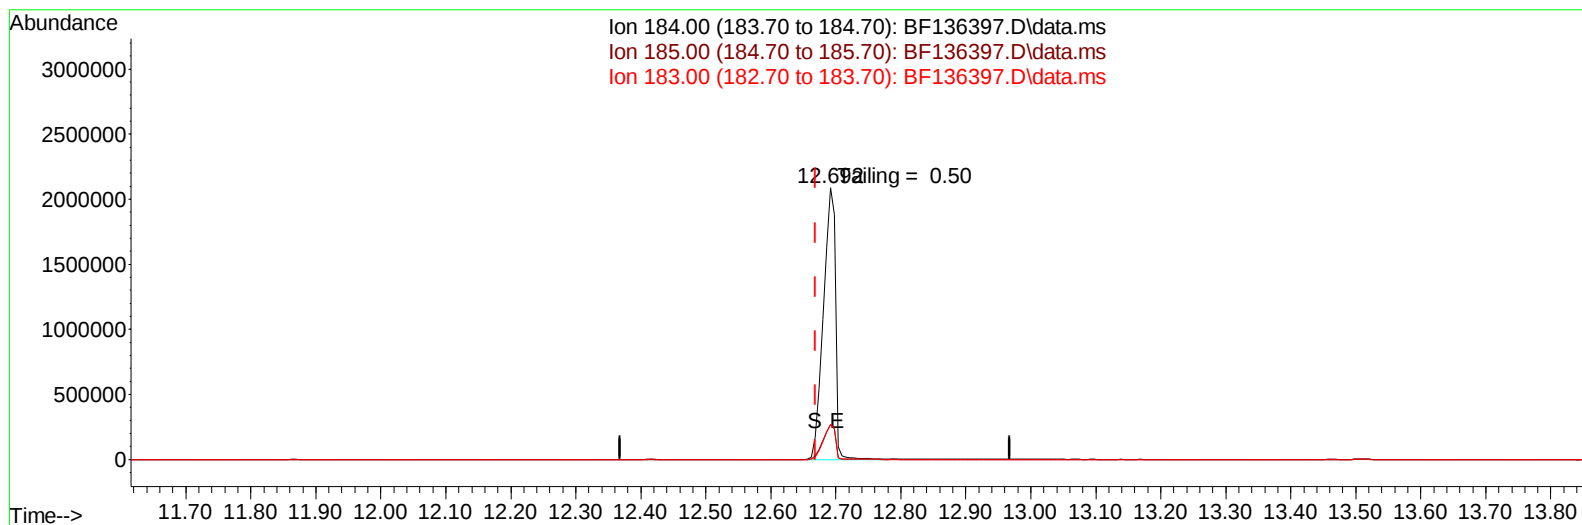

TIC: BF136397.D\data.ms

(77) Benzidine

12.692min (+ 0.024) 182868.31 ng

response 2699421

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	12.83
183.00	11.20	12.96
0.00	0.00	0.00