
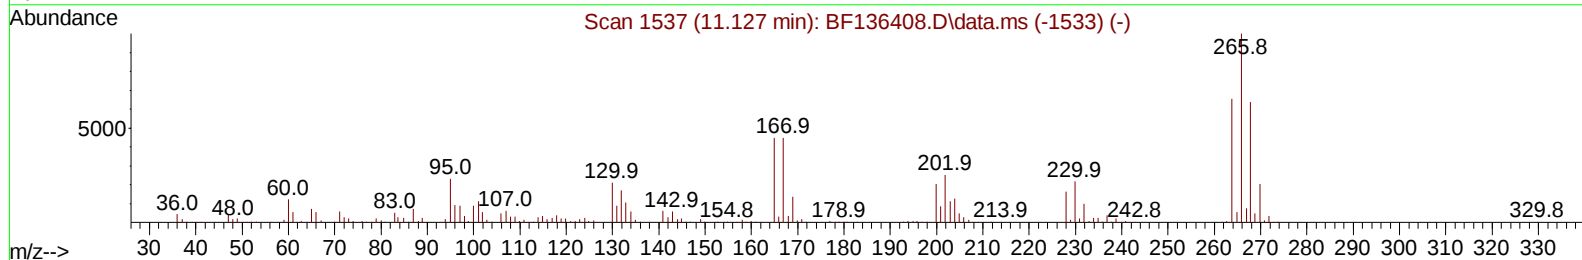
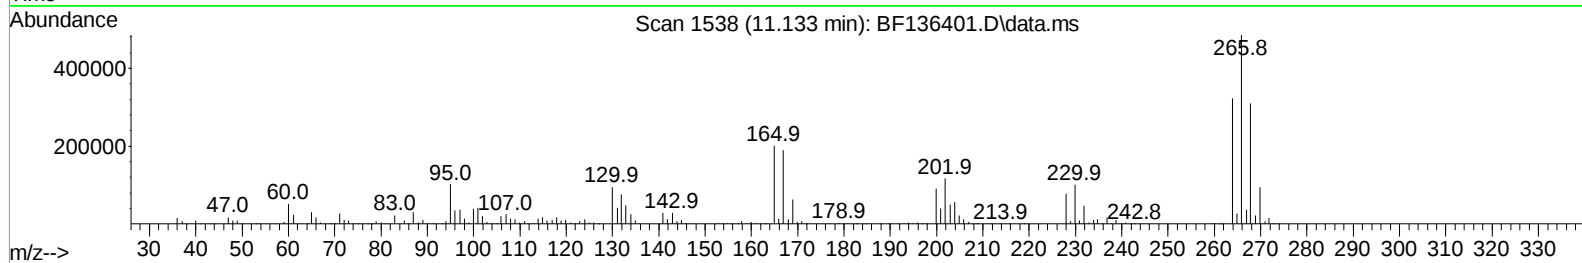


Quant Time: Dec 05 17:41:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 05 17:37:37 2023
Response via : Initial Calibration

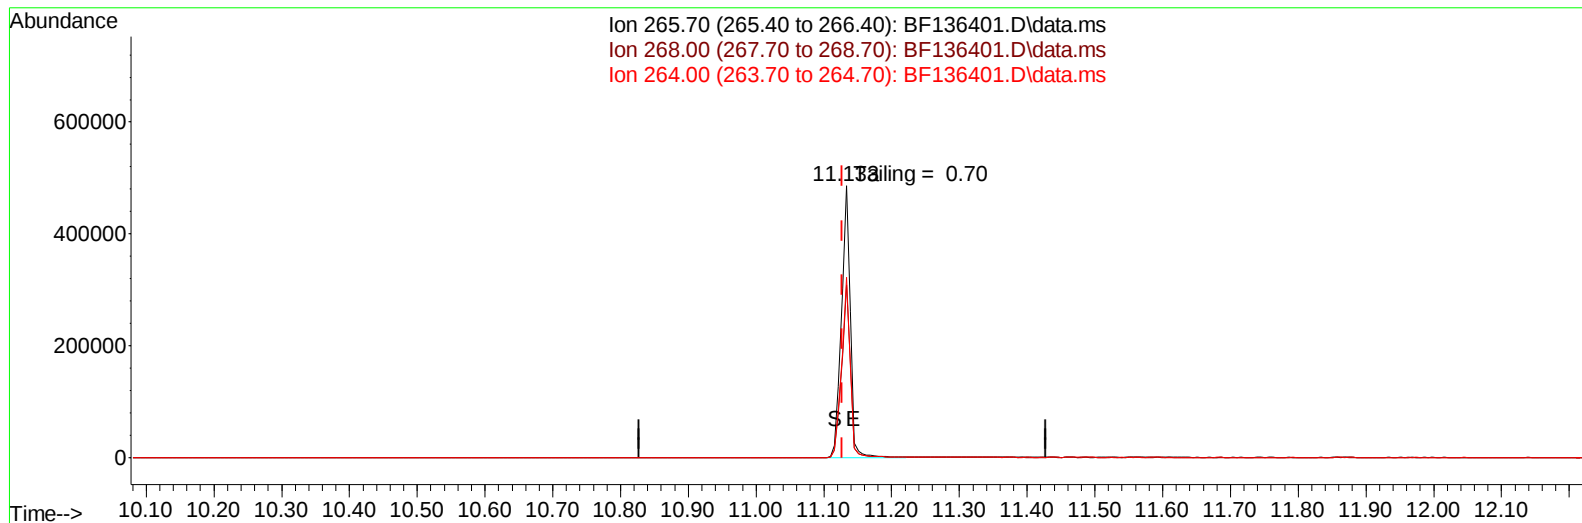

TIC: BF136401.D\data.ms




11.133min (+ 0.006) 45366.72 ng

response **446248**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.61
264.00	63.40	66.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120523\
Data File : BF136401.D
Acq On : 05 Dec 2023 12:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 05 17:41:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 05 17:37:37 2023
Response via : Initial Calibration

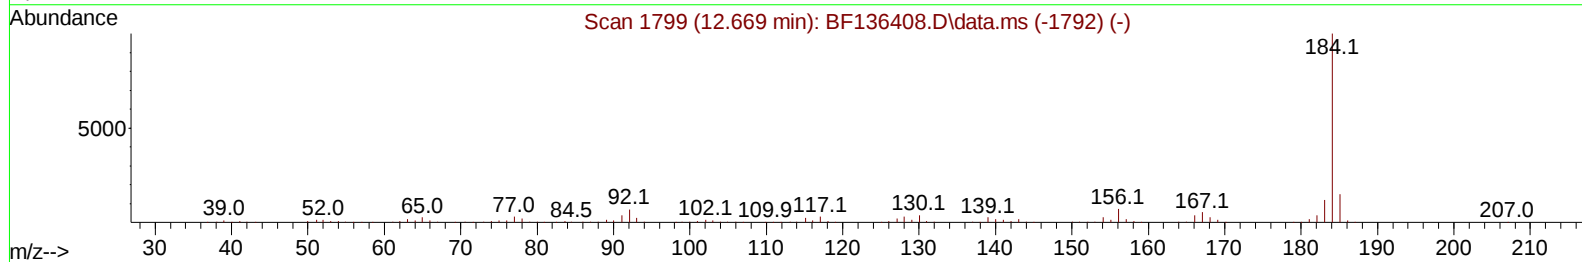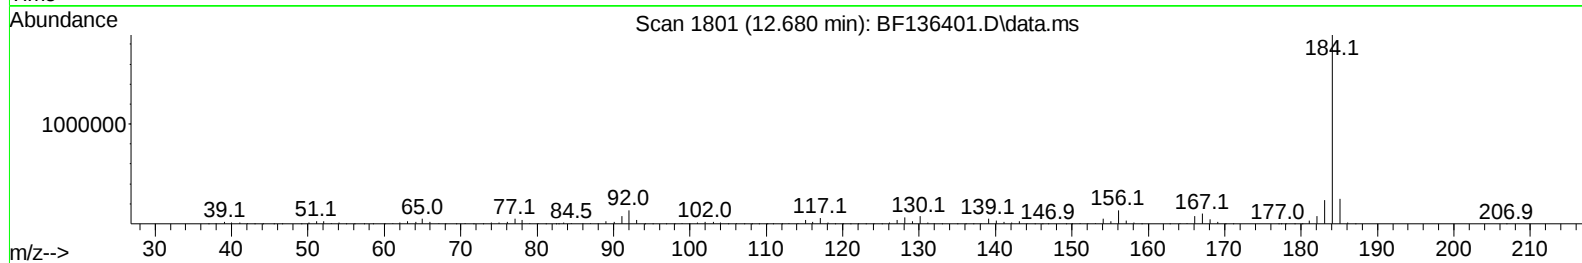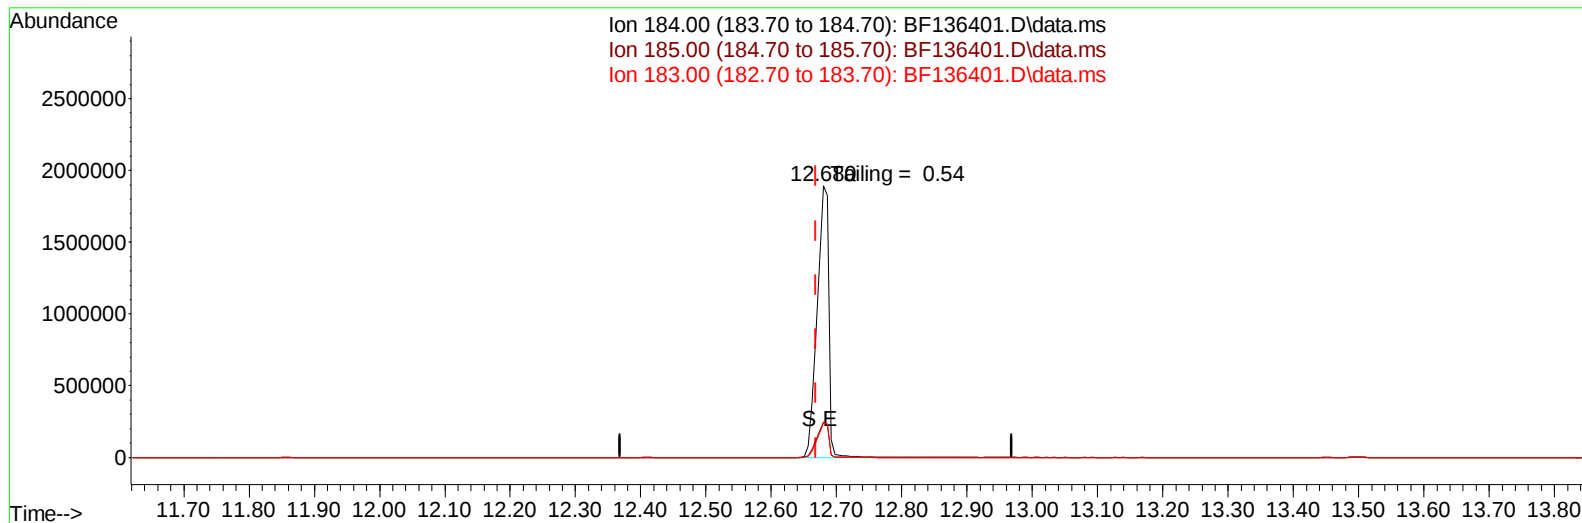

TIC: BF136401.D\data.ms

(77) Benzidine**12.680min (+ 0.011) 131568.41 ng****response 2347142**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.20
183.00	11.90	12.68
0.00	0.00	0.00