
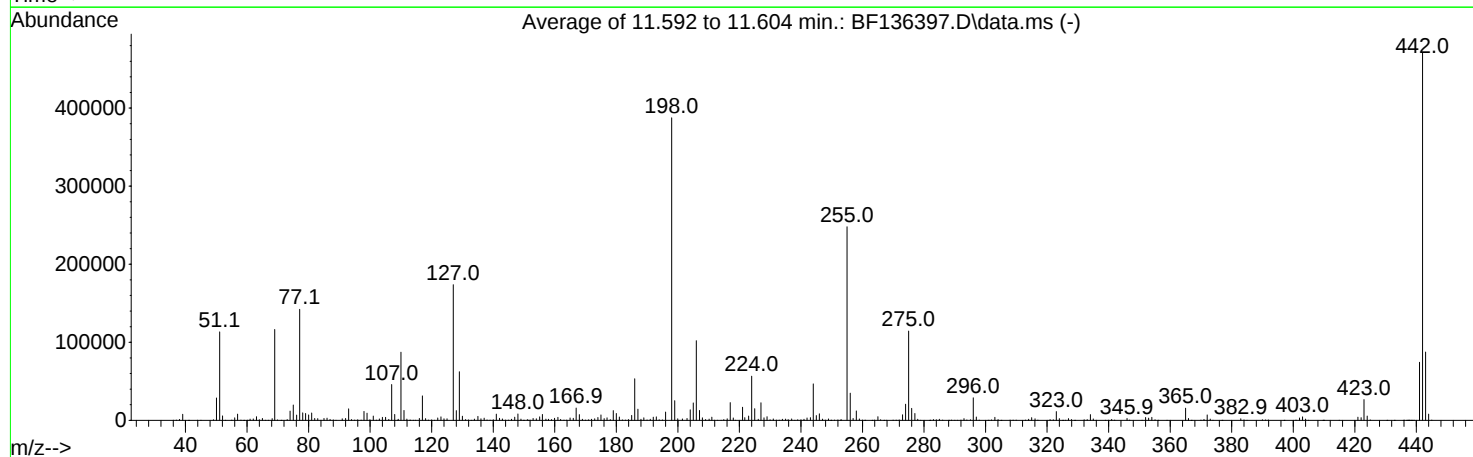


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120523\
Data File : BF136397.D
Acq On : 05 Dec 2023 09:33
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Dec 04 13:30:53 2023

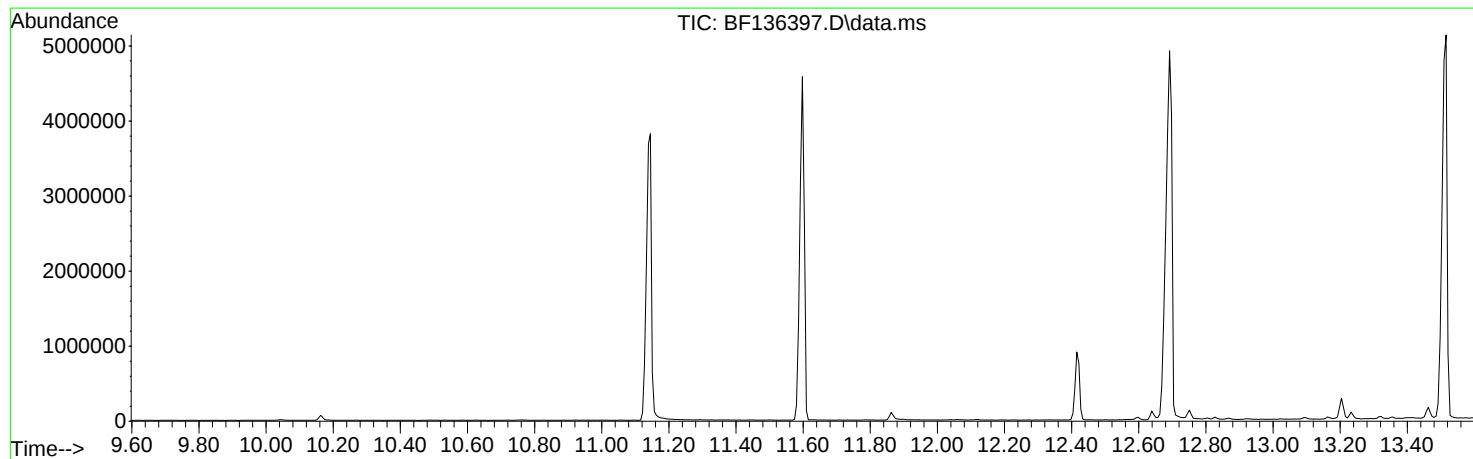




AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.2	113320	PASS
68	69	0.00	2	2.0	2294	PASS
69	198	0.00	100	30.1	116494	PASS
70	69	0.00	2	0.6	690	PASS
127	198	10	80	44.8	173805	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	387584	PASS
199	198	5	9	6.5	25191	PASS
275	198	10	60	29.5	114355	PASS
365	198	1	100	4.0	15659	PASS
441	198	0.01	100	19.2	74493	PASS
442	442	50	100	100.0	471211	PASS
443	442	15	24	18.6	87531	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120523\
Data File : BF136397.D
Acq On : 05 Dec 2023 09:33
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 05 10:56:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 04 13:30:53 2023
Response via : Initial Calibration

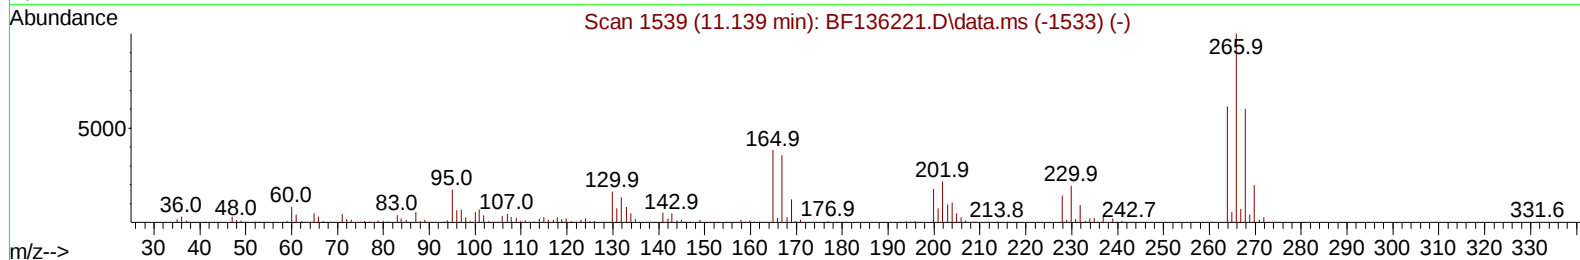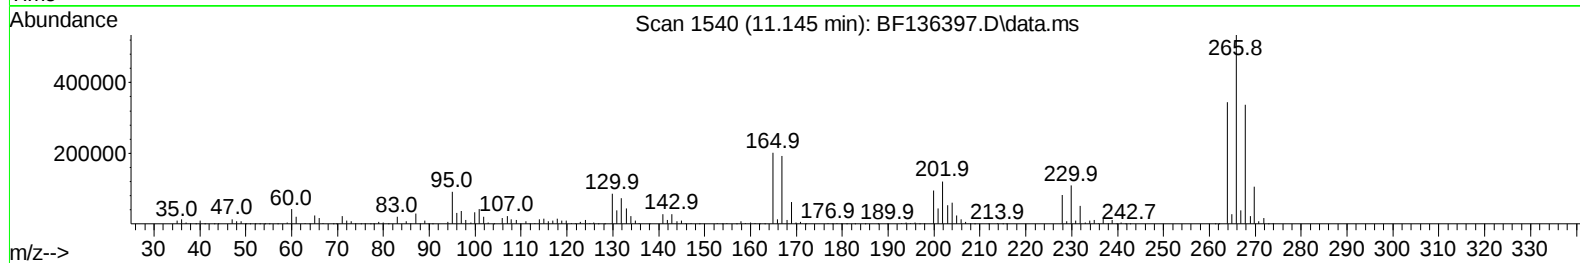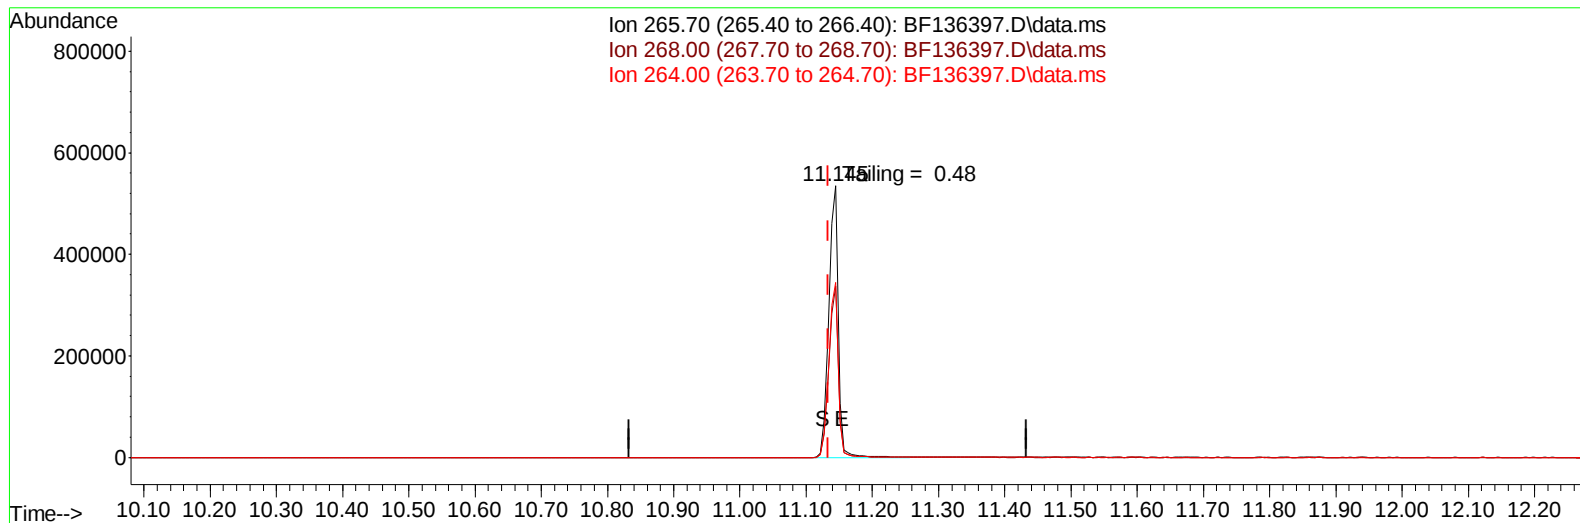

TIC: BF136397.D\data.ms

(70) Pentachlorophenol (C)

11.145min (+ 0.012) 44025.82 ng




response 523524

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.90	63.16
264.00	61.40	64.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120523\
Data File : BF136397.D
Acq On : 05 Dec 2023 09:33
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 05 10:56:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 04 13:30:53 2023
Response via : Initial Calibration

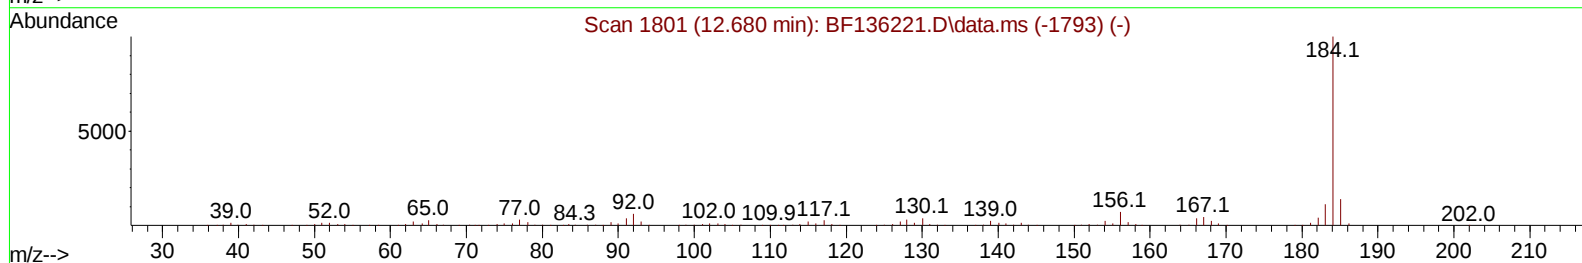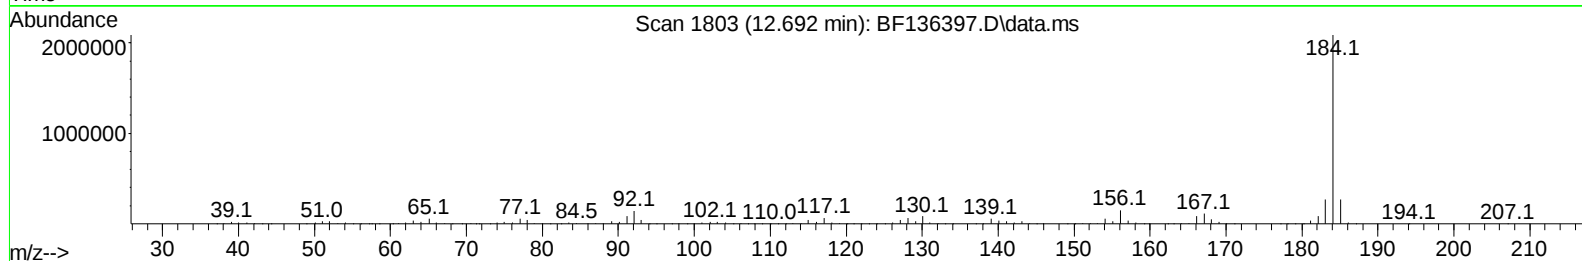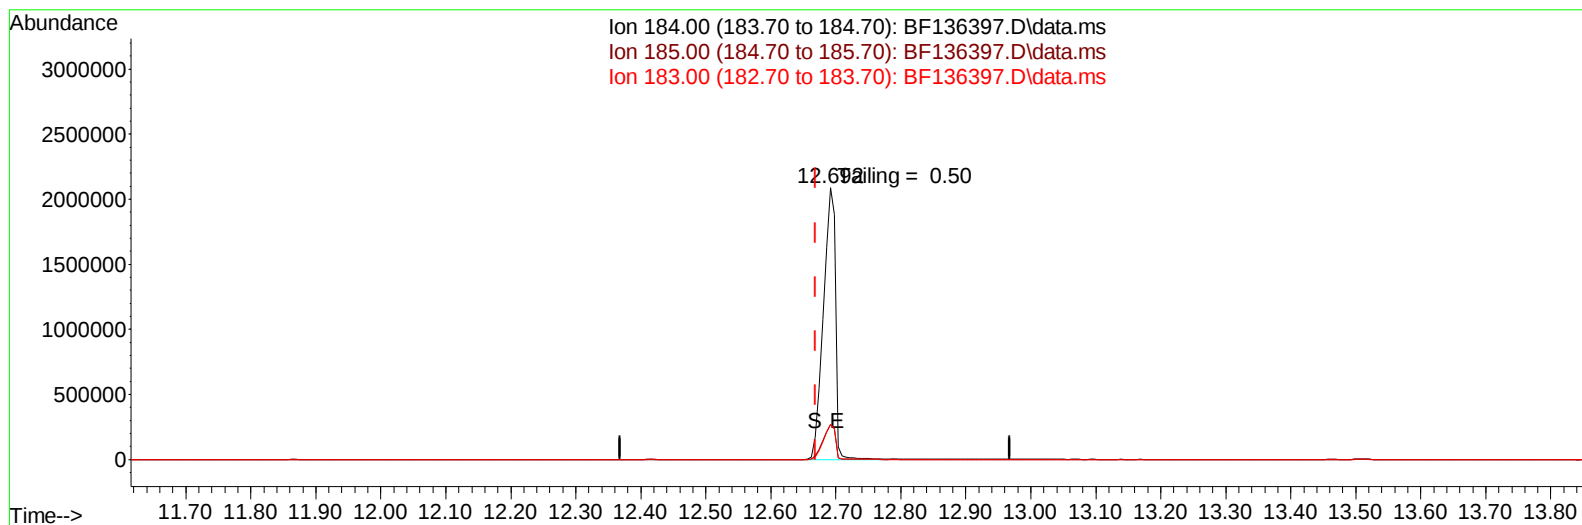

TIC: BF136397.D\data.ms

(77) Benzidine

12.692min (+ 0.024) 182868.31 ng

response 2699421

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	12.83
183.00	11.20	12.96
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/5/2023	BNA_F	<u>BF136397.D</u>
Compound Name	Response	Retention Time
DDT	1126021	13.515
DDD	60853	13.204
DDE	1077	12.863
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
61930	1187951	5.21

Instrument :
BNA_F
ClientSampleId :
DFTPP