
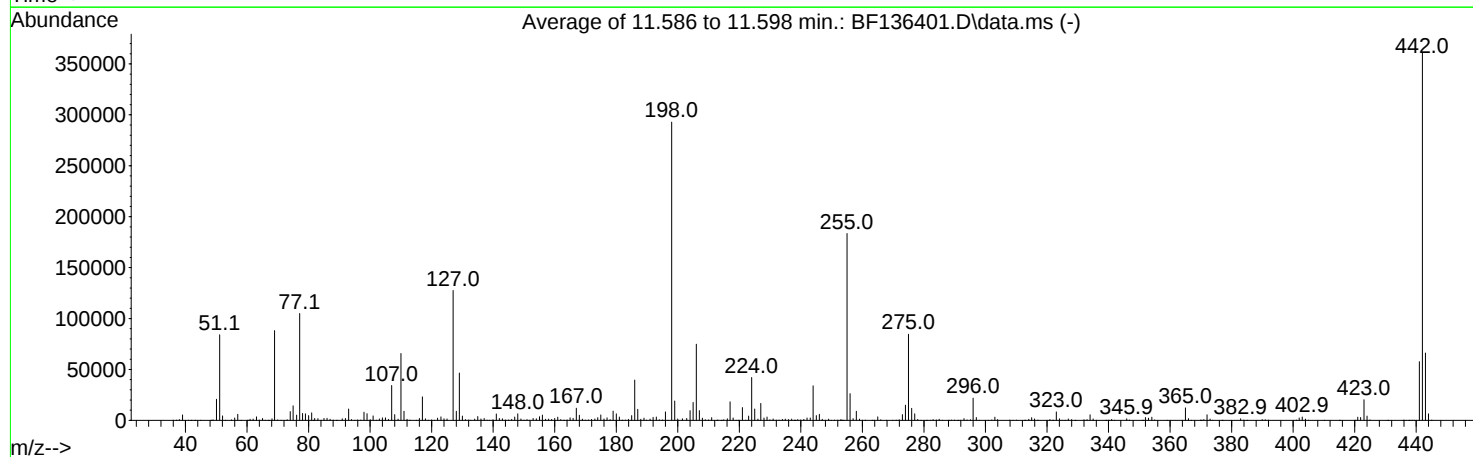


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120523\
Data File : BF136401.D
Acq On : 05 Dec 2023 12:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 06 09:40:27 2023

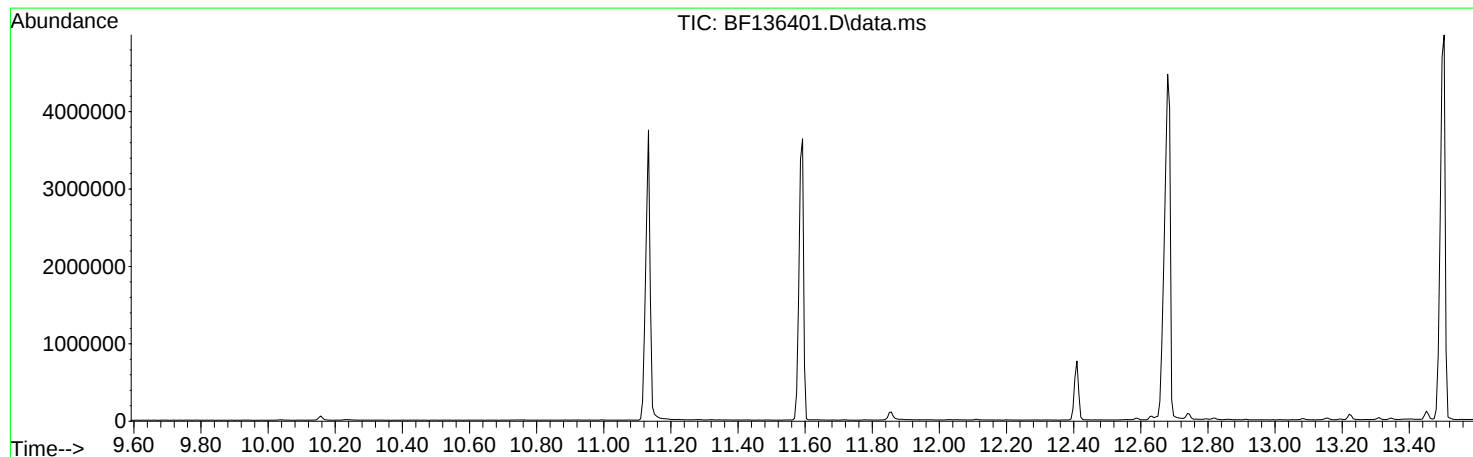




AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.7	84047	PASS
68	69	0.00	2	1.8	1558	PASS
69	198	0.00	100	30.1	88208	PASS
70	69	0.00	2	0.5	427	PASS
127	198	10	80	43.6	127573	PASS
197	198	0.00	2	0.0	138	PASS
198	198	100	100	100.0	292824	PASS
199	198	5	9	6.5	19002	PASS
275	198	10	60	28.9	84523	PASS
365	198	1	100	4.2	12234	PASS
441	198	0.01	100	19.7	57709	PASS
442	442	50	100	100.0	361195	PASS
443	442	15	24	18.3	66181	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120523\
Data File : BF136401.D
Acq On : 05 Dec 2023 12:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 05 17:41:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 05 17:37:37 2023
Response via : Initial Calibration

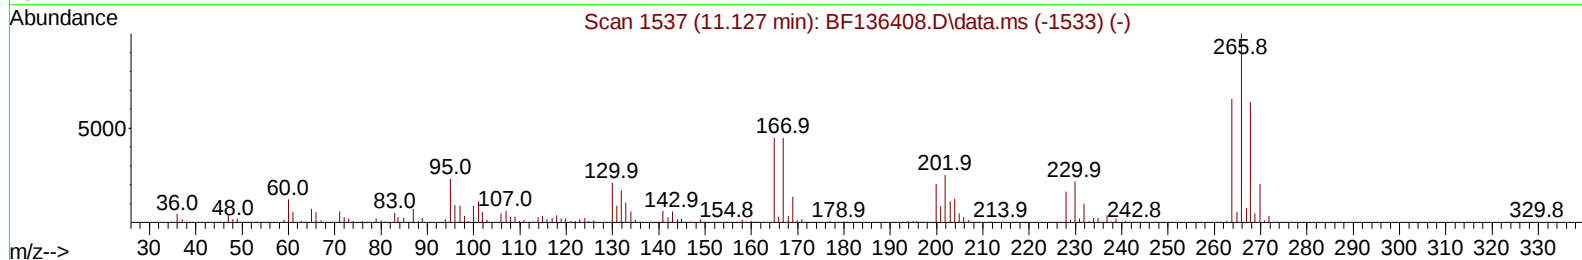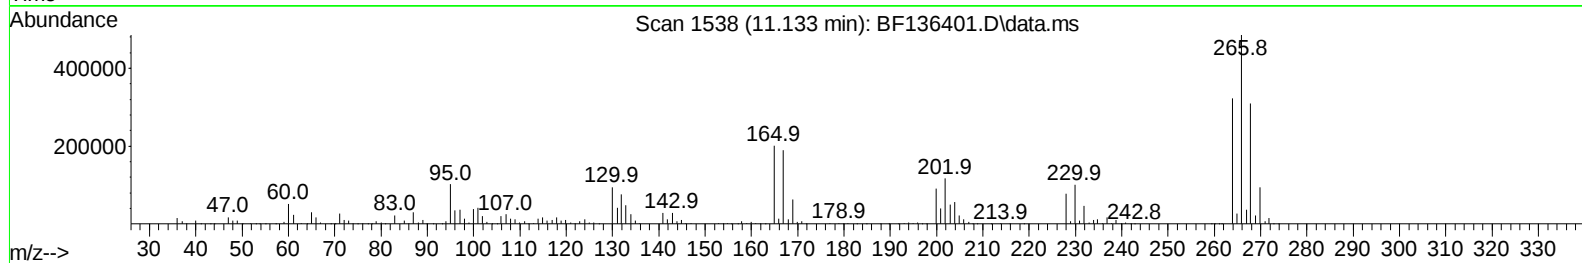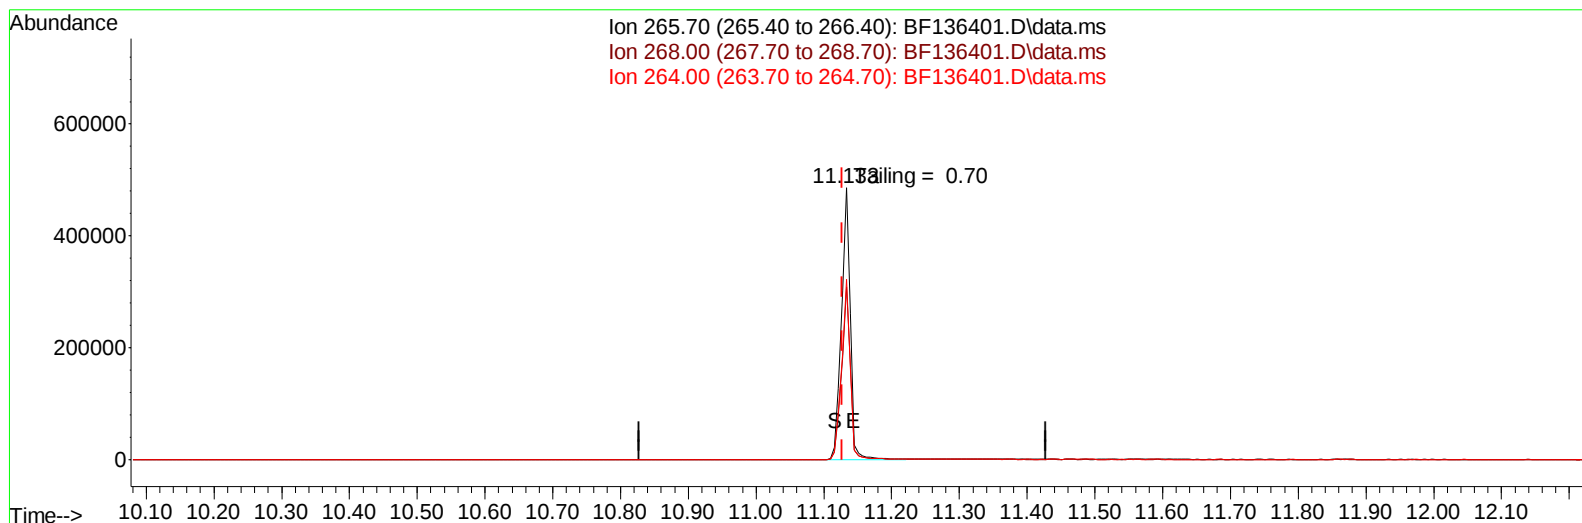

TIC: BF136401.D\data.ms

(70) Pentachlorophenol (C)

11.133min (+ 0.006) 45366.72 ng




response 446248

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.61
264.00	63.40	66.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120523\
Data File : BF136401.D
Acq On : 05 Dec 2023 12:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 05 17:41:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 05 17:37:37 2023
Response via : Initial Calibration

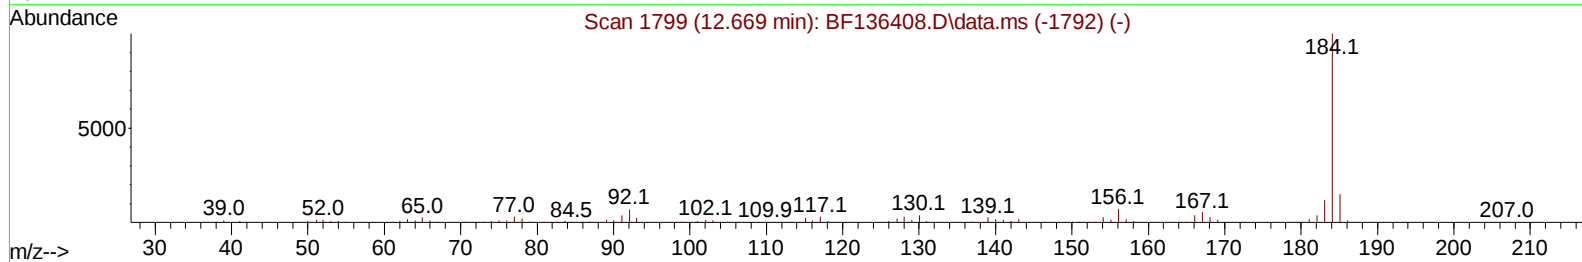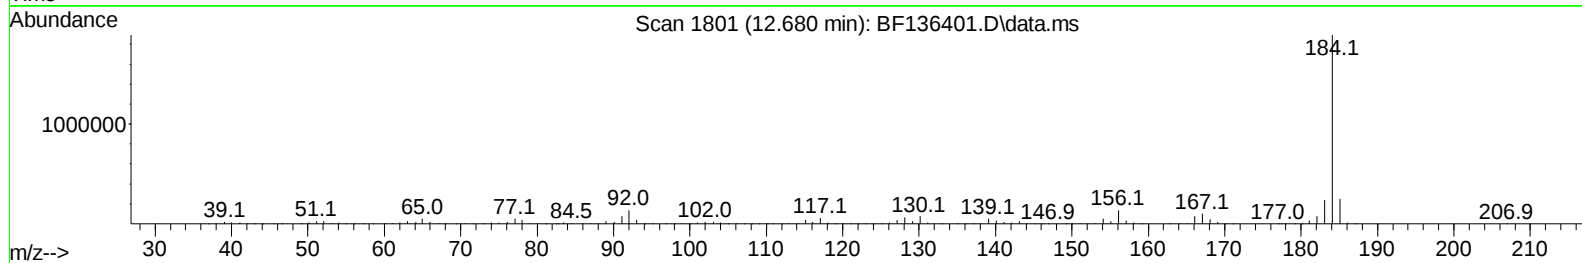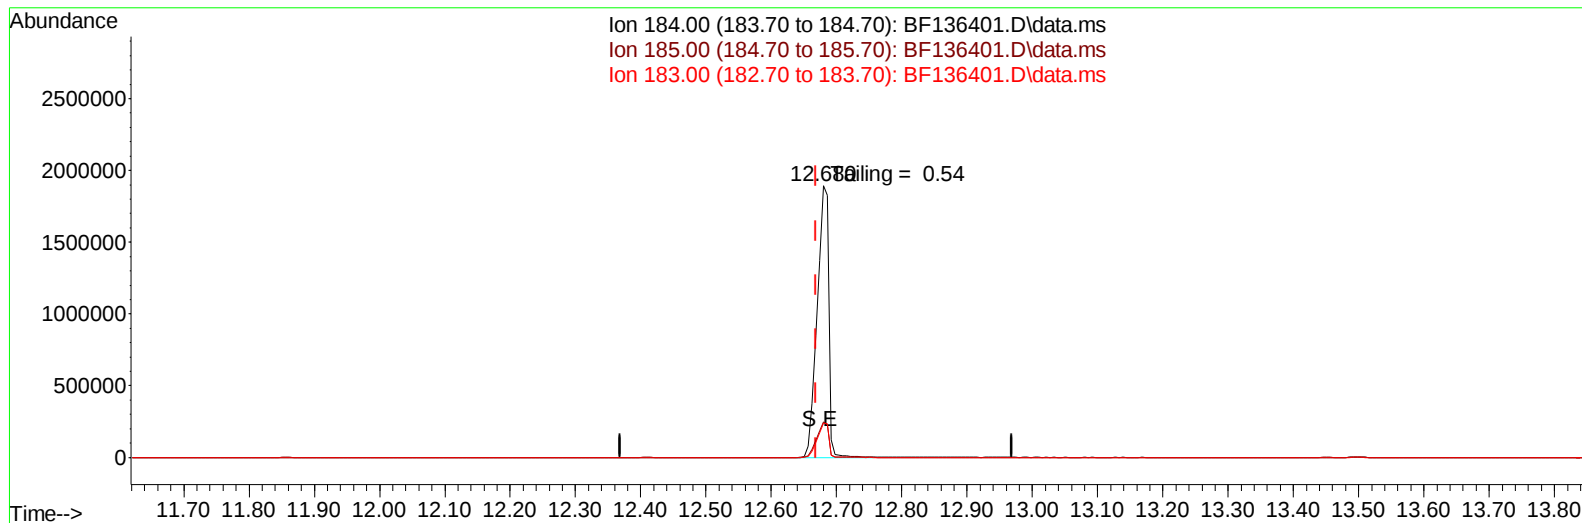

TIC: BF136401.D\data.ms

(77) Benzidine

12.680min (+ 0.011) 131568.41 ng

response 2347142

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.20
183.00	11.90	12.68
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/4/2023	BNA_F	<u>BF136401.D</u>
Compound Name	Response	Retention Time
DDT	1073744	13.504
DDD	13093	13.221
DDE	502	12.857
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13595	1087339	1.25

Instrument :
BNA_F
ClientSampleId :
DFTPP