
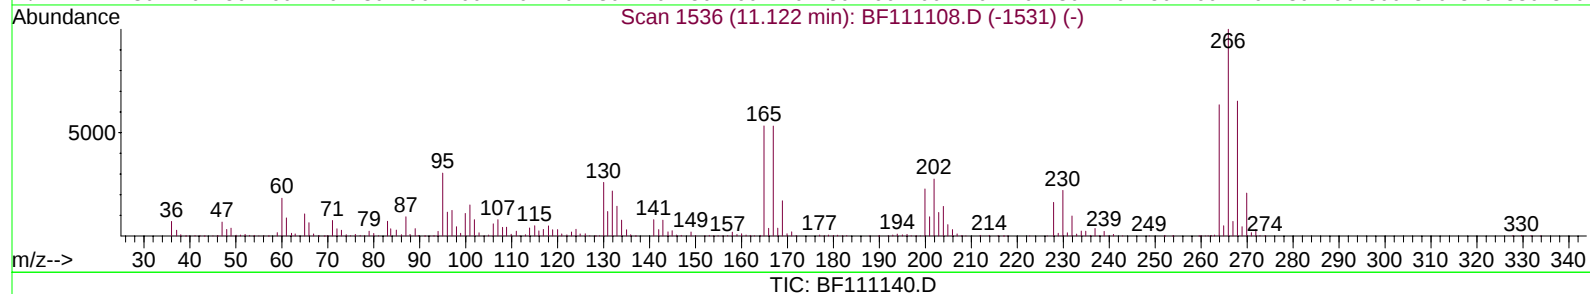
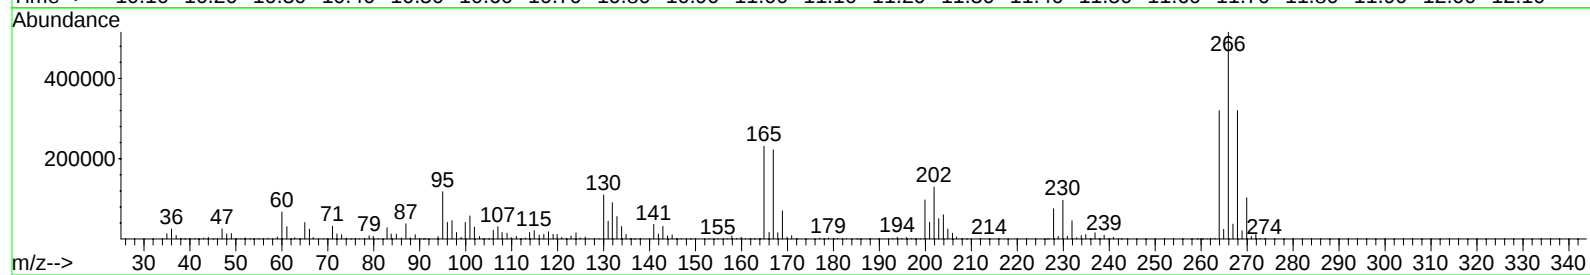


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF120618\
Data File : BF111140.D
Acq On : 6 Dec 2018 16:11
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 16:58:27 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF120518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 05 17:30:55 2018
Response via : Initial Calibration

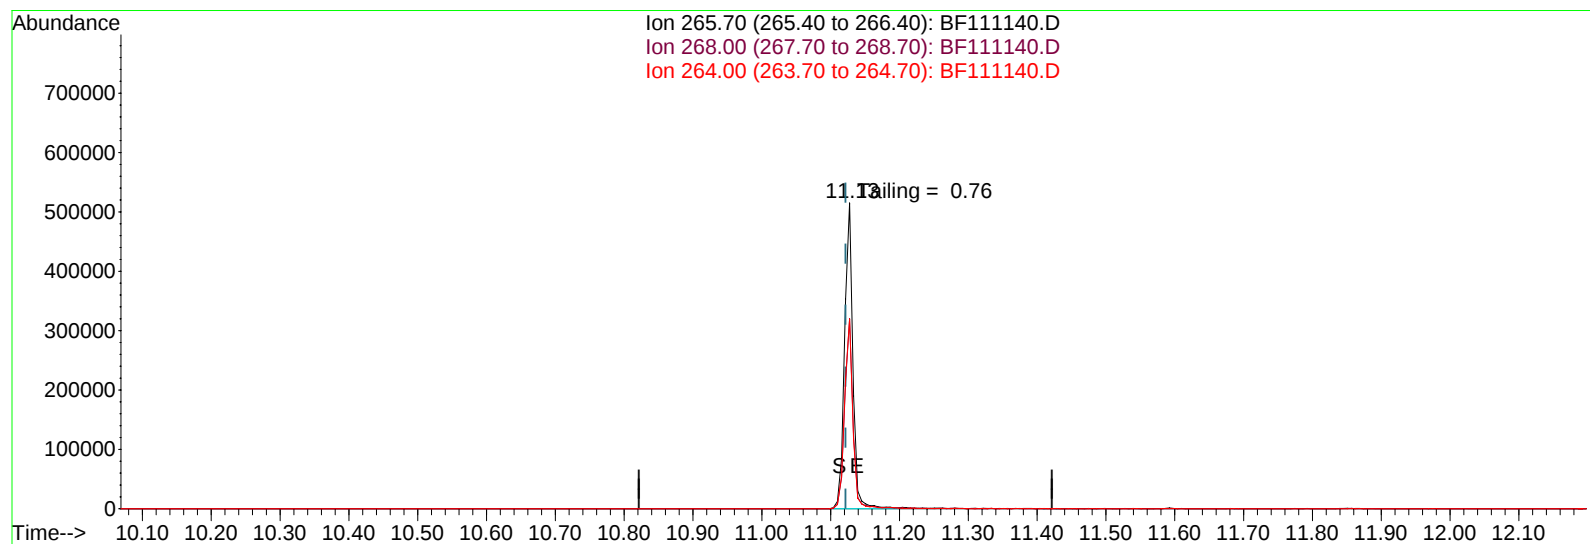

(70) Pentachlorophenol (C)




11.128min (+0.006) 106405.18ng

response 435502

Ion	Exp%	Act%
265.70	100	100
268.00	65.30	62.16
264.00	63.50	62.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF120618\
Data File : BF111140.D
Acq On : 6 Dec 2018 16:11
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 16:58:27 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF120518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 05 17:30:55 2018
Response via : Initial Calibration

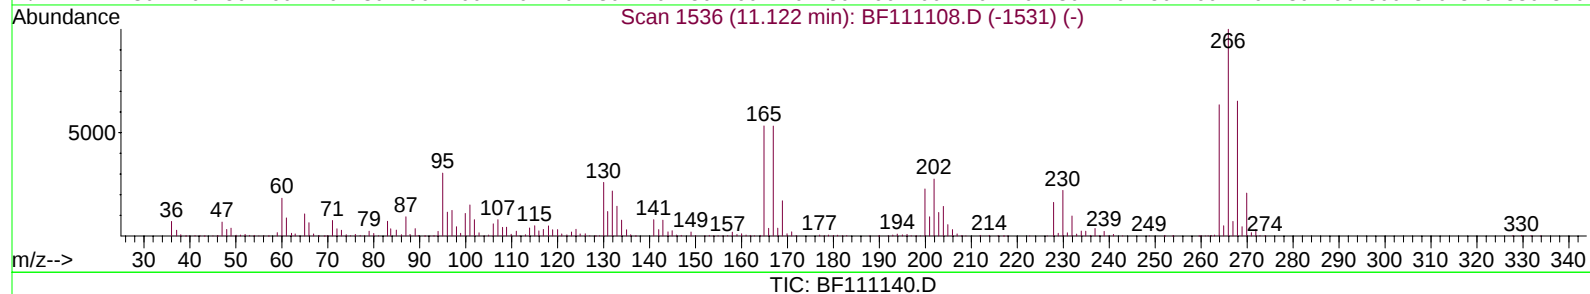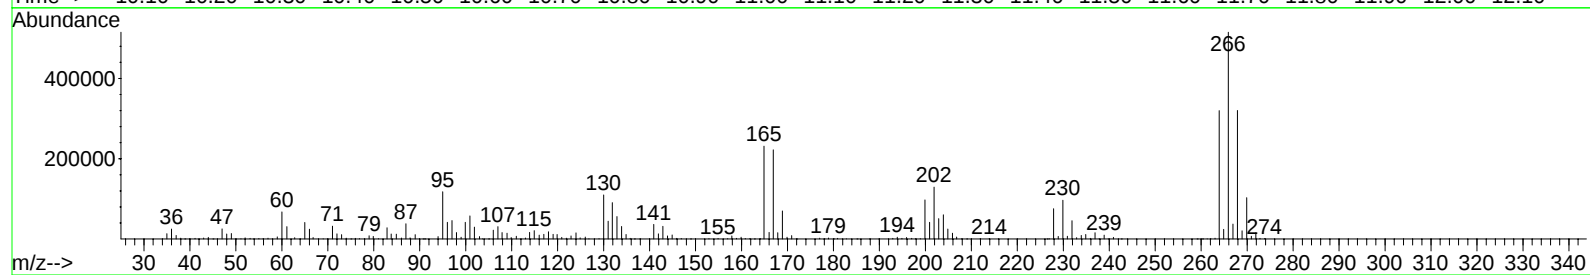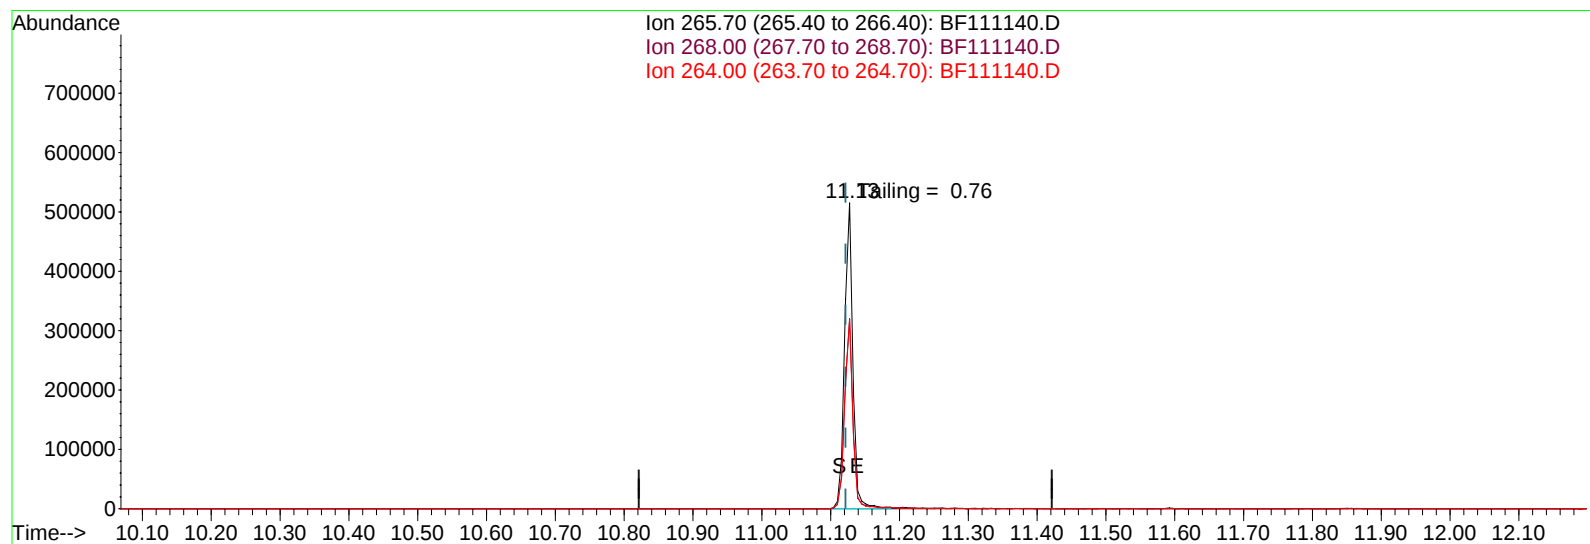

(70) Pentachlorophenol (C)

11.128min (+0.006) 106405.18ng

response 435502

Ion	Exp%	Act%
265.70	100	100
268.00	65.30	62.16
264.00	63.50	62.07
0.00	0.00	0.00