

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF120618\
 Data File : BF111175.D
 Acq On : 7 Dec 2018 9:04
 Operator : JU/SJ
 Sample : J6219-10
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 NM-342-135-120418-DEBRI

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.375	45	49	55	rVB	85593	115147	1.97%	0.145%
2	5.010	489	497	504	rVB	268369	329607	5.64%	0.416%
3	5.422	562	567	570	rBV	6174272	5663263	96.96%	7.152%
4	6.434	734	739	742	rBV	6298169	5840820	100.00%	7.376%
5	6.575	759	763	766	rBV	6776181	5722728	97.98%	7.227%
6	6.634	770	773	780	rVV	233203	194793	3.34%	0.246%
7	6.810	799	803	806	rBV	2461995	2259800	38.69%	2.854%
8	6.963	825	829	833	rVB	5339723	4475815	76.63%	5.652%
9	7.363	892	897	900	rBV	4289800	3538781	60.59%	4.469%
10	7.622	937	941	944	rVB	172524	140712	2.41%	0.178%
11	7.869	979	983	986	rBV	593096	457264	7.83%	0.577%
12	8.086	1016	1020	1024	rBV	3261198	2717136	46.52%	3.431%
13	8.545	1096	1098	1102	rVB2	88725	74922	1.28%	0.095%
14	8.716	1123	1127	1131	rVB	81740	74105	1.27%	0.094%
15	8.992	1169	1174	1178	rBV	68550	70908	1.21%	0.090%
16	9.163	1199	1203	1207	rBV	6636376	5659678	96.90%	7.147%
17	9.733	1292	1300	1306	rBV	391333	382896	6.56%	0.484%
18	9.786	1306	1309	1311	rVB	90932	75145	1.29%	0.095%
19	9.839	1314	1318	1322	rVB	2578286	2495720	42.73%	3.152%
20	9.933	1331	1334	1336	rBV	483288	355407	6.08%	0.449%
21	9.963	1336	1339	1342	rVV	313064	293519	5.03%	0.371%
22	10.016	1345	1348	1351	rBV2	93515	100553	1.72%	0.127%
23	10.057	1351	1355	1363	rBV	1781006	1853237	31.73%	2.340%
24	10.122	1363	1366	1368	rVB	68138	72602	1.24%	0.092%
25	10.557	1437	1440	1445	rBV2	74149	70648	1.21%	0.089%
26	10.622	1448	1451	1455	rBV	2572228	2417939	41.40%	3.053%
27	10.769	1470	1476	1481	rBV	678530	667510	11.43%	0.843%
28	10.910	1496	1500	1504	rBV2	107412	120841	2.07%	0.153%
29	10.969	1507	1510	1512	rVV	546372	451456	7.73%	0.570%
30	10.992	1512	1514	1520	rVV2	381431	459625	7.87%	0.580%
31	11.051	1522	1524	1529	rVB	108054	121634	2.08%	0.154%
32	11.175	1542	1545	1547	rBV3	84387	73556	1.26%	0.093%
33	11.204	1547	1550	1553	rVB	87723	76098	1.30%	0.096%
34	11.280	1560	1563	1566	rBV3	118339	102785	1.76%	0.130%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF120618\
 Data File : BF111175.D
 Acq On : 7 Dec 2018 9:04
 Operator : JU/SJ
 Sample : J6219-10
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 NM-342-135-120418-DEBRI

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	11.322	1566	1570	1574	rBV	2298565	2011934	34.45%	2.541%
36	11.633	1616	1623	1628	rBV	76382	101374	1.74%	0.128%
37	11.698	1630	1634	1636	rBV	621507	594207	10.17%	0.750%
38	11.727	1636	1639	1645	rVB2	105799	150461	2.58%	0.190%
39	11.780	1645	1648	1652	rBV3	137007	176490	3.02%	0.223%
40	11.822	1652	1655	1657	rVV	137624	106535	1.82%	0.135%
41	11.857	1657	1661	1665	rVV2	1678912	2119873	36.29%	2.677%
42	11.892	1665	1667	1671	rVV	1423313	1149798	19.69%	1.452%
43	11.939	1671	1675	1677	rVV2	134104	146746	2.51%	0.185%
44	11.969	1677	1680	1683	rVV2	89696	91945	1.57%	0.116%
45	12.133	1706	1708	1713	rVB	73172	67638	1.16%	0.085%
46	12.427	1755	1758	1761	rVB	95848	78014	1.34%	0.099%
47	12.527	1772	1775	1777	rBV	475729	527687	9.03%	0.666%
48	12.545	1777	1778	1780	rVV	326045	292407	5.01%	0.369%
49	12.645	1791	1795	1799	rBV	1467401	1407077	24.09%	1.777%
50	12.686	1799	1802	1805	rVV	550875	646150	11.06%	0.816%
51	12.739	1808	1811	1814	rVV2	345101	353281	6.05%	0.446%
52	12.769	1814	1816	1819	rVV3	84918	94391	1.62%	0.119%
53	12.816	1819	1824	1828	rVB	835603	899272	15.40%	1.136%
54	12.910	1836	1840	1843	rBV	5180950	4284695	73.36%	5.411%
55	13.027	1858	1860	1864	rBV3	60717	69546	1.19%	0.088%
56	13.157	1879	1882	1884	rBV	152827	131437	2.25%	0.166%
57	13.286	1901	1904	1906	rBV	305316	284113	4.86%	0.359%
58	13.380	1916	1920	1921	rBV2	491070	492168	8.43%	0.622%
59	13.392	1921	1922	1925	rVV2	375890	343624	5.88%	0.434%
60	13.427	1925	1928	1930	rVV	392876	396257	6.78%	0.500%
61	13.451	1930	1932	1934	rVV	272454	310130	5.31%	0.392%
62	13.469	1934	1935	1938	rVV	325076	290839	4.98%	0.367%
63	13.498	1938	1940	1941	rVV	325111	260152	4.45%	0.329%
64	13.516	1941	1943	1945	rVV	420073	349420	5.98%	0.441%
65	13.539	1945	1947	1949	rVB	93867	81529	1.40%	0.103%
66	13.827	1992	1996	1999	rBV	399280	393711	6.74%	0.497%
67	13.957	2014	2018	2021	rBV	2106747	1891154	32.38%	2.388%
68	13.980	2021	2022	2025	rVV	182525	158428	2.71%	0.200%
69	14.004	2025	2026	2031	rVB2	85406	95615	1.64%	0.121%
70	14.080	2037	2039	2041	rBV2	90455	76058	1.30%	0.096%
71	14.110	2041	2044	2046	rBV	240873	206564	3.54%	0.261%

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF120618\
Data File : BF111175.D
Acq On : 7 Dec 2018 9:04
Operator : JU/SJ
Sample : J6219-10
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
NM-342-135-120418-DEBRI

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120518.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	14.139	2046	2049	2054	rVB	540677	573241	9.81%	0.724%
73	14.186	2054	2057	2059	rBV2	96746	126017	2.16%	0.159%
74	14.445	2098	2101	2110	rVB	581393	585038	10.02%	0.739%
75	14.598	2125	2127	2129	rBV3	78775	68857	1.18%	0.087%
76	14.721	2145	2148	2149	rBV2	101061	106989	1.83%	0.135%
77	14.751	2149	2153	2155	rVV	524196	542640	9.29%	0.685%
78	14.821	2162	2165	2169	rBV	1354917	1301170	22.28%	1.643%
79	15.080	2205	2209	2213	rBV	593914	646707	11.07%	0.817%
80	15.398	2258	2263	2267	rVB	1047200	1215051	20.80%	1.534%
81	15.451	2269	2272	2275	rBV	285308	322889	5.53%	0.408%
82	15.880	2341	2345	2348	rBV	235572	331056	5.67%	0.418%
83	16.345	2419	2424	2433	rBV4	374052	715629	12.25%	0.904%
84	17.421	2602	2607	2615	rVB5	290566	641997	10.99%	0.811%
85	17.651	2638	2646	2656	rVB2	1304367	3353573	57.42%	4.235%


Sum of corrected areas: 79188224

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF120618\
Data File : BF111175.D
Acq On : 7 Dec 2018 9:04
Operator : JU/SJ
Sample : J6219-10
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
NM-342-135-120418-DEBRI

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF120518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

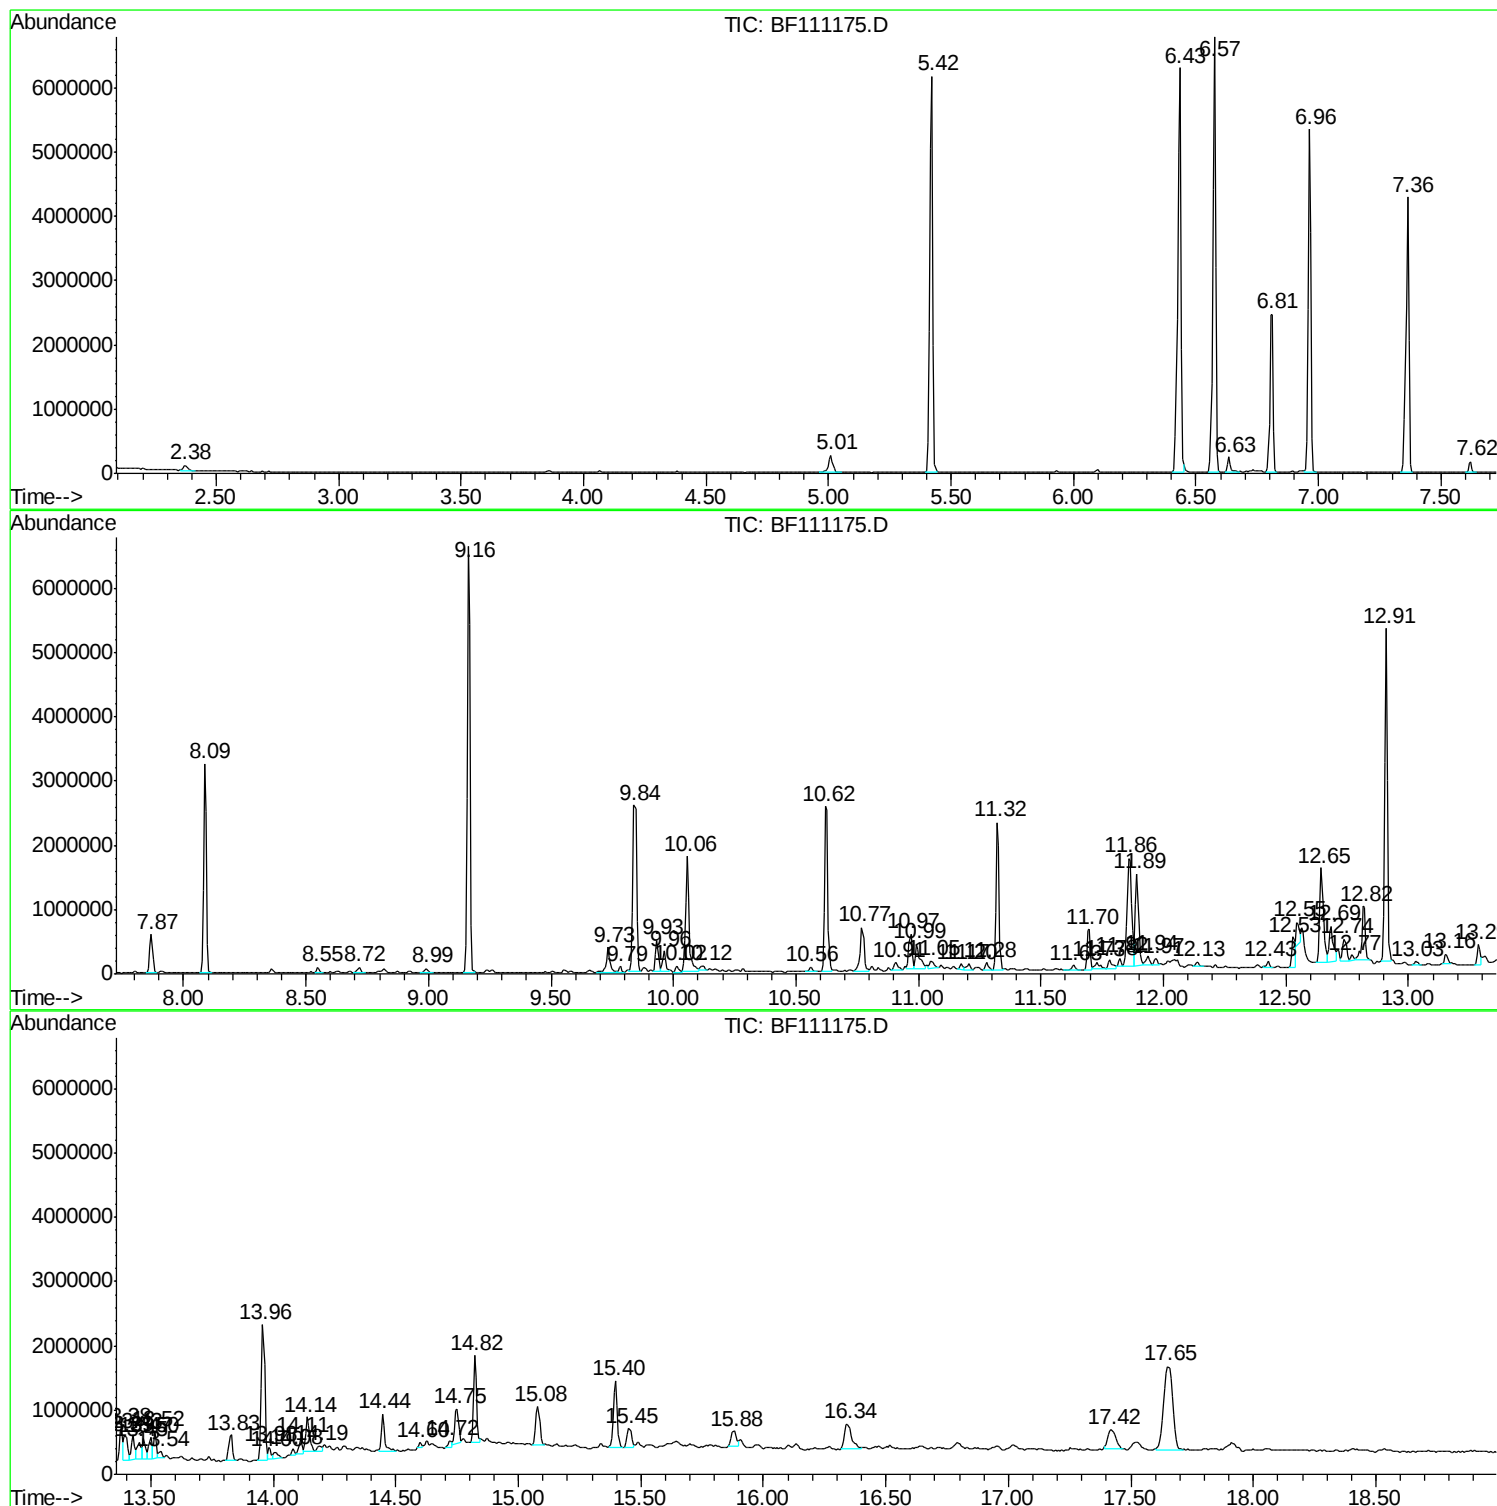

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF120618\
Data_File : BF111175.D
Acq_On : 7 Dec 2018 9:044
Operator : JU/SJJ
Sample : J6219-100
Misc :
ALS_Vial : 34 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
NM-342-135-120418-DEBRI

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120518.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
