


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120618\
 Data File : BF111140.D
 Acq On : 6 Dec 2018 16:11
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 05 17:30:55 2018

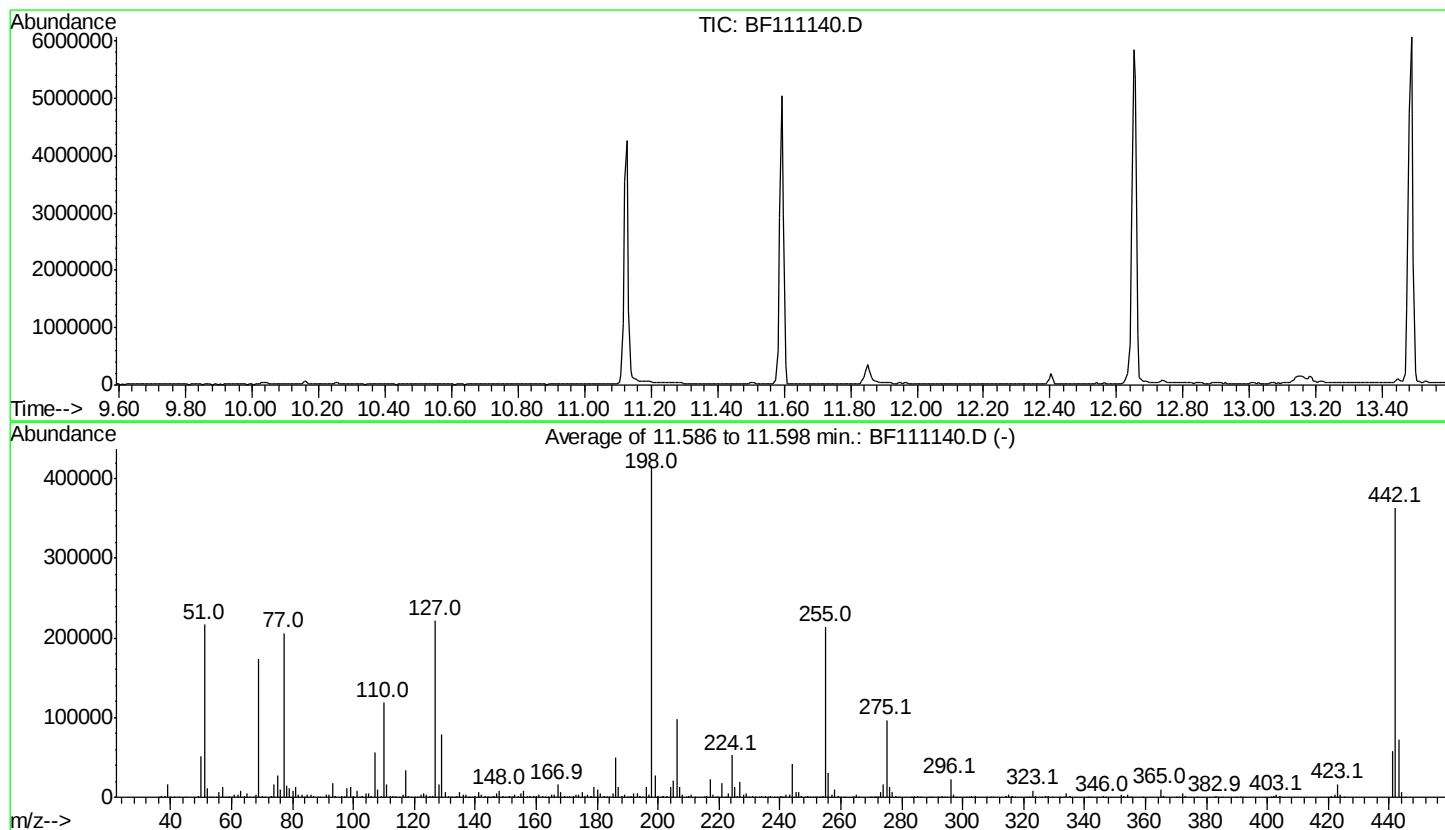

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.0	216410	PASS
68	69	0.00	2	1.5	2655	PASS
69	198	0.00	100	41.5	172724	PASS
70	69	0.00	2	0.6	1097	PASS
127	198	10	80	53.2	221312	PASS
197	198	0.00	2	0.7	2974	PASS
198	198	100	100	100.0	416064	PASS
199	198	5	9	6.6	27426	PASS
275	198	10	60	23.3	96808	PASS
365	198	1	100	2.4	9849	PASS
441	198	0.01	100	13.9	57986	PASS
442	198	50	100	87.4	363562	PASS
443	442	15	24	19.9	72344	PASS