


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120618\
 Data File : BF111167.D
 Acq On : 7 Dec 2018 5:28
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 05 17:30:55 2018

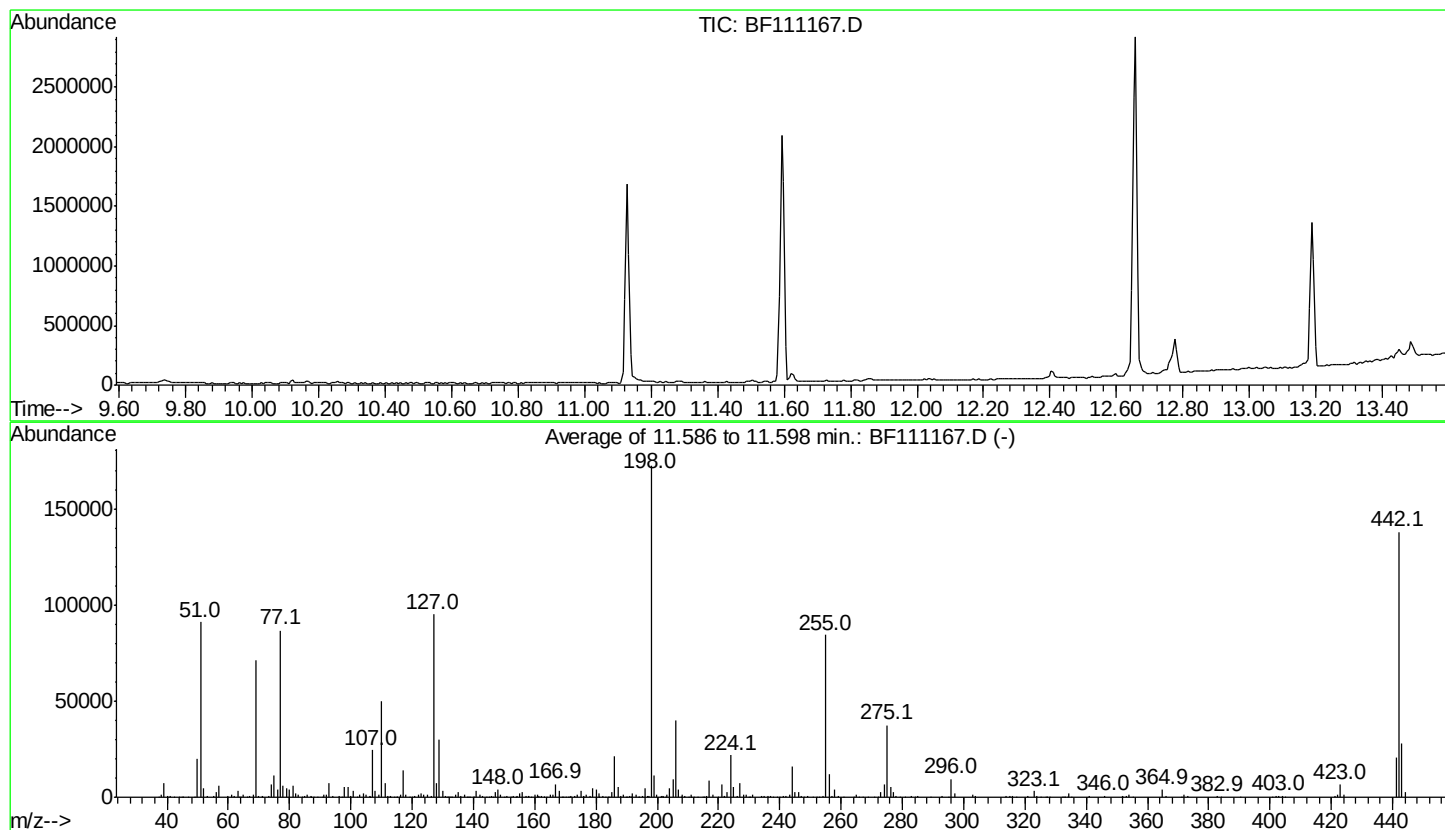

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1611

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.7	90882	PASS
68	69	0.00	2	1.8	1309	PASS
69	198	0.00	100	41.3	71176	PASS
70	69	0.00	2	0.8	589	PASS
127	198	10	80	55.1	94930	PASS
197	198	0.00	2	0.5	901	PASS
198	198	100	100	100.0	172357	PASS
199	198	5	9	6.5	11196	PASS
275	198	10	60	21.7	37423	PASS
365	198	1	100	2.2	3851	PASS
441	198	0.01	100	11.9	20583	PASS
442	198	50	100	80.0	137866	PASS
443	442	15	24	20.3	27939	PASS