
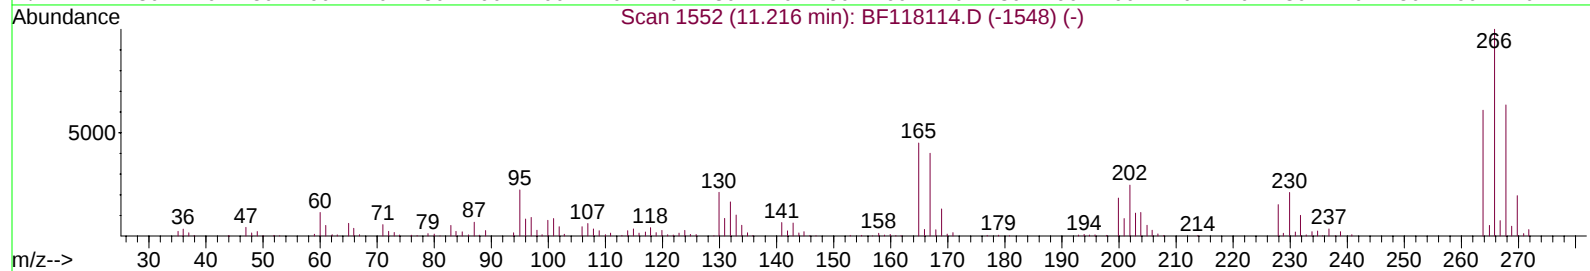
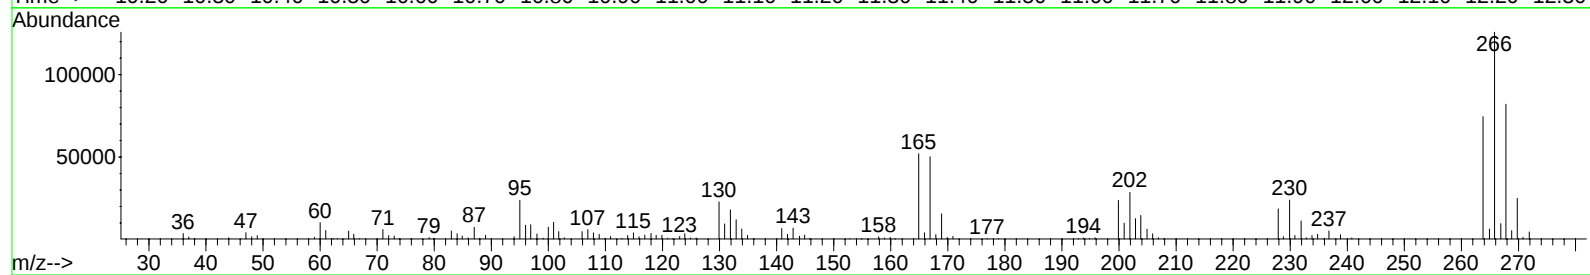


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF120619\
Data File : BF118111.D
Acq On : 6 Dec 2019 13:32
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 16:49:59 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF120619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 15:39:13 2019
Response via : Initial Calibration

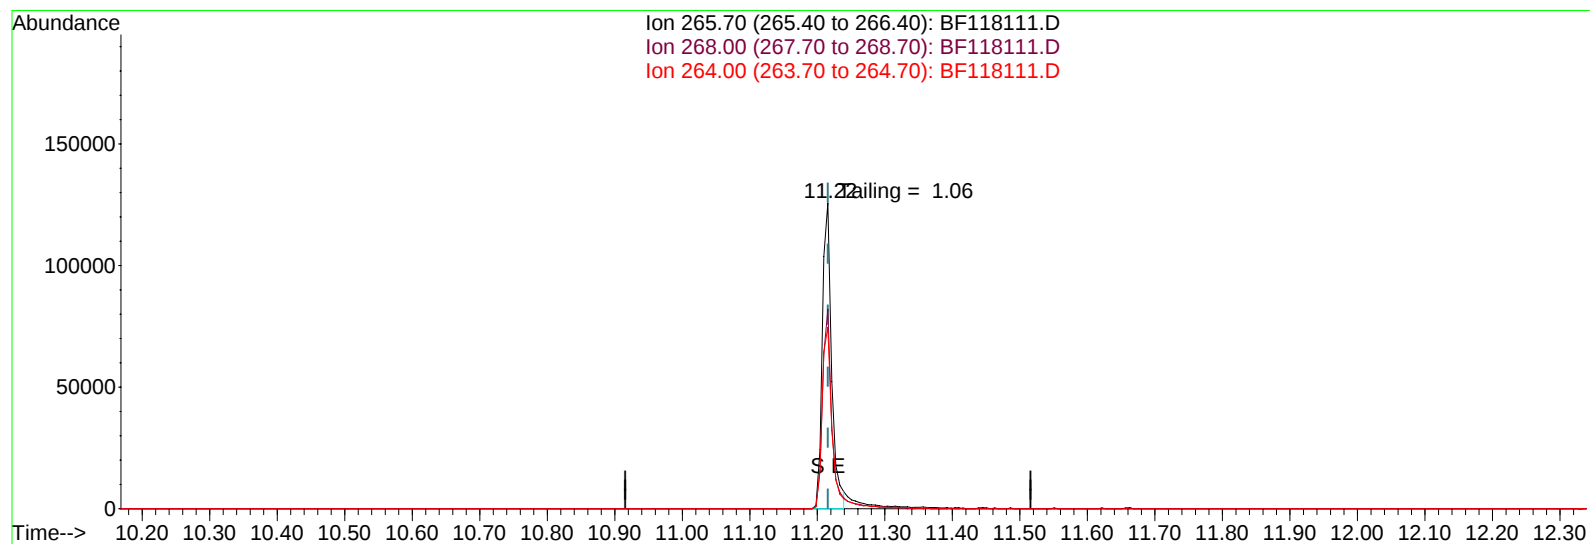

TIC: BF118111.D

(70) Pentachlorophenol (C)




11.216min (-0.000) 43501.82ng

response 131102

Ion	Exp%	Act%
265.70	100	100
268.00	63.40	65.24
264.00	60.90	59.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF120619\
Data File : BF118111.D
Acq On : 6 Dec 2019 13:32
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 16:49:59 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF120619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 15:39:13 2019
Response via : Initial Calibration

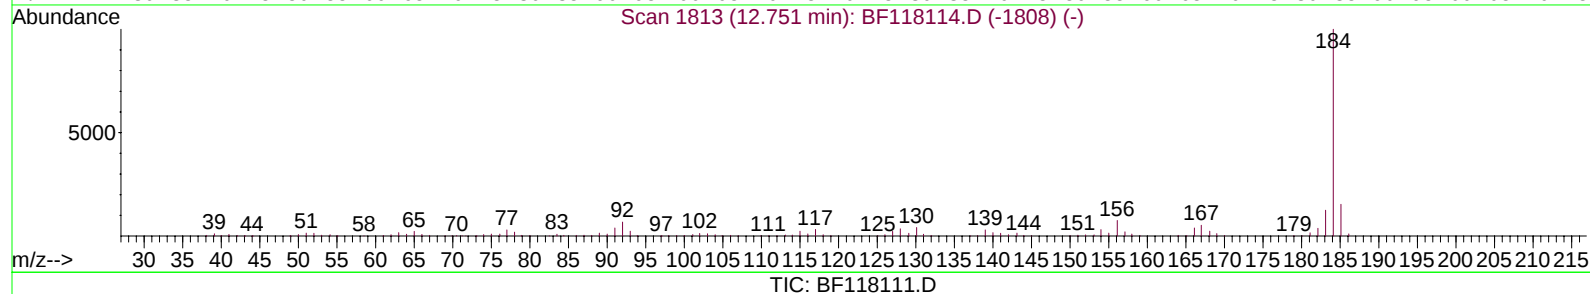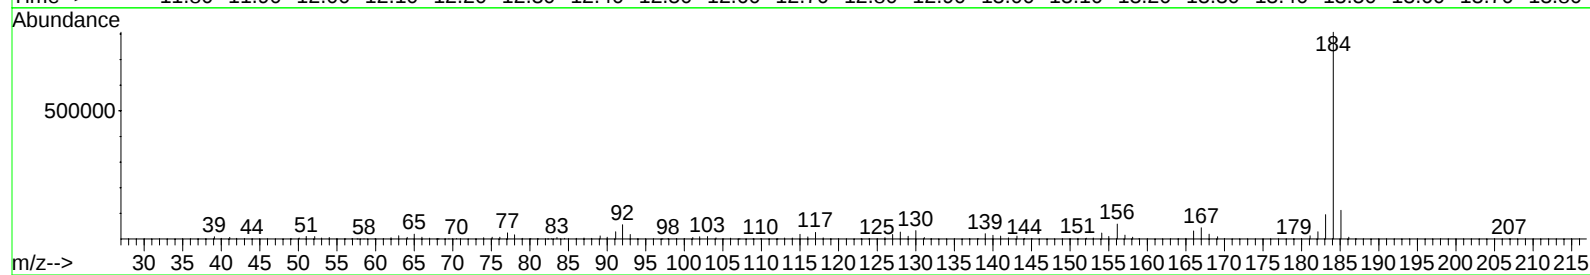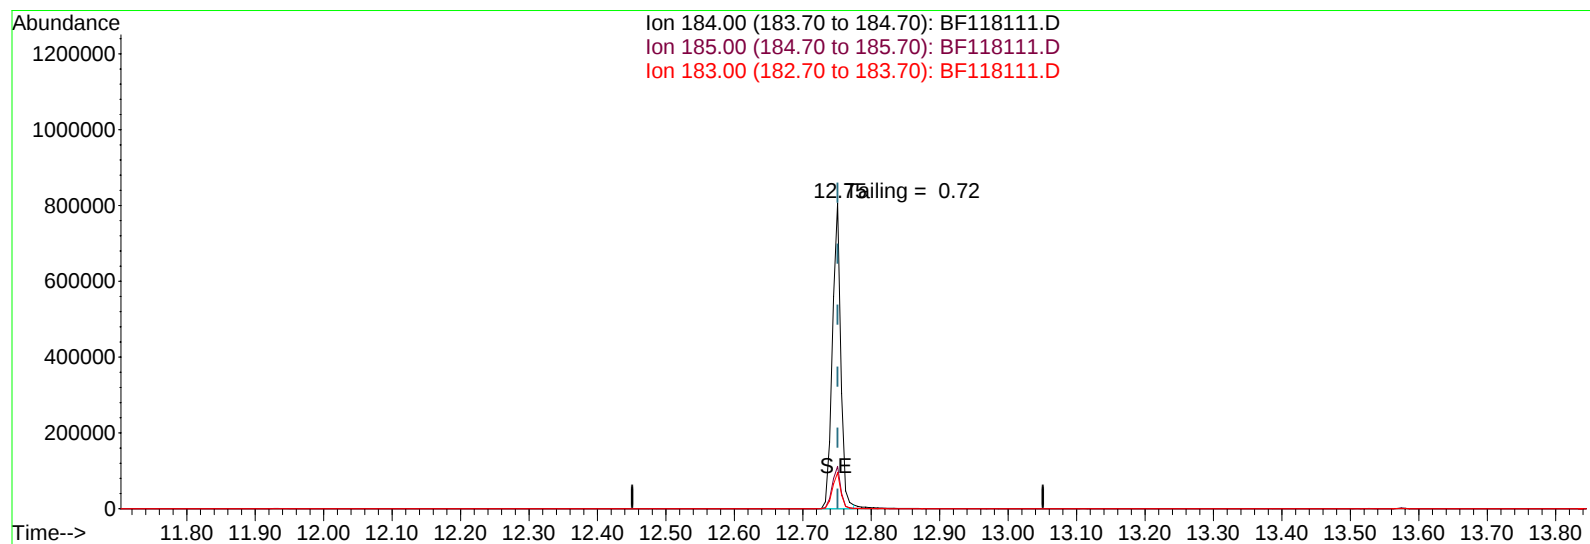

(77) Benzidine

12.751min (-0.000) 0.00ng

response 695139

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	13.87
183.00	12.40	11.78
0.00	0.00	0.00