


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF120619\
 Data File : BF118111.D
 Acq On : 6 Dec 2019 13:32
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 06 17:34:43 2019

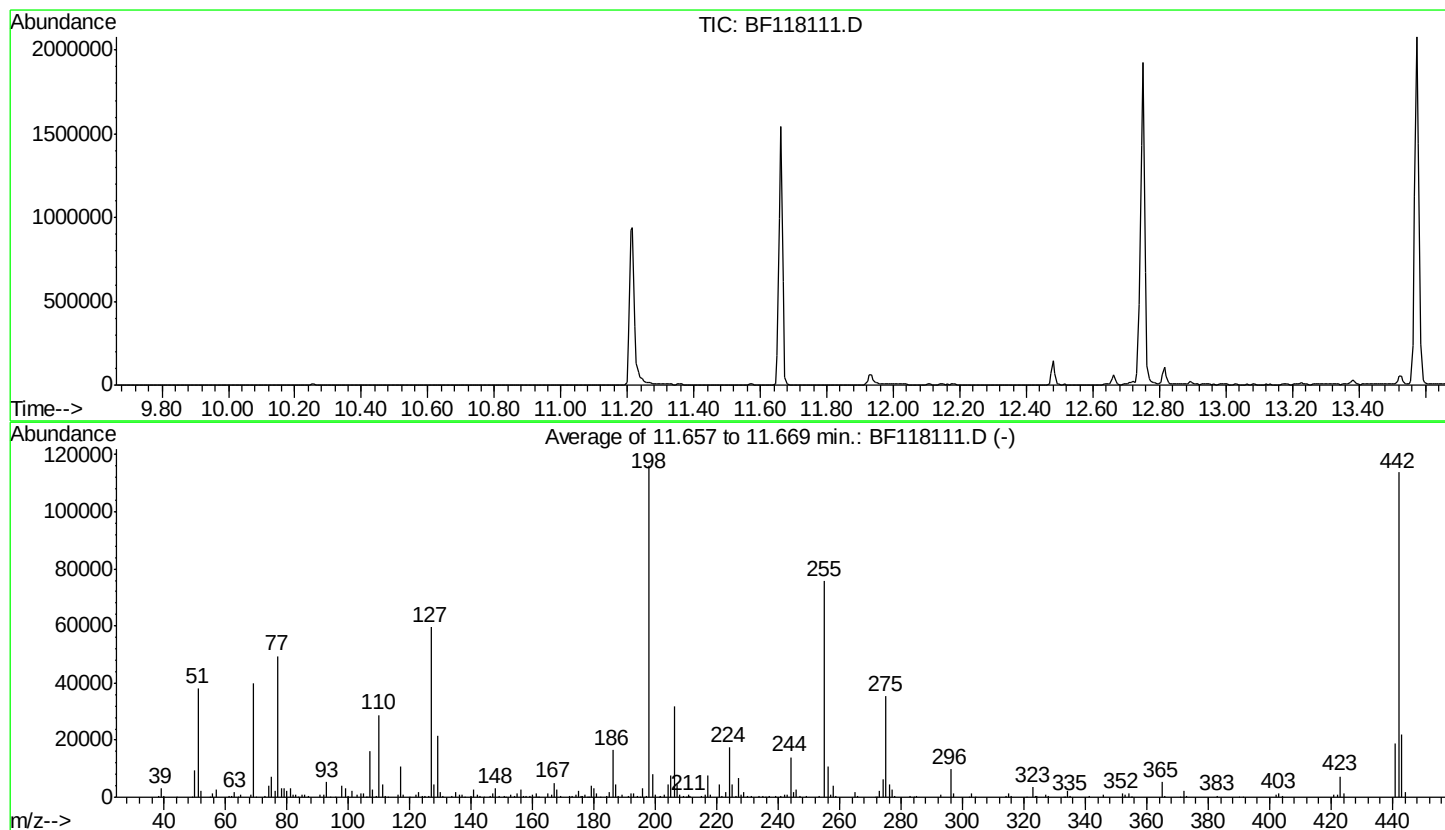

AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.8	38046	PASS
68	69	0.00	2	1.9	778	PASS
69	198	0.00	100	34.5	40031	PASS
70	69	0.00	2	0.3	108	PASS
127	198	10	80	51.2	59482	PASS
197	198	0.00	2	0.5	570	PASS
198	198	100	100	100.0	116144	PASS
199	198	5	9	7.0	8128	PASS
275	198	10	60	30.3	35216	PASS
365	198	1	100	4.6	5355	PASS
441	198	0.01	100	16.3	18910	PASS
442	198	50	100	98.1	113994	PASS
443	442	15	24	19.4	22101	PASS