

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120623\
 Data File : BF136420.D
 Acq On : 06 Dec 2023 10:37
 Operator : CG\JU
 Sample : PB157498BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB157498BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136420.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.075	504	508	513	rBV	45653	61509	1.17%	0.223%
2	5.451	566	572	575	rBV	3223739	3389194	64.67%	12.272%
3	6.439	734	740	743	rBV	2985545	3309420	63.14%	11.983%
4	6.798	797	801	804	rBV	925769	717012	13.68%	2.596%
5	7.363	890	897	900	rBV	2115366	2220974	42.38%	8.042%
6	8.075	1013	1018	1022	rBV	1110934	996423	19.01%	3.608%
7	9.157	1195	1202	1205	rBV	4953181	4583177	87.45%	16.595%
8	9.833	1310	1317	1320	rBV	1437389	1178645	22.49%	4.268%
9	10.627	1445	1452	1455	rBV	3072108	2740626	52.29%	9.923%
10	11.321	1566	1570	1573	rBV	1598898	1260501	24.05%	4.564%
11	12.921	1837	1842	1845	rBV	4974865	5241101	100.00%	18.977%
12	13.974	2017	2021	2024	rBV	1180480	1042507	19.89%	3.775%
13	15.451	2267	2272	2279	rBV	654212	808969	15.44%	2.929%
14	17.256	2569	2579	2581	rBV9	25390	67800	1.29%	0.245%




Sum of corrected areas: 27617858

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120623\
Data File : BF136420.D
Acq On : 06 Dec 2023 10:37
Operator : CG\JU
Sample : PB157498BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157498BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

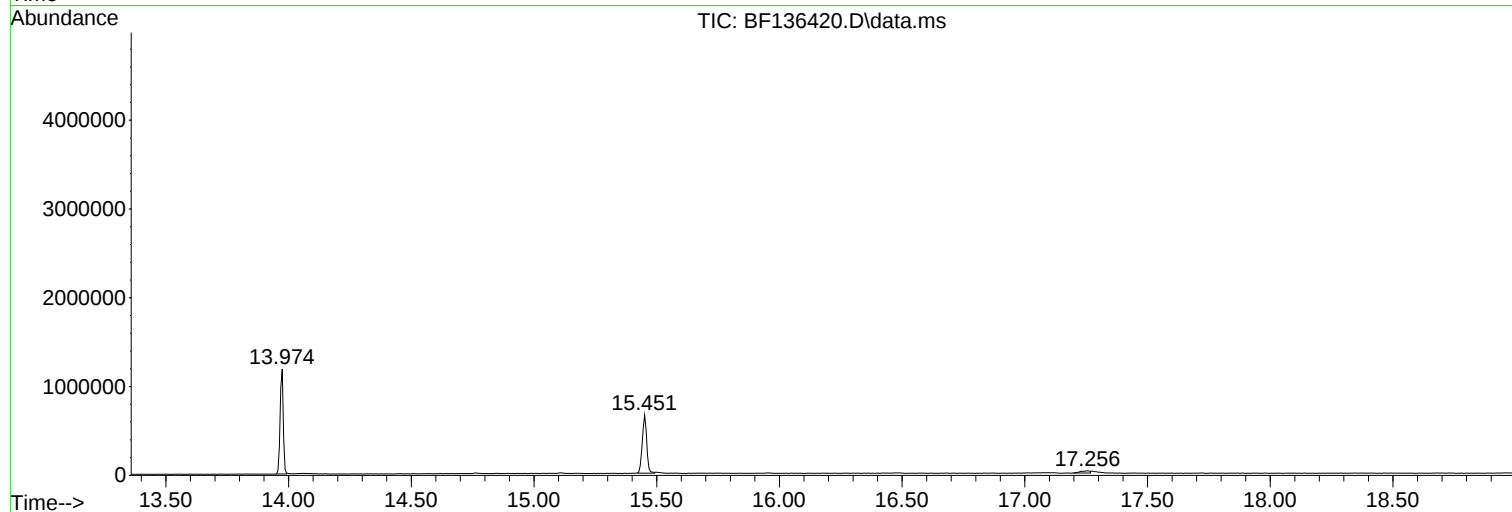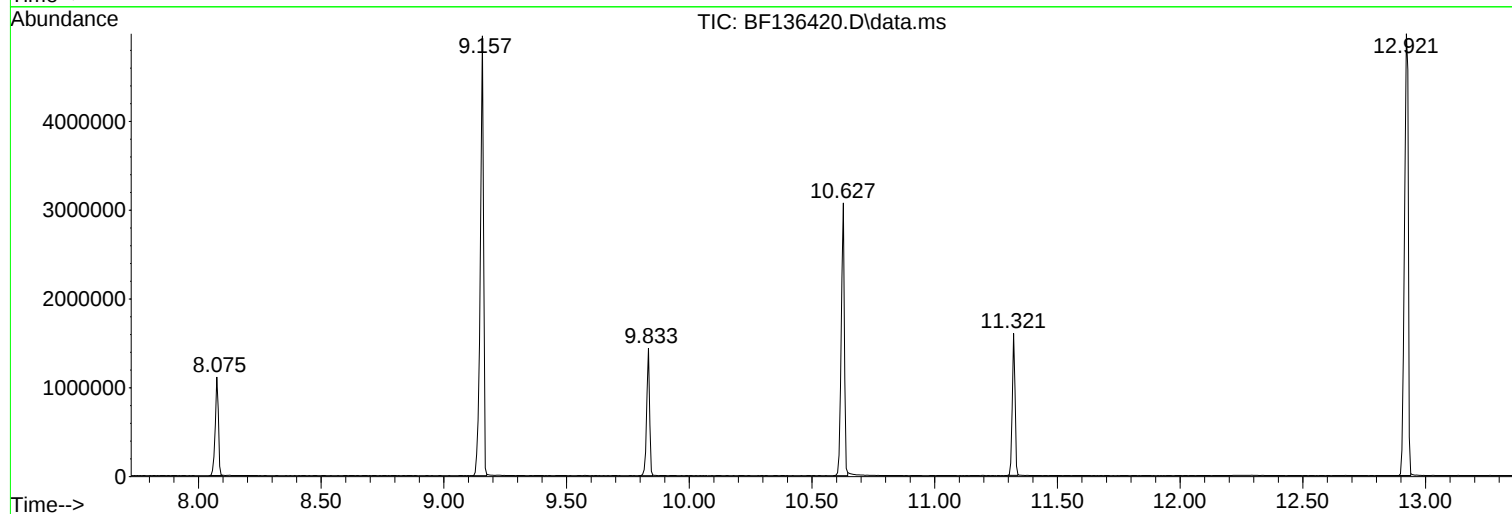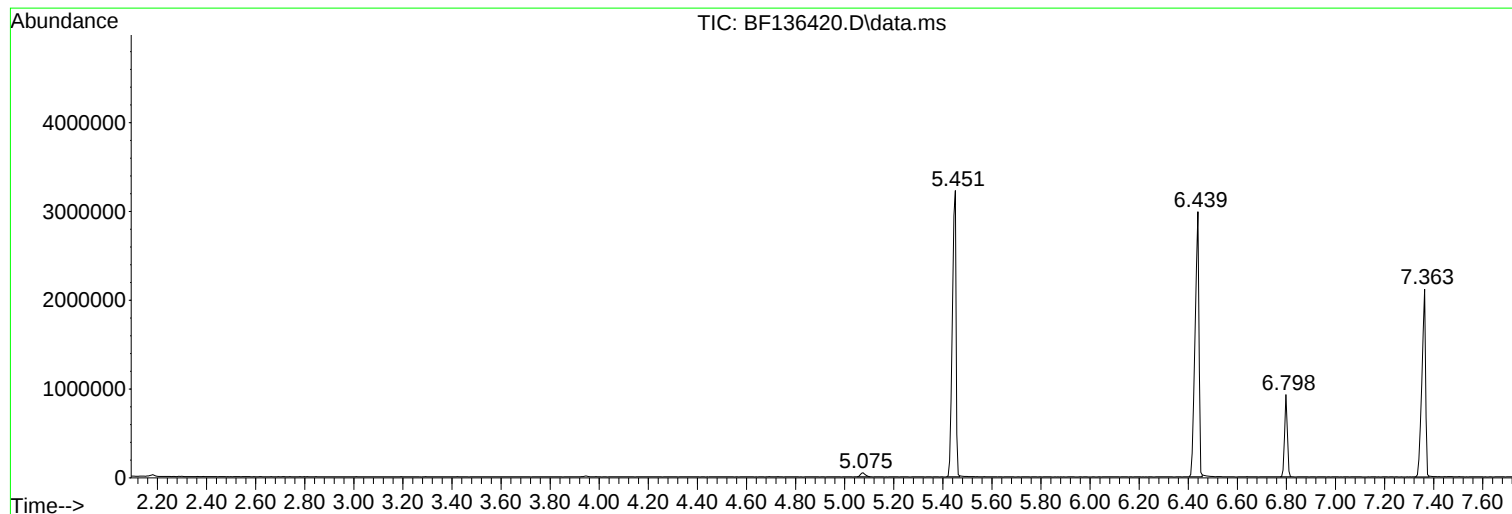

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120623\
Data File : BF136420.D
Acq On : 06 Dec 2023 10:37
Operator : CG\JU
Sample : PB157498BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157498BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120623\
Data File : BF136420.D
Acq On : 06 Dec 2023 10:37
Operator : CG\JU
Sample : PB157498BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157498BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------