

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120723\
 Data File : BF136452.D
 Acq On : 07 Dec 2023 17:57
 Operator : CG\JU
 Sample : 05599-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 LKWD-BACKFILL-02

Quant Time: Dec 08 00:41:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 06 09:40:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.798	152	99805	20.000	ng	0.00
21) Naphthalene-d8	8.075	136	355749	20.000	ng	0.00
39) Acenaphthene-d10	9.834	164	138794	20.000	ng	0.00
64) Phenanthrene-d10	11.322	188	229837	20.000	ng	0.00
76) Chrysene-d12	13.974	240	224192	20.000	ng	# 0.00
86) Perylene-d12	15.457	264	182211	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.446	112	561564	83.095	ng	0.01
7) Phenol-d6	6.446	99	733884	87.038	ng	0.00
23) Nitrobenzene-d5	7.363	82	475652	72.281	ng	0.00
42) 2,4,6-Tribromophenol	10.628	330	119148	69.623	ng	0.00
45) 2-Fluorobiphenyl	9.157	172	848551	83.422	ng	0.00
79) Terphenyl-d14	12.922	244	884230	51.985	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120723\
Data File : BF136452.D
Acq On : 07 Dec 2023 17:57
Operator : CG\JU
Sample : 05599-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LKWD-BACKFILL-02

Quant Time: Dec 08 00:41:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 06 09:40:27 2023
Response via : Initial Calibration




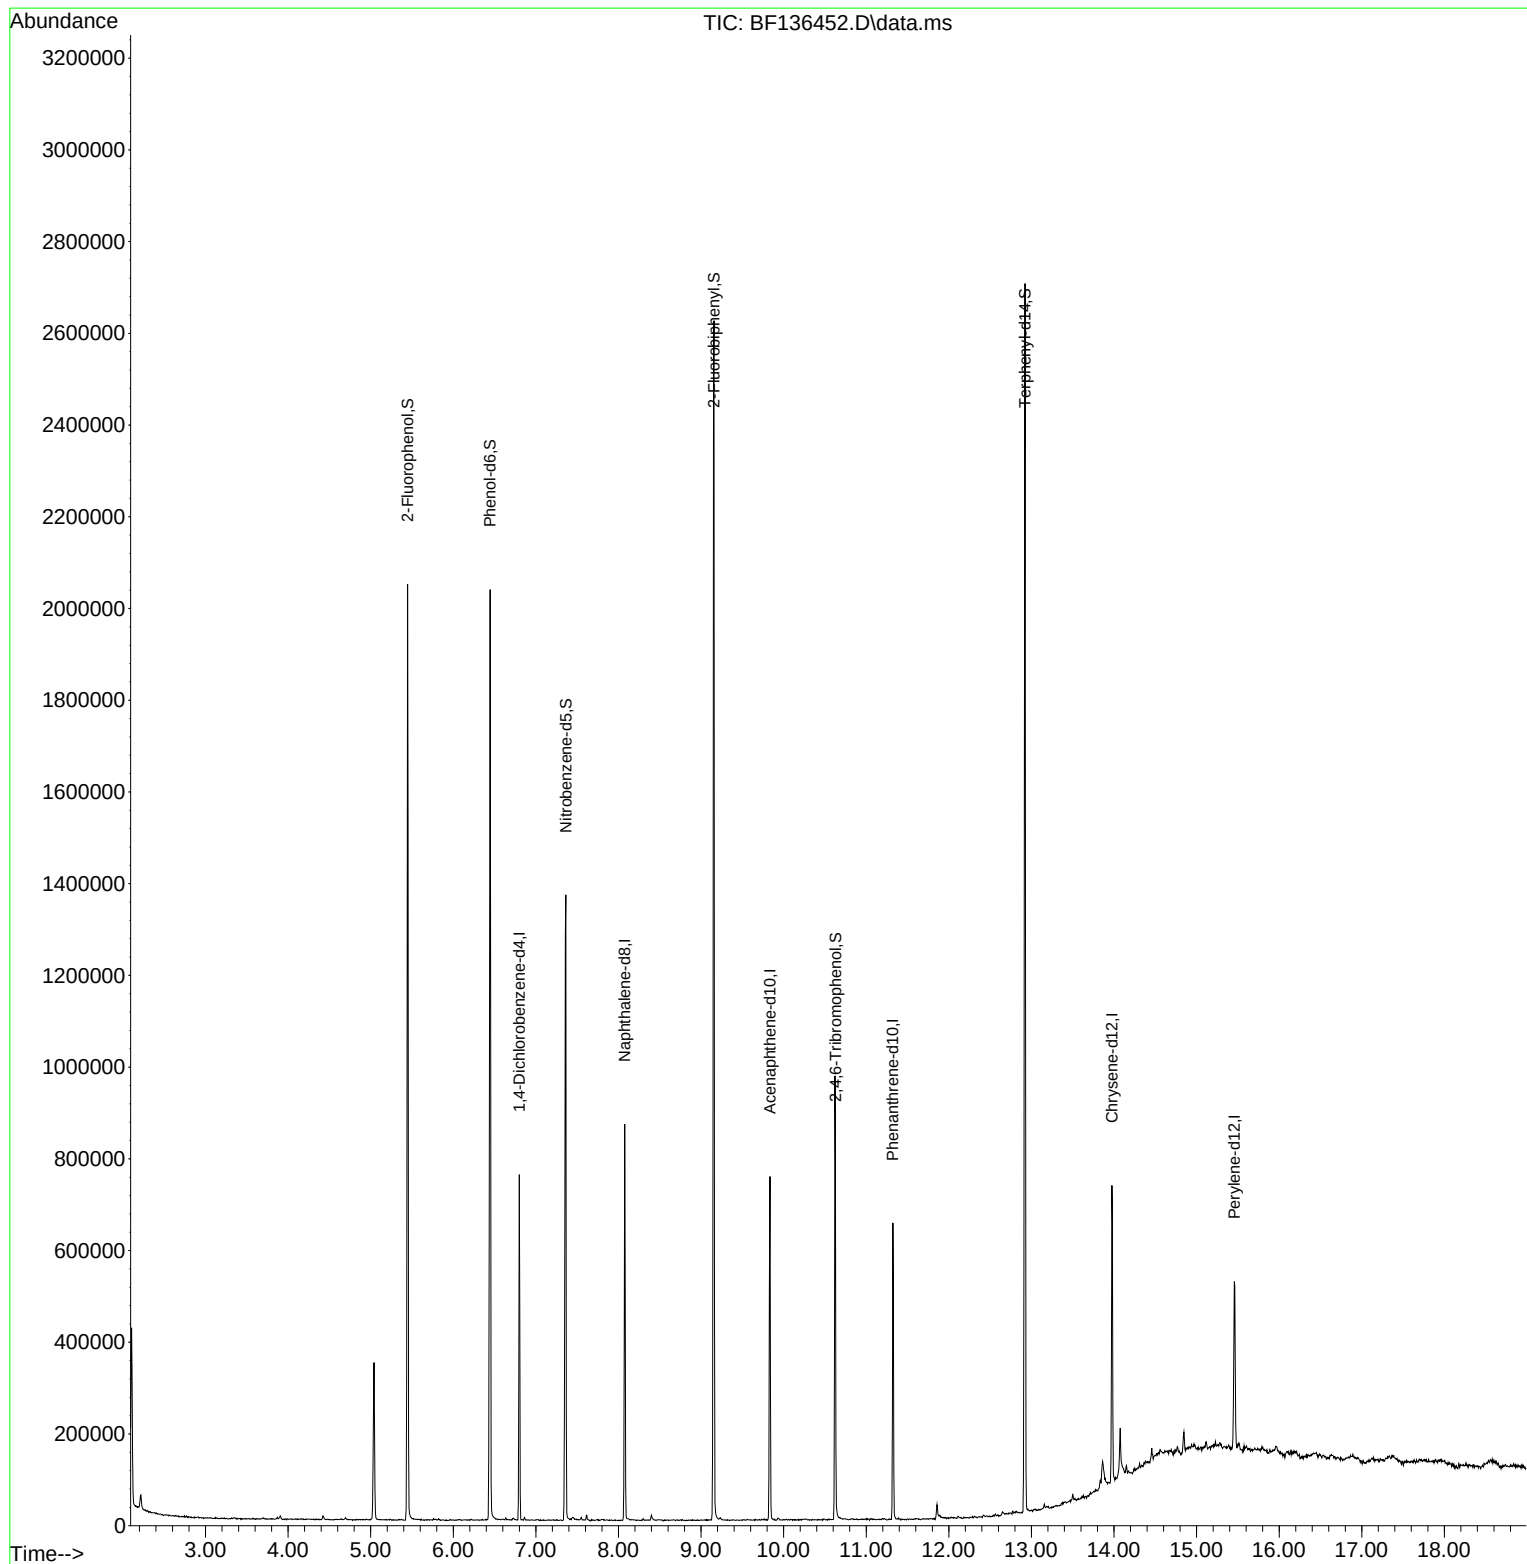


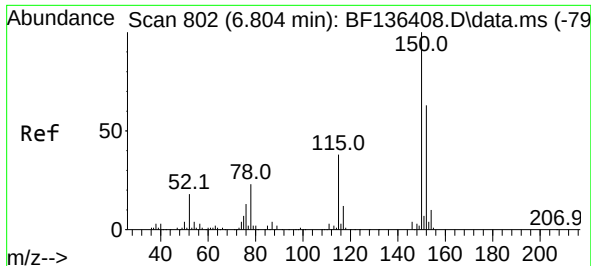

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.798 min Scan# 802
 Delta R.T. -0.006 min
 Lab File: BF136452.D
 Acq: 07 Dec 2023 17:57




Instrument :
 BNA_F
 ClientSampleId :
 LKWD-BACKFILL-02


Tgt Ion:152 Resp: 99805
 Ion Ratio Lower Upper
 152 100
 150 160.9 126.4 189.6
 115 62.7 48.2 72.4

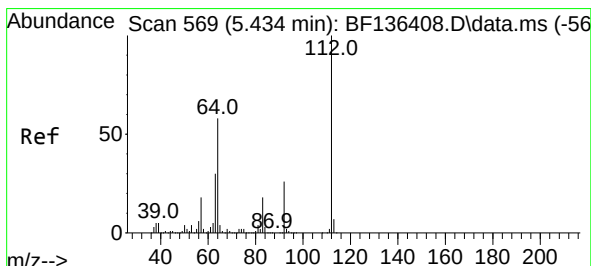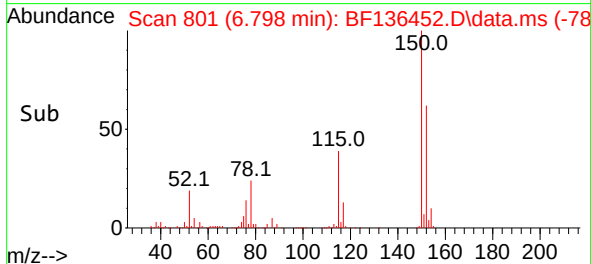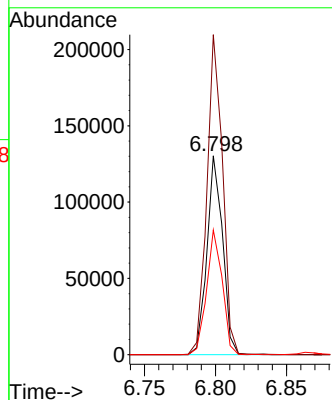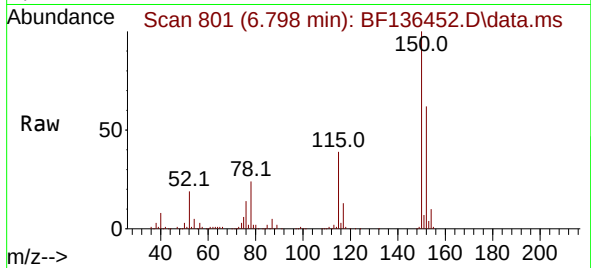

#5
 2-Fluorophenol
 Concen: 83.095 ng
 RT: 5.446 min Scan# 571
 Delta R.T. 0.012 min
 Lab File: BF136452.D
 Acq: 07 Dec 2023 17:57

Tgt Ion:112 Resp: 561564
 Ion Ratio Lower Upper
 112 100
 64 56.8 46.5 69.7
 63 30.7 23.9 35.9


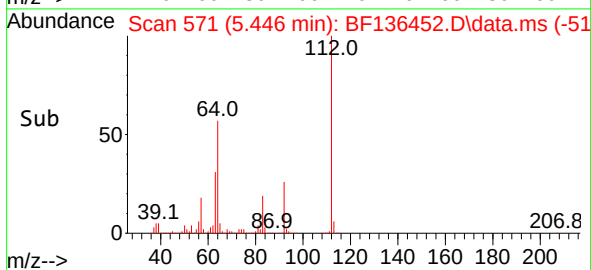
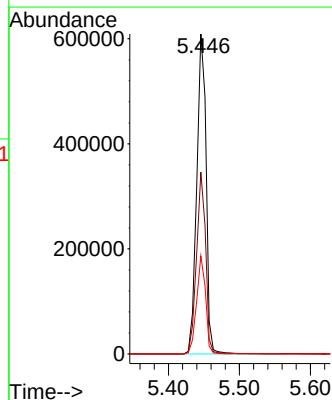
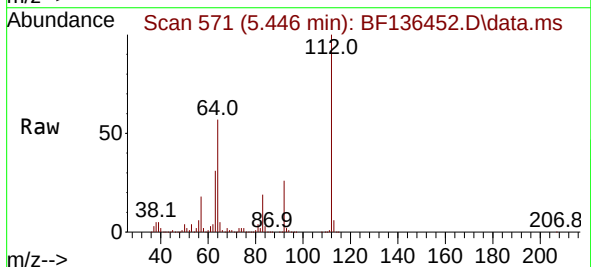


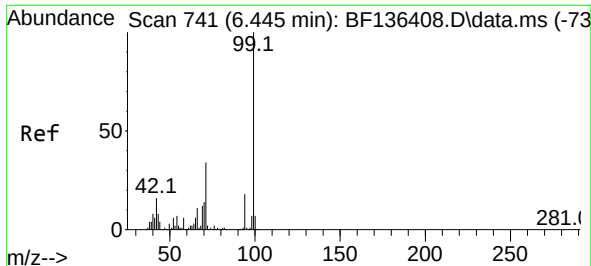

#7
Phenol-d6
Concen: 87.038 ng
RT: 6.446 min Scan# 741
Delta R.T. 0.000 min
Lab File: BF136452.D
Acq: 07 Dec 2023 17:57




Instrument :
BNA_F
ClientSampleId :
LKWD-BACKFILL-02


Tgt Ion: 99 Resp: 733884
Ion Ratio Lower Upper
99 100
42 15.8 12.8 19.2
71 34.8 27.0 40.4

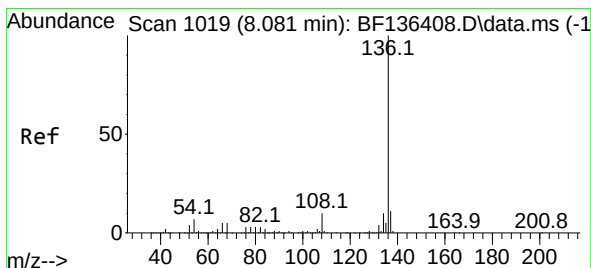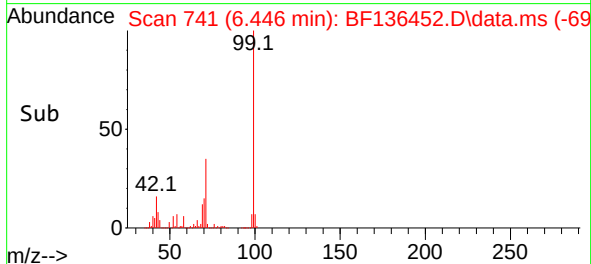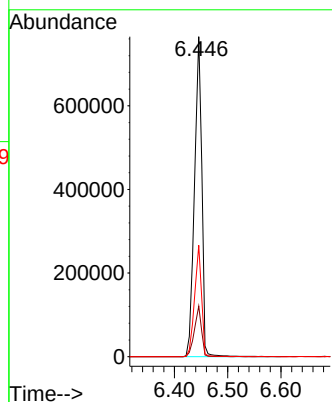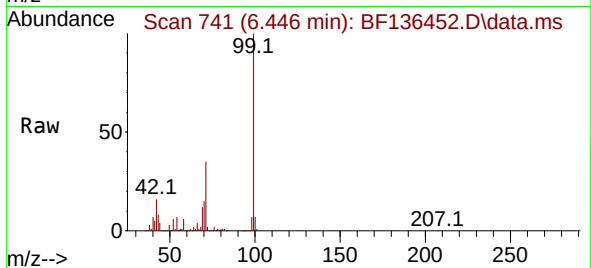

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.075 min Scan# 1018
Delta R.T. -0.006 min
Lab File: BF136452.D
Acq: 07 Dec 2023 17:57

Tgt Ion:136 Resp: 355749
Ion Ratio Lower Upper
136 100
137 10.8 8.6 12.8
54 7.2 5.7 8.5
68 5.1 4.0 6.0

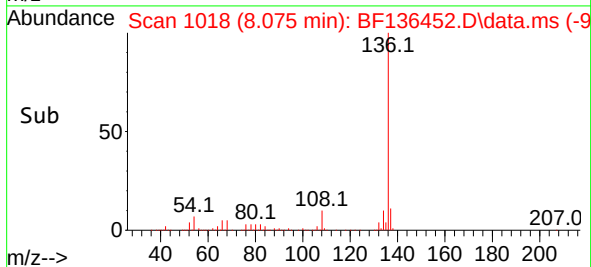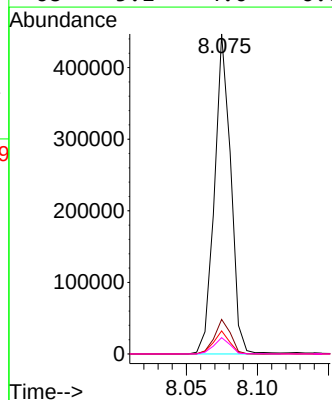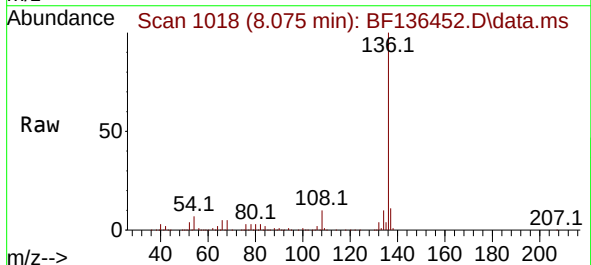

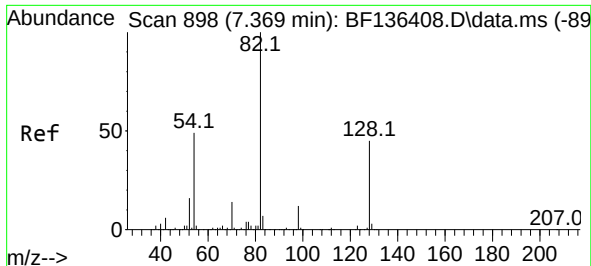

#23

Nitrobenzene-d5

Concen: 72.281 ng

RT: 7.363 min Scan# 89

Delta R.T. -0.006 min

Lab File: BF136452.D

Acq: 07 Dec 2023 17:57

Instrument :

BNA_F

ClientSampleId :

LKWD-BACKFILL-02





Tgt Ion: 82 Resp: 475652

Ion Ratio Lower Upper

82 100

128 48.2 36.3 54.5

54 46.7 39.0 58.6

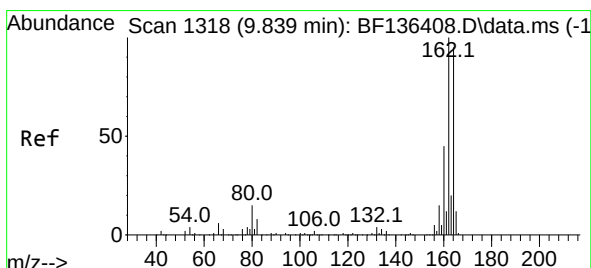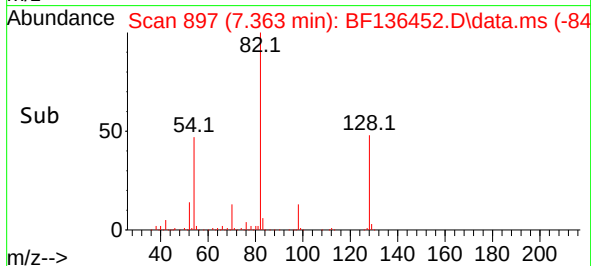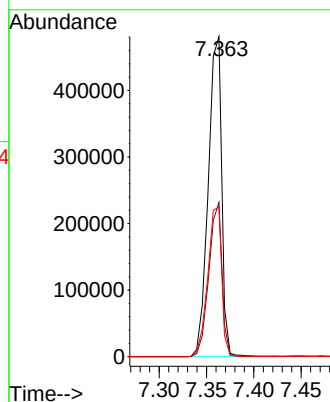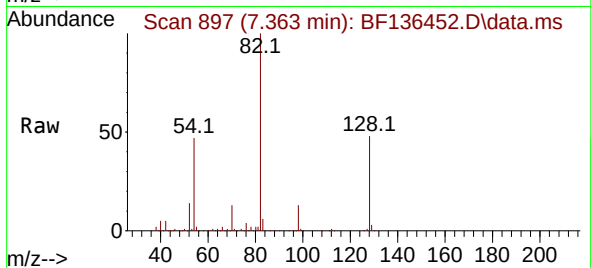

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.834 min Scan# 1317

Delta R.T. -0.006 min

Lab File: BF136452.D

Acq: 07 Dec 2023 17:57




Tgt Ion:164 Resp: 138794


Ion Ratio Lower Upper

164 100

162 100.5 84.4 126.6

160 45.3 37.6 56.4

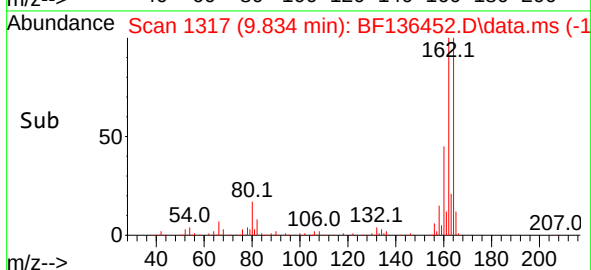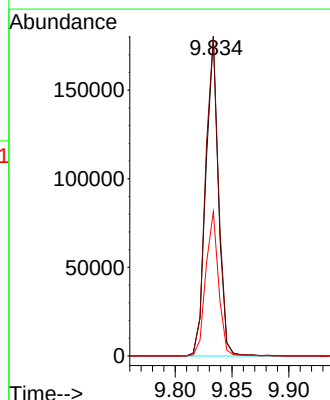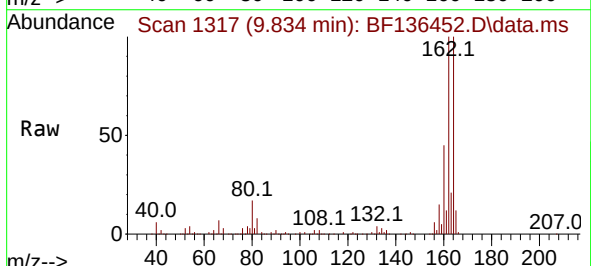

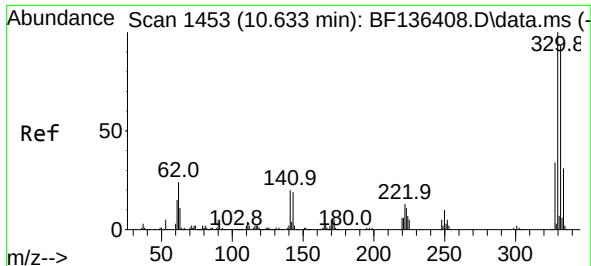

#42

2,4,6-Tribromophenol

Concen: 69.623 ng

RT: 10.628 min Scan# 1452

Delta R.T. -0.006 min

Lab File: BF136452.D

Acq: 07 Dec 2023 17:57

Instrument :

BNA_F

ClientSampleId :

LKWD-BACKFILL-02





Tgt Ion:330 Resp: 119148

Ion Ratio Lower Upper

330 100

332 95.9 76.4 114.6

141 29.4 23.4 35.2

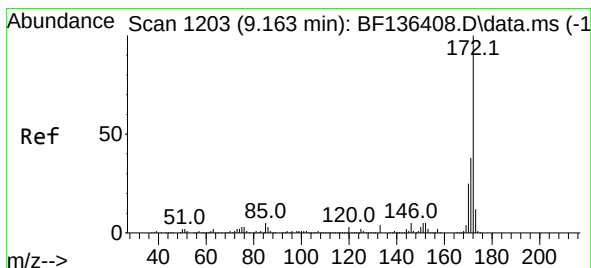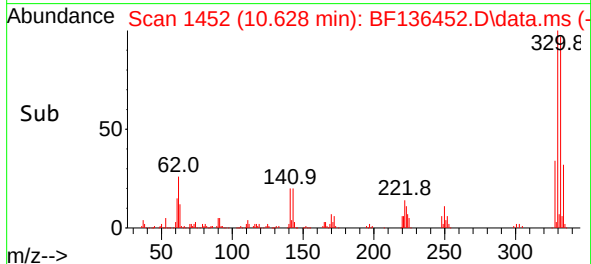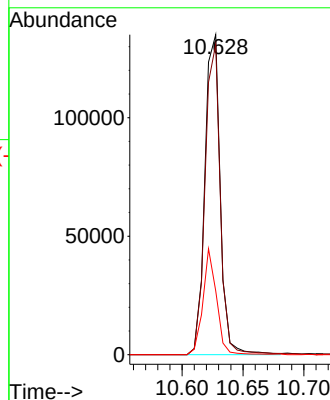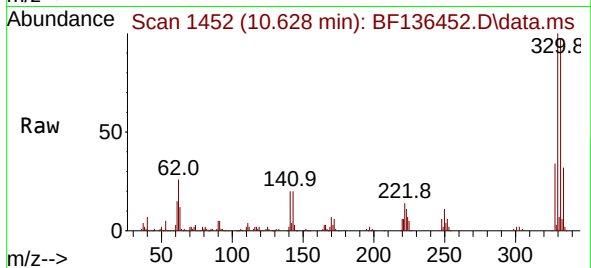

#45

2-Fluorobiphenyl

Concen: 83.422 ng

RT: 9.157 min Scan# 1202

Delta R.T. -0.006 min

Lab File: BF136452.D

Acq: 07 Dec 2023 17:57




Tgt Ion:172 Resp: 848551


Ion Ratio Lower Upper

172 100

171 36.5 30.5 45.7

170 23.8 19.9 29.9


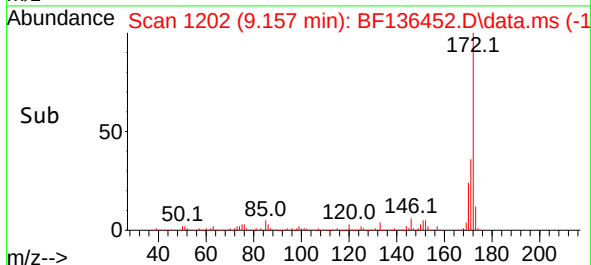
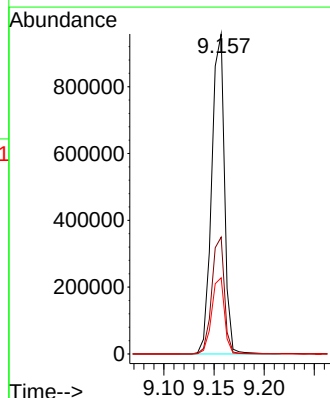
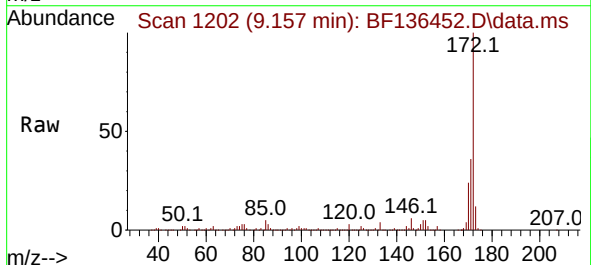


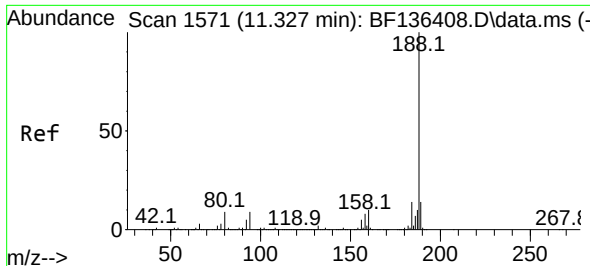

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.322 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF136452.D
Acq: 07 Dec 2023 17:57




Instrument :
BNA_F
ClientSampleId :
LKWD-BACKFILL-02


Tgt Ion:188 Resp: 229837
Ion Ratio Lower Upper
188 100
94 9.3 7.2 10.8
80 9.5 7.2 10.8

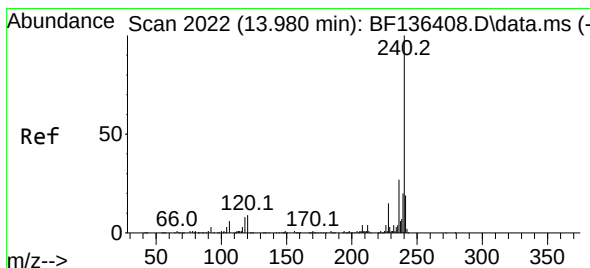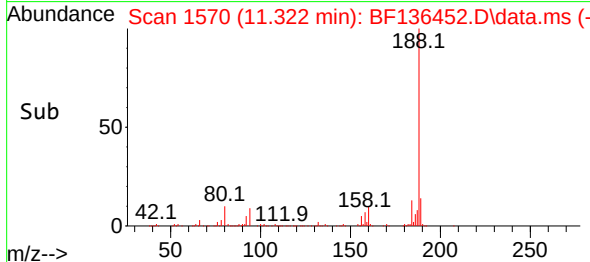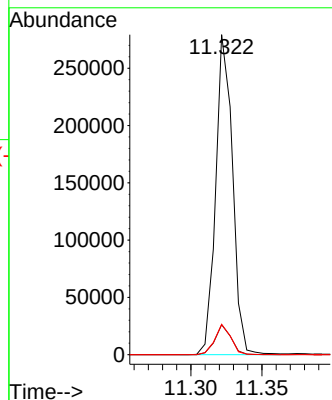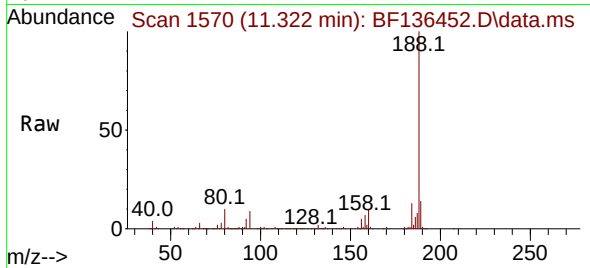

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.974 min Scan# 2021
Delta R.T. -0.006 min
Lab File: BF136452.D
Acq: 07 Dec 2023 17:57


Tgt Ion:240 Resp: 224192
Ion Ratio Lower Upper
240 100
120 11.1 7.3 10.9#
236 24.6 21.3 31.9

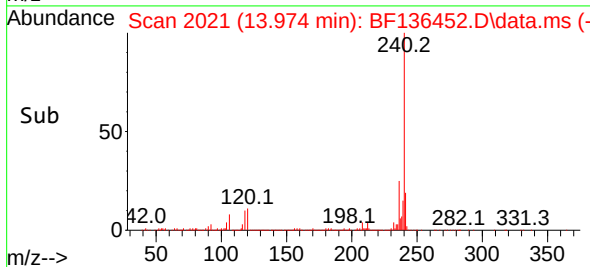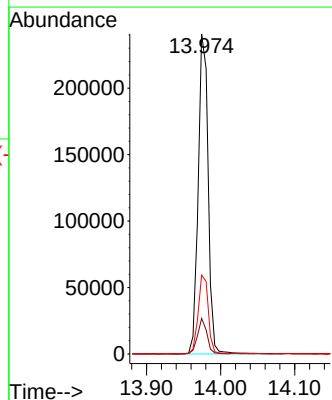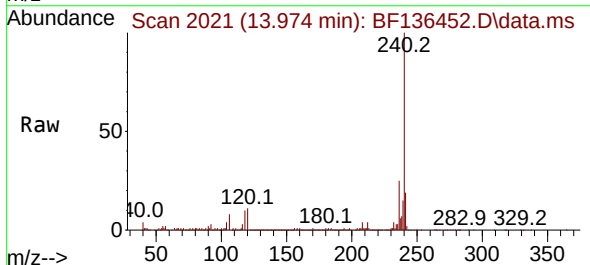



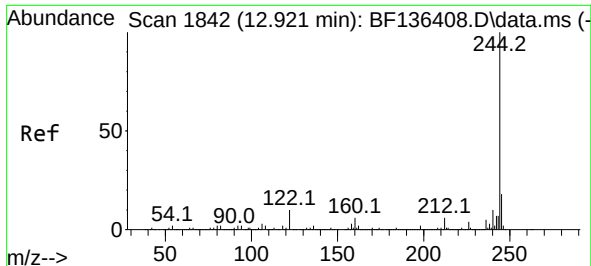


#79
 Terphenyl-d14
 Concen: 51.985 ng
 RT: 12.922 min Scan# 1842
 Delta R.T. 0.000 min
 Lab File: BF136452.D
 Acq: 07 Dec 2023 17:57

Instrument :
 BNA_F
 ClientSampleId :
 LKWD-BACKFILL-02

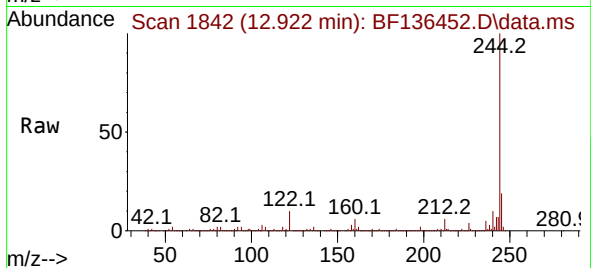

Tgt Ion:244 Resp: 884230
 Ion Ratio Lower Upper
 244 100
 212 6.2 5.0 7.4
 122 9.9 8.3 12.5

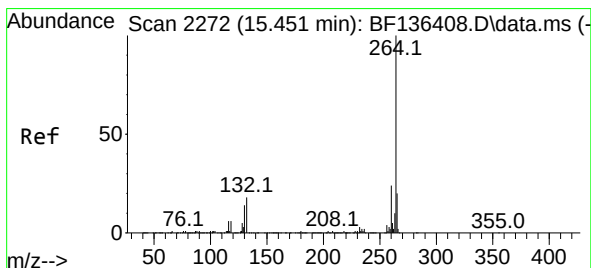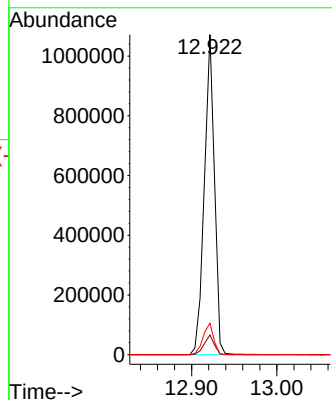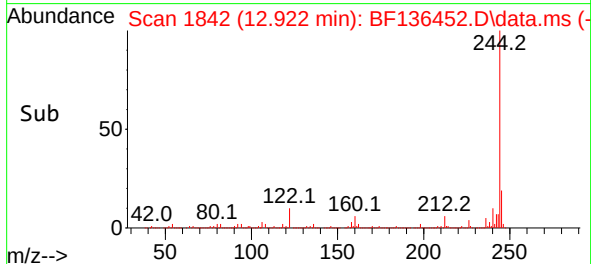

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.457 min Scan# 2273
 Delta R.T. 0.006 min
 Lab File: BF136452.D
 Acq: 07 Dec 2023 17:57

Tgt Ion:264 Resp: 182211
 Ion Ratio Lower Upper
 264 100
 260 24.6 19.2 28.8
 265 20.4 15.9 23.9

