


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120723\
 Data File : BF136441.D
 Acq On : 07 Dec 2023 11:43
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 06 09:40:27 2023

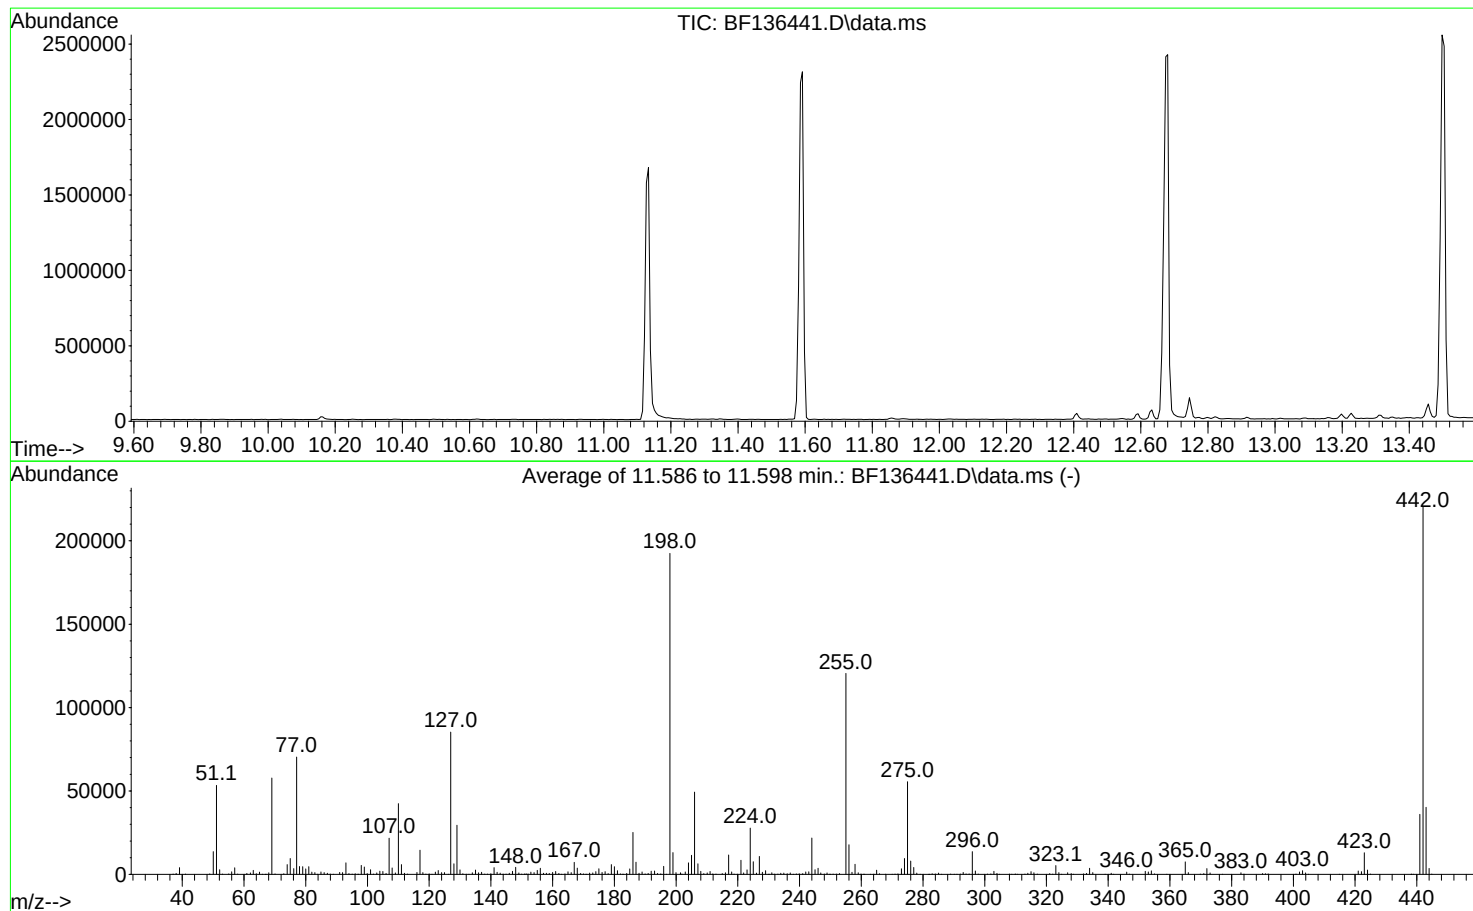




AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.7	53387	PASS
68	69	0.00	2	1.7	968	PASS
69	198	0.00	100	30.0	57725	PASS
70	69	0.00	2	0.6	320	PASS
127	198	10	80	44.3	85287	PASS
197	198	0.00	2	0.1	128	PASS
198	198	100	100	100.0	192493	PASS
199	198	5	9	6.8	13028	PASS
275	198	10	60	28.9	55562	PASS
365	198	1	100	3.9	7501	PASS
441	198	0.01	100	18.7	35952	PASS
442	442	50	100	100.0	220579	PASS
443	442	15	24	18.2	40208	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120723\
Data File : BF136441.D
Acq On : 07 Dec 2023 11:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 07 13:04:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 06 09:40:27 2023
Response via : Initial Calibration

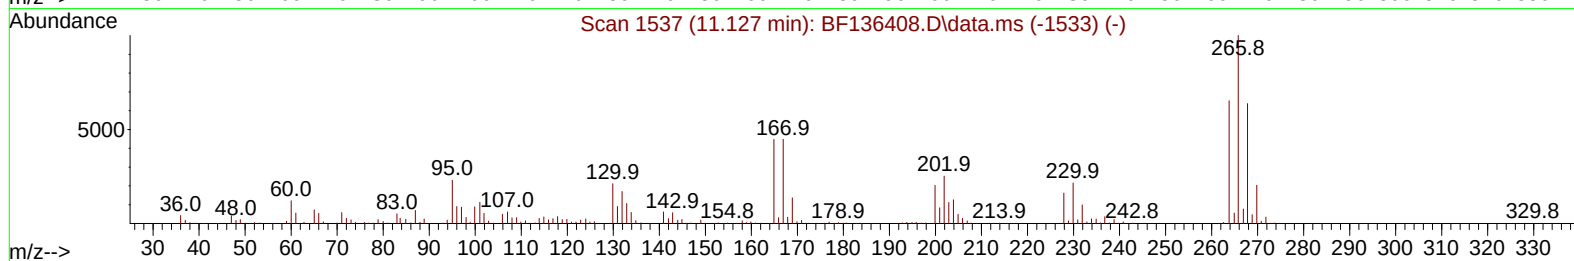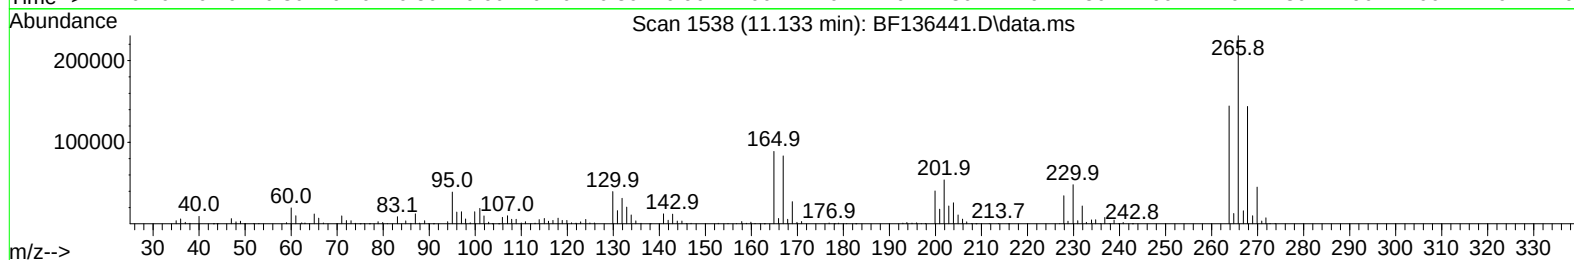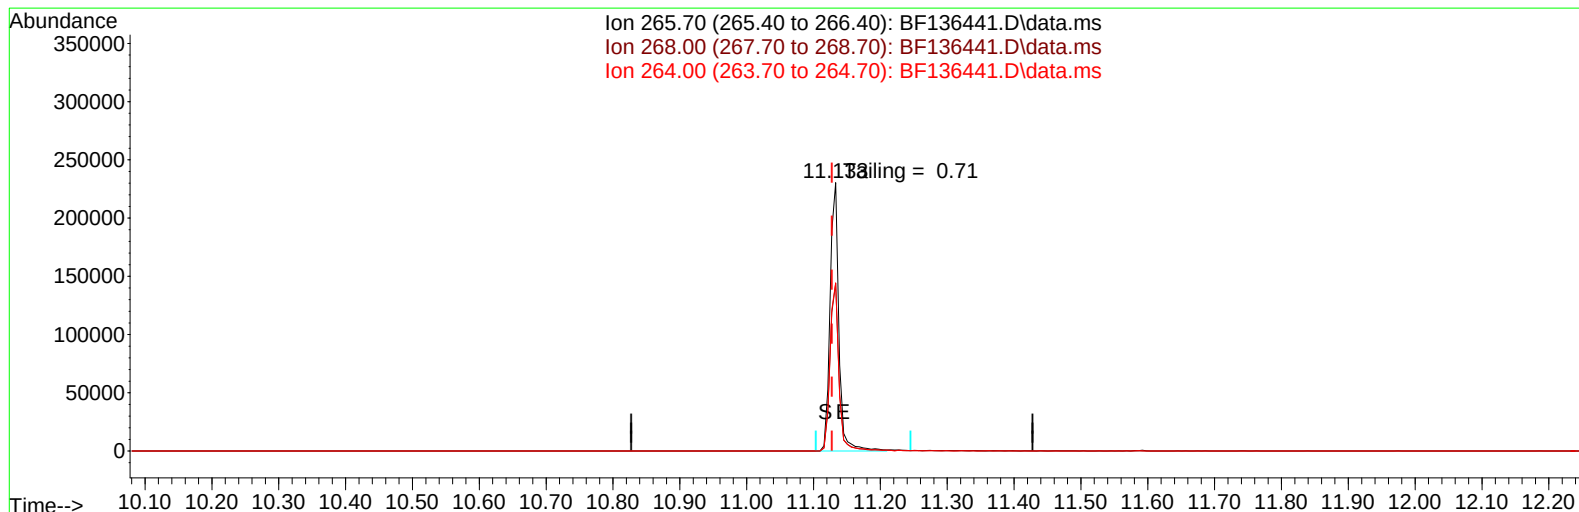

TIC: BF136441.D\data.ms

(70) Pentachlorophenol (C)

11.133min (+ 0.006) 29029.51 ng




response 213115

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	62.43
264.00	65.30	62.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120723\
Data File : BF136441.D
Acq On : 07 Dec 2023 11:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 07 13:04:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 06 09:40:27 2023
Response via : Initial Calibration

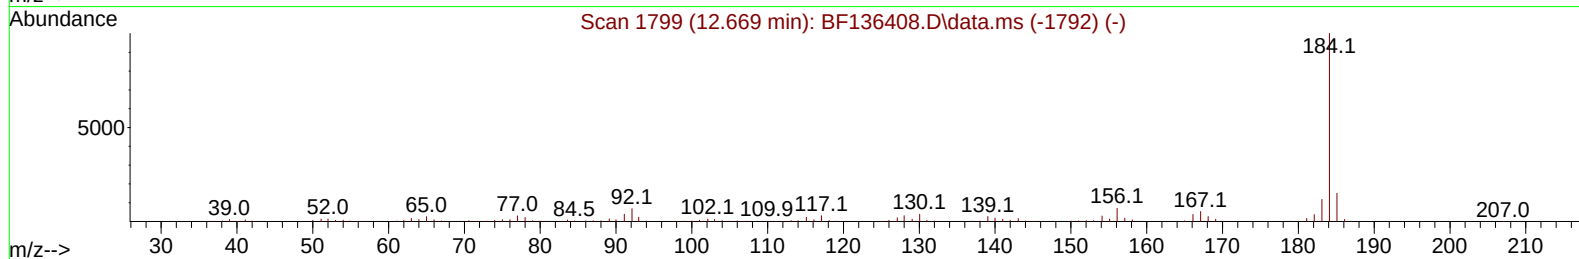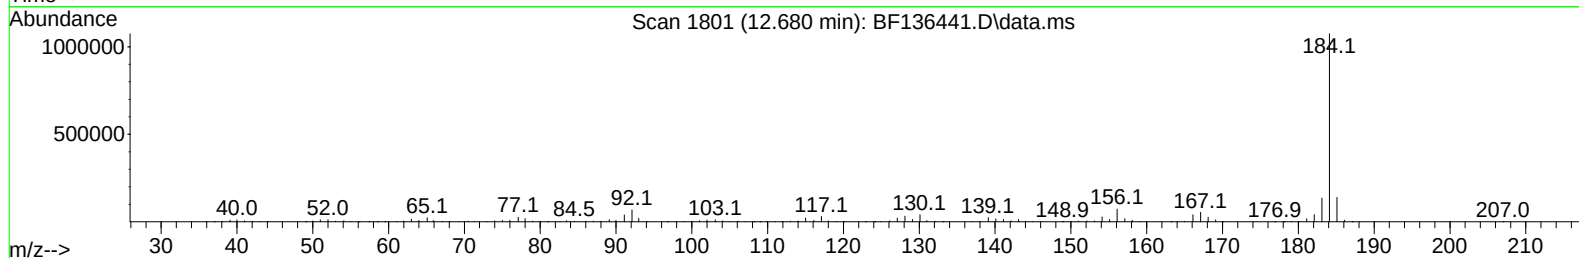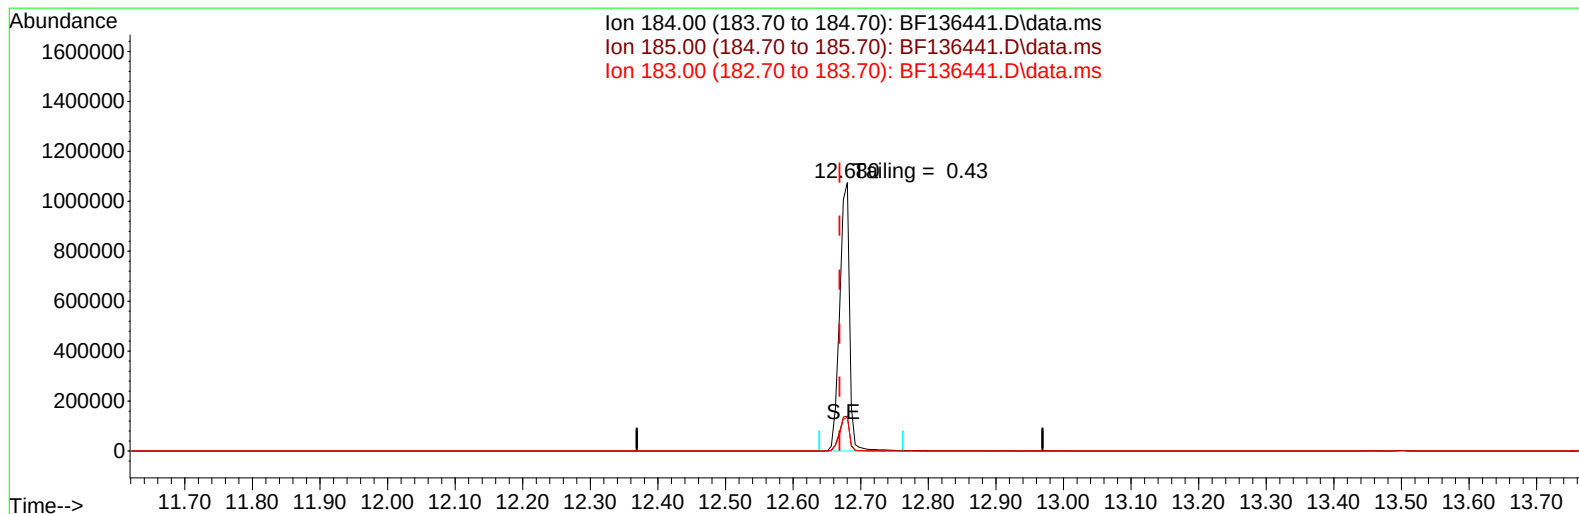

TIC: BF136441.D\data.ms

(77) Benzidine

12.680min (+ 0.011) 1872.15 ng

response 1085015

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	12.99
183.00	11.70	12.62
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/7/2023	BNA_F	<u>BF1364441.D</u>
Compound Name	Response	Retention Time
DDT	514967	13.505
DDD	10974	13.227
DDE	550	12.862
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11524	526491	2.19

Instrument :
BNA_F
ClientSampleId :
DFTPP