


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF120818\
 Data File : BF111221.D
 Acq On : 8 Dec 2018 11:09
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 10 01:15:27 2018

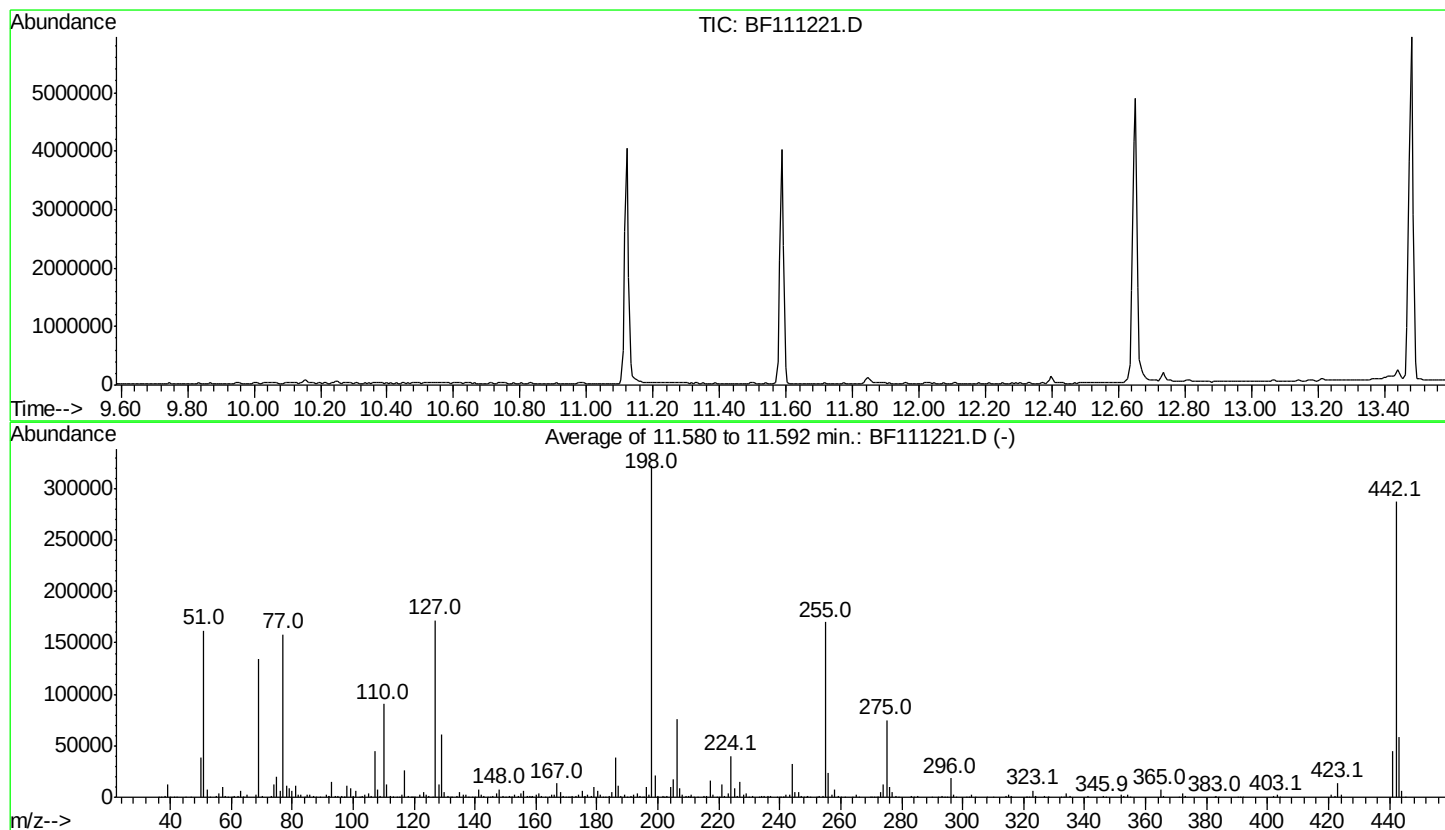

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.2	161809	PASS
68	69	0.00	2	1.6	2115	PASS
69	198	0.00	100	41.8	134845	PASS
70	69	0.00	2	0.5	704	PASS
127	198	10	80	53.4	172056	PASS
197	198	0.00	2	0.7	2407	PASS
198	198	100	100	100.0	322368	PASS
199	198	5	9	6.7	21546	PASS
275	198	10	60	23.3	75000	PASS
365	198	1	100	2.2	7010	PASS
441	198	0.01	100	14.1	45423	PASS
442	198	50	100	89.2	287469	PASS
443	442	15	24	20.2	58026	PASS