
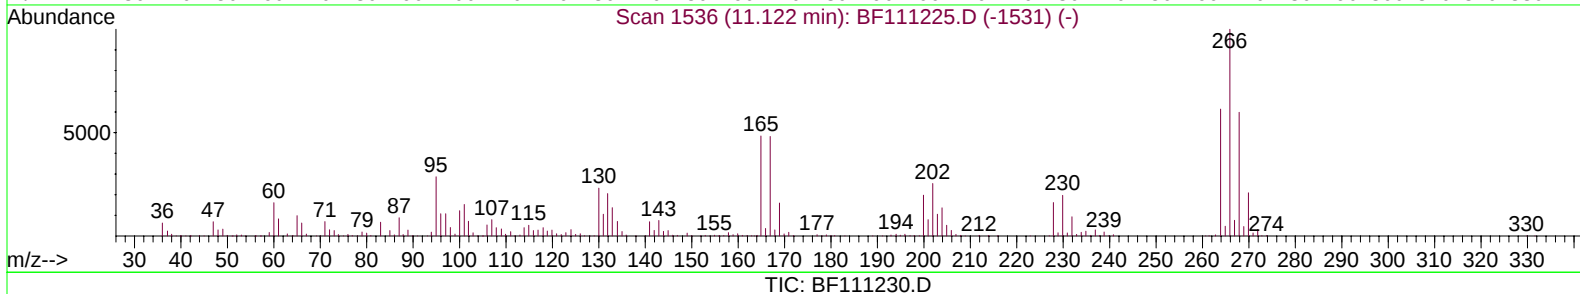
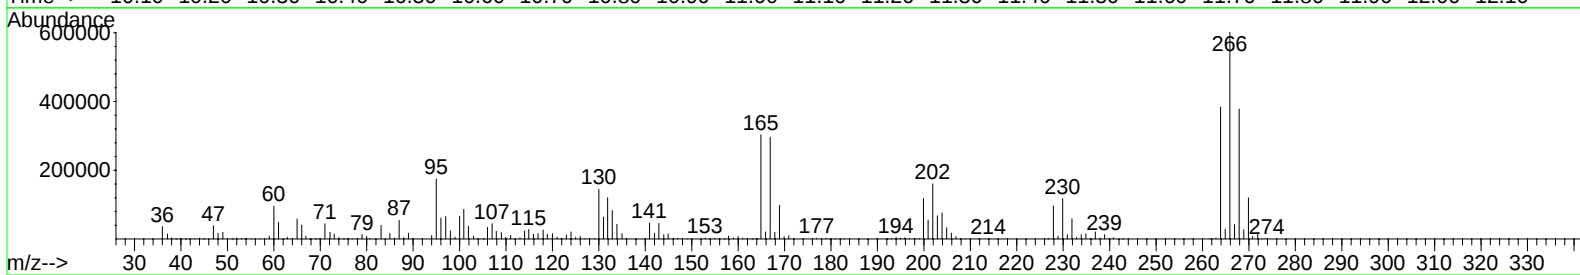


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF120918\
Data File : BF111230.D
Acq On : 10 Dec 2018 9:26
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 10 09:52:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF120818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 10 01:15:27 2018
Response via : Initial Calibration

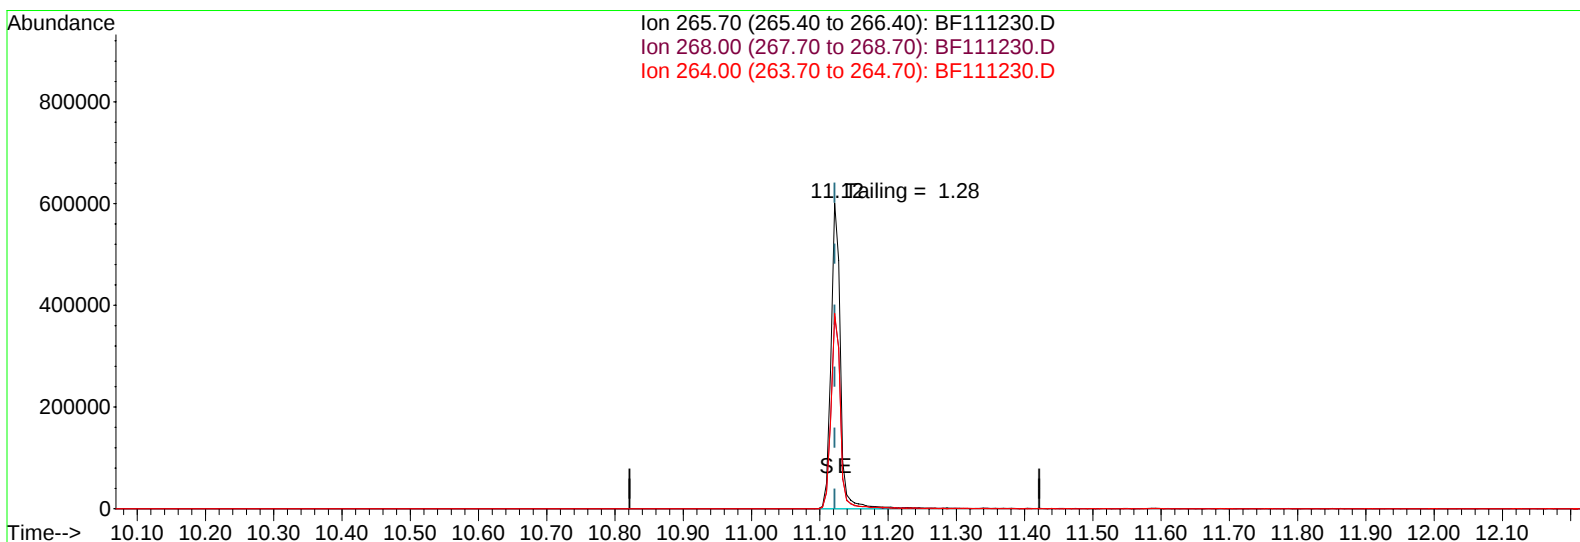

(70) Pentachlorophenol (C)




11.122min (-0.000) 15191.69ng

response 569011

Ion	Exp%	Act%
265.70	100	100
268.00	59.90	62.86
264.00	61.40	63.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF120918\
Data File : BF111230.D
Acq On : 10 Dec 2018 9:26
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 10 09:52:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF120818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 10 01:15:27 2018
Response via : Initial Calibration

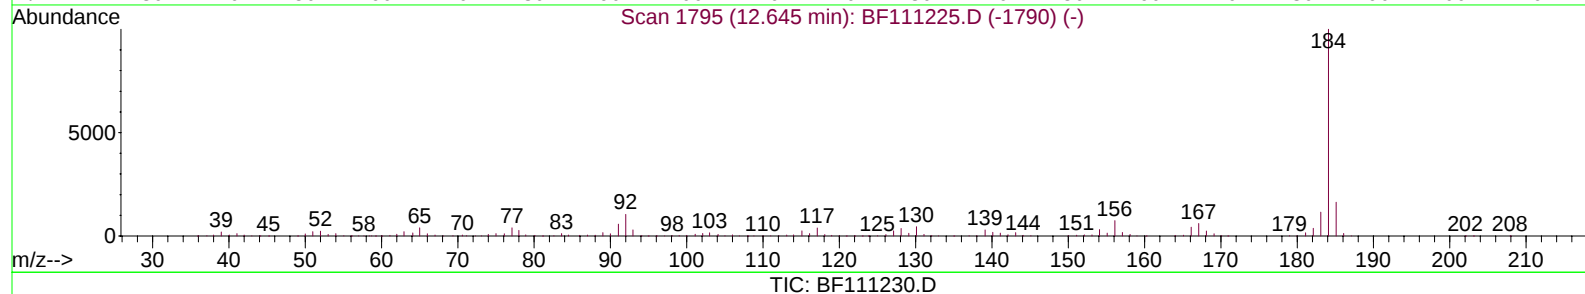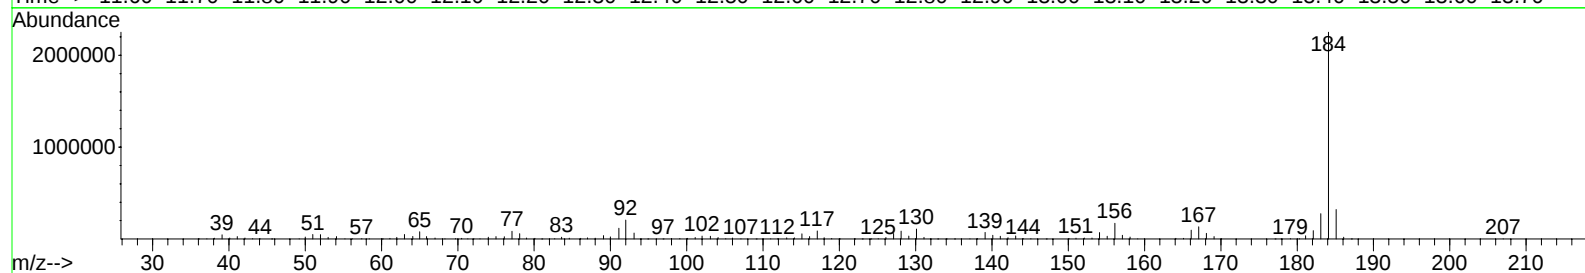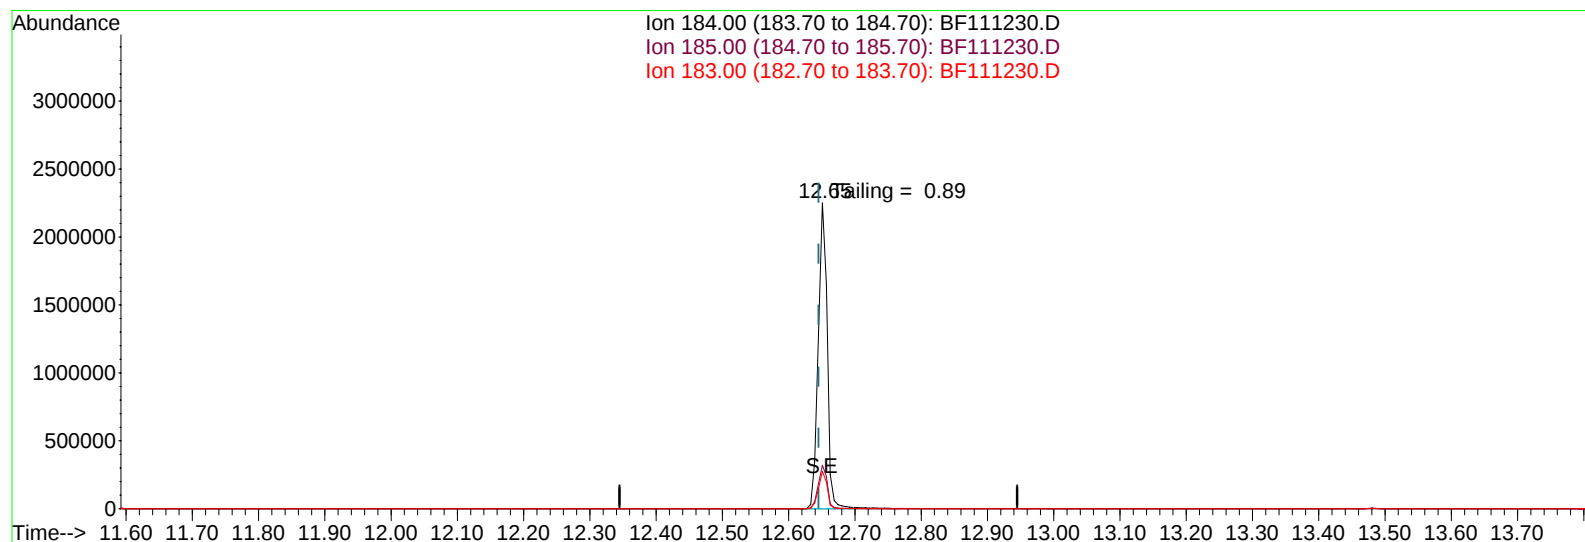

(77) Benzidine

12.651min (+0.006) 39239.28ng

response 2136794

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.24
183.00	11.60	12.24
0.00	0.00	0.00