


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF120918\
 Data File : BF111230.D
 Acq On : 10 Dec 2018 9:26
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 10 01:15:27 2018

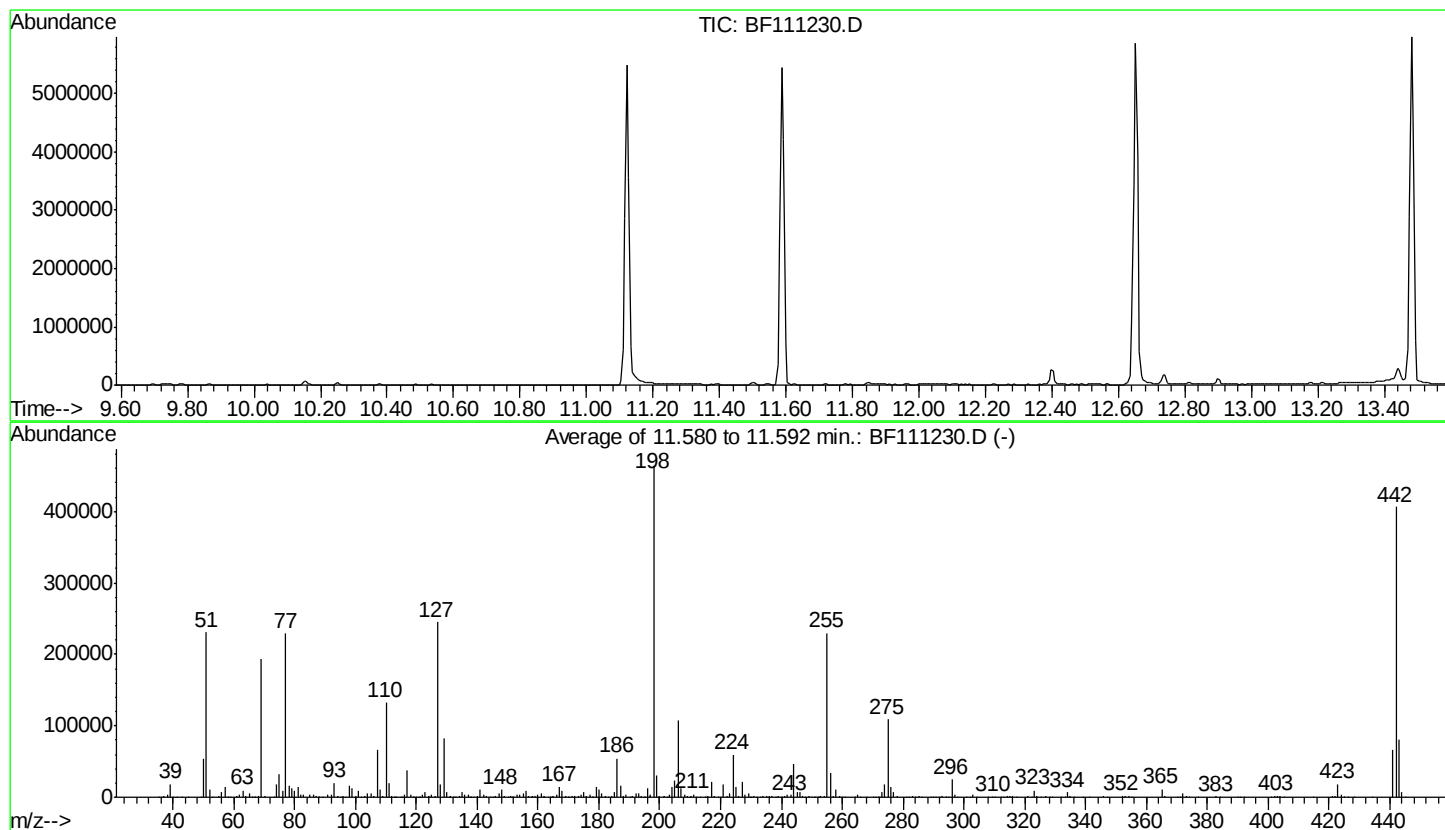

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.7	230782	PASS
68	69	0.00	2	1.3	2463	PASS
69	198	0.00	100	41.6	193280	PASS
70	69	0.00	2	0.7	1300	PASS
127	198	10	80	52.8	245162	PASS
197	198	0.00	2	0.8	3636	PASS
198	198	100	100	100.0	464149	PASS
199	198	5	9	6.5	30365	PASS
275	198	10	60	23.4	108477	PASS
365	198	1	100	2.3	10847	PASS
441	198	0.01	100	14.3	66602	PASS
442	198	50	100	87.6	406498	PASS
443	442	15	24	20.1	81581	PASS