


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121018\
 Data File : BF111243.D
 Acq On : 10 Dec 2018 15:44
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 10 01:15:27 2018

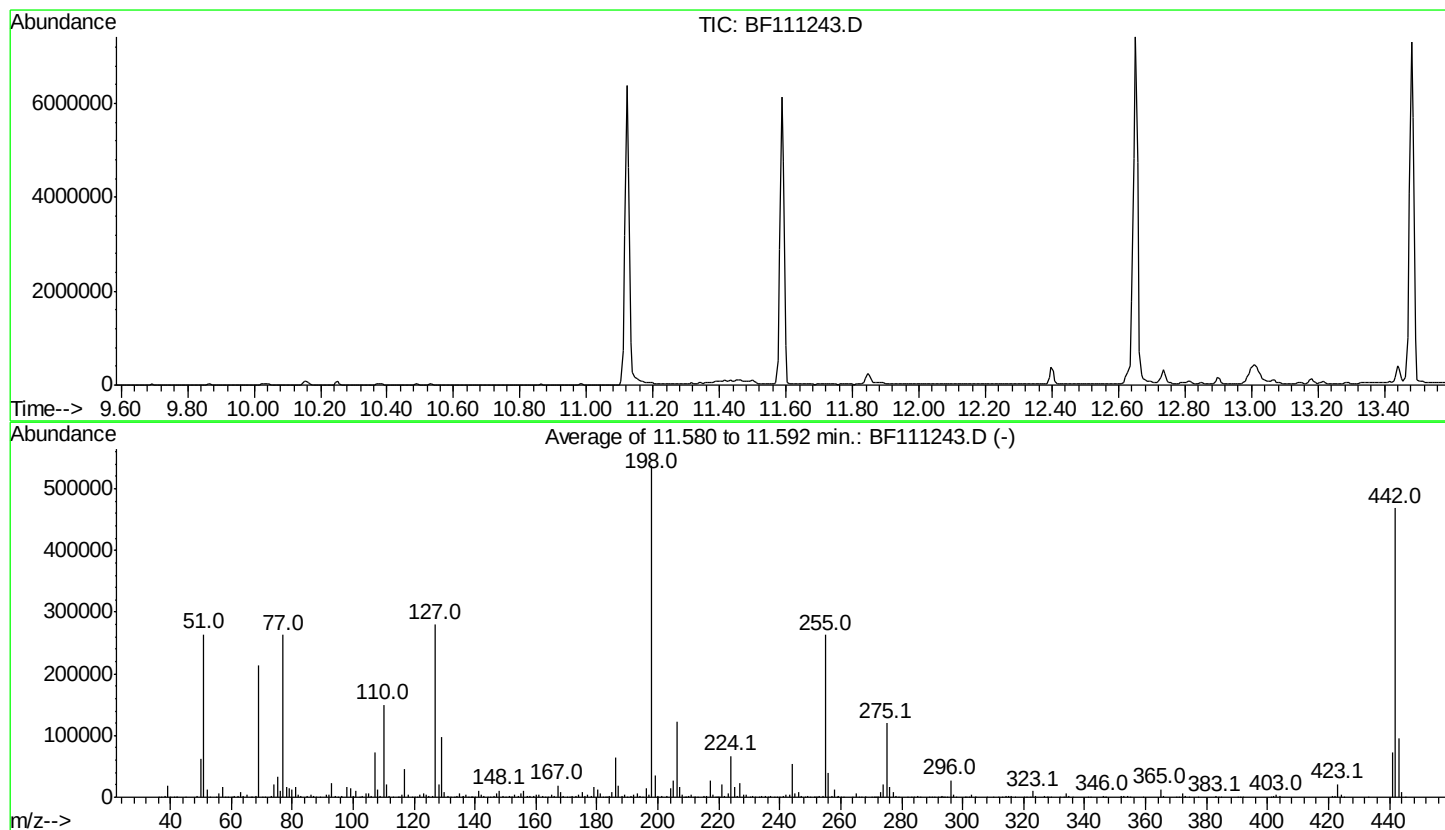

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.2	264204	PASS
68	69	0.00	2	1.4	3069	PASS
69	198	0.00	100	39.9	214395	PASS
70	69	0.00	2	0.3	654	PASS
127	198	10	80	52.0	279466	PASS
197	198	0.00	2	0.8	4248	PASS
198	198	100	100	100.0	537429	PASS
199	198	5	9	6.6	35208	PASS
275	198	10	60	22.3	119773	PASS
365	198	1	100	2.4	12734	PASS
441	198	0.01	100	13.6	73208	PASS
442	198	50	100	87.1	468160	PASS
443	442	15	24	20.3	95178	PASS