

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF121019\
 Data File : BF118173.D
 Acq On : 10 Dec 2019 19:58
 Operator : JU
 Sample : K6204-15
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Dec 11 02:35:43 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF120619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 06 17:34:43 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.87	152	74385	20.00	ng	0.00
21) Naphthalene-d8	8.16	136	281284	20.00	ng	0.00
39) Acenaphthene-d10	9.92	164	136952	20.00	ng	0.00
64) Phenanthrene-d10	11.41	188	237008	20.00	ng	0.00
76) Chrysene-d12	14.06	240	188539	20.00	ng	0.00
87) Perylene-d12	15.56	264	180433	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.49	112	559275	131.69	ng	0.00
7) Phenol-d6	6.50	99	624928	121.65	ng	0.00
23) Nitrobenzene-d5	7.43	82	445384	89.08	ng	0.00
42) 2,4,6-Tribromophenol	10.71	330	215393	129.46	ng	0.00
45) 2-Fluorobiphenyl	9.23	172	890234	98.91	ng	0.00
79) Terphenyl-d14	13.00	244	933134	85.11	ng	0.00
Target Compounds						
9) Benzaldehyde	6.50	77	942	Below Cal	Qvalue	# 1
15) Benzyl Alcohol	7.03	79	8136	2.029 ng	#	48
19) n-Nitroso-di-n-propylamine	7.43	70	59918	19.196 ng	#	76
25) Isophorone	7.43	82	440212	51.937 ng	#	62
51) 2,6-Dinitrotoluene	9.92	165	16679	7.583 ng	#	28
57) 2,4-Dinitrotoluene	9.92	165	16679	5.681 ng	#	26
67) 4-Bromophenyl-phenylether	10.71	248	13120	4.849 ng	#	1
77) Benzidine	13.00	184	12960	2.611 ng	#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF121019\
Data File : BF118173.D
Acq On : 10 Dec 2019 19:58
Operator : JU
Sample : K6204-15
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Dec 11 02:35:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF120619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 17:34:43 2019
Response via : Initial Calibration

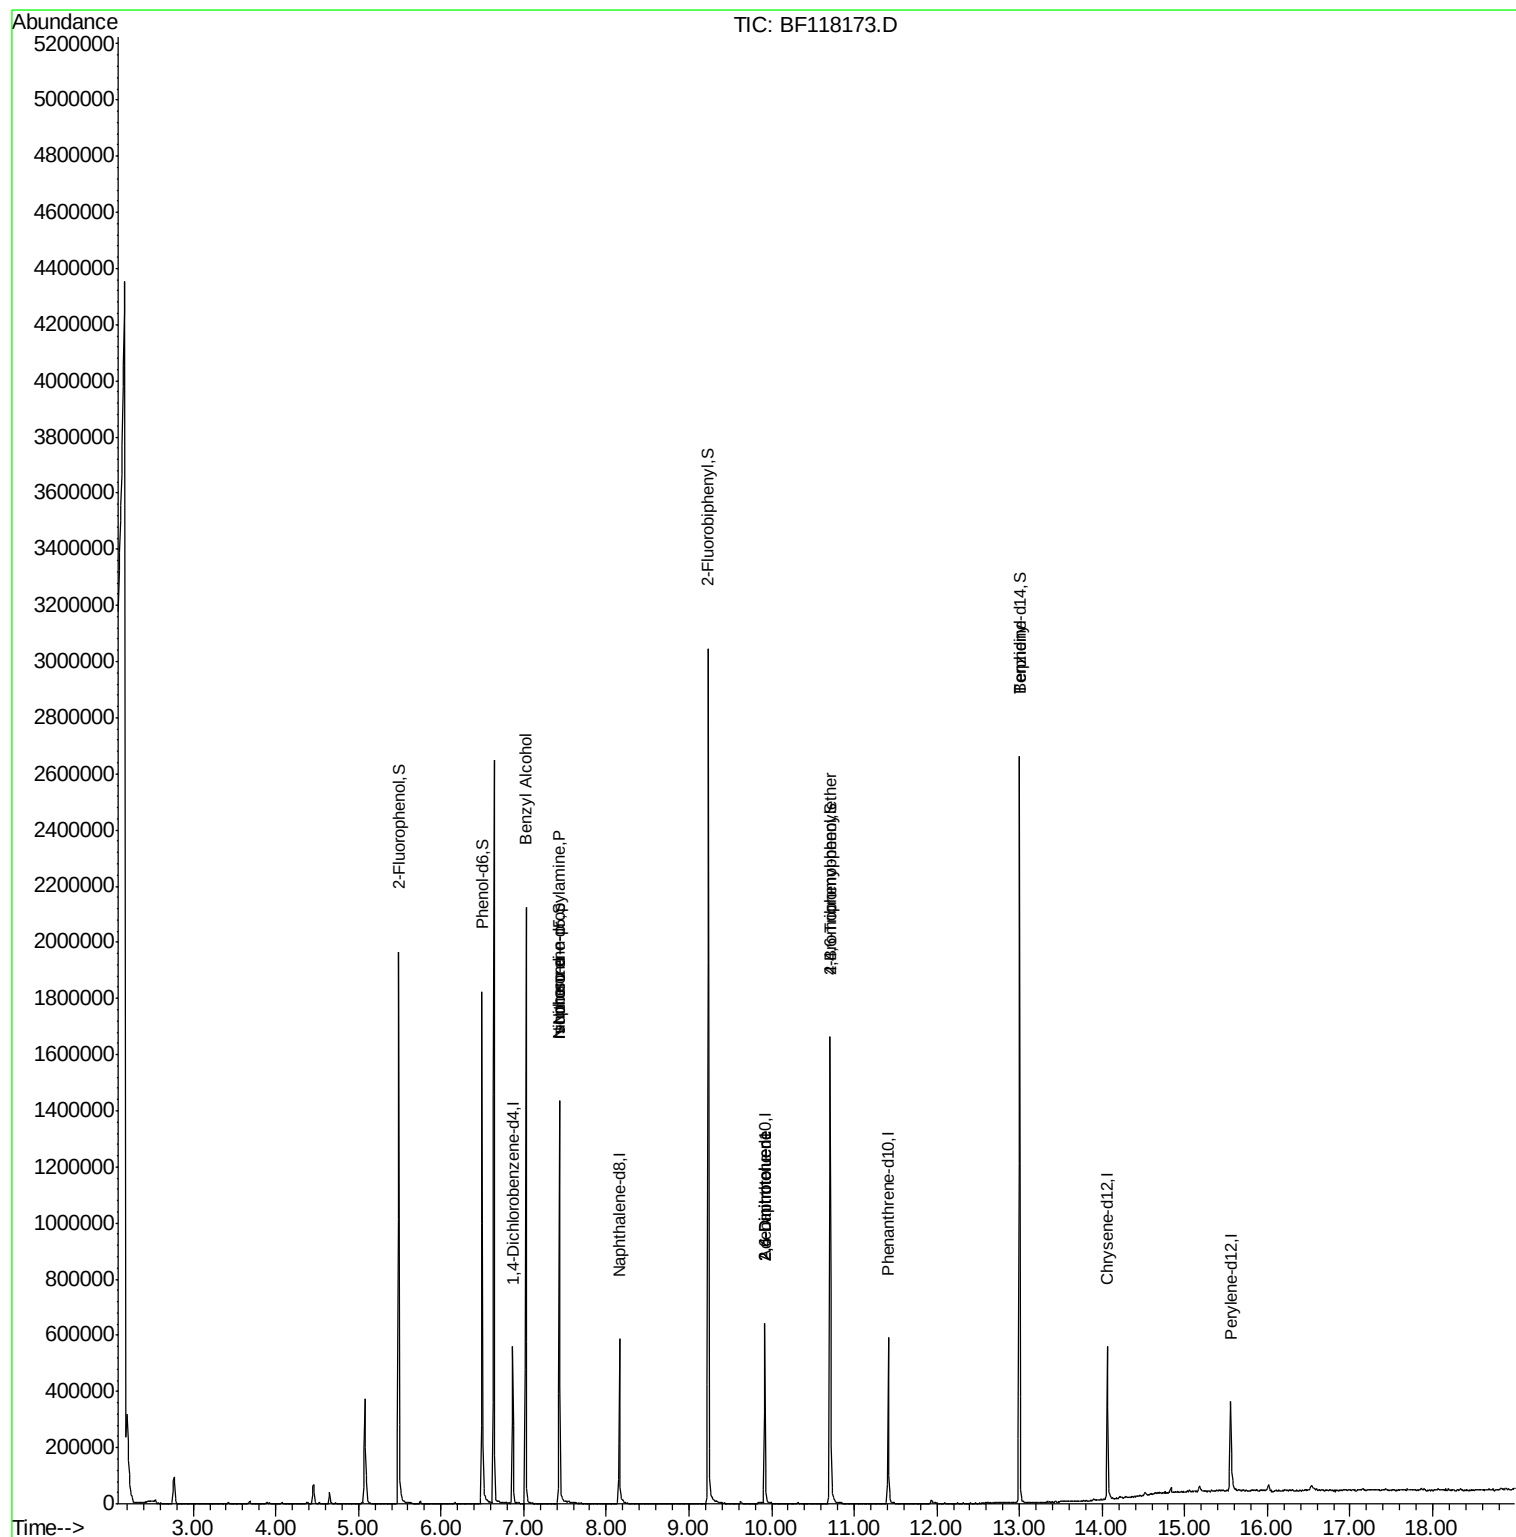




#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.87 min Scan# 813
Delta R.T. -0.00 min
Lab File: BF118173.D
Acq: 10 Dec 2019 19:58

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	158.7	128.3	192.5
115	65.4	51.1	76.7






Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

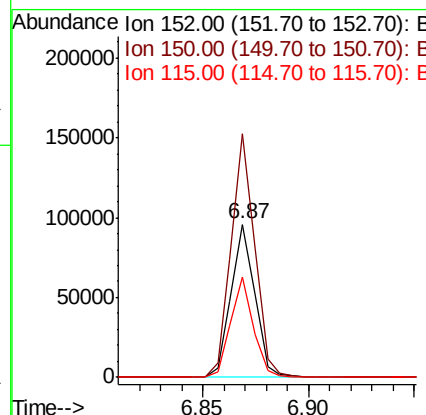

#5

2-Fluorophenol
Concen: 131.687 ng
RT: 5.49 min Scan# 578
Delta R.T. 0.01 min
Lab File: BF118173.D
Acq: 10 Dec 2019 19:58

Tgt Ion	Ratio	Lower	Upper
112	100		
64	54.1	41.3	61.9
63	30.3	22.4	33.6






Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

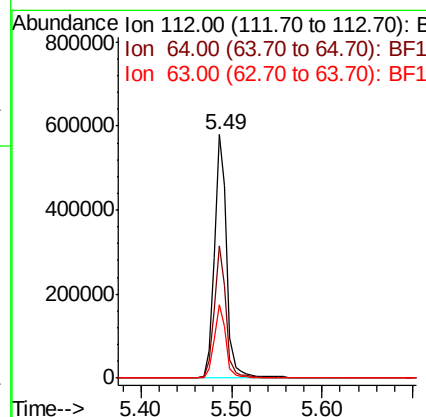

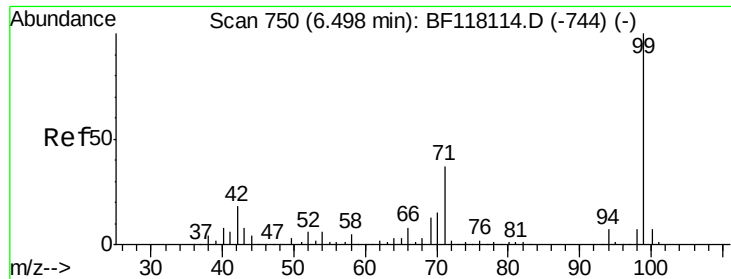

#7

Phenol-d6

Concen: 121.655 ng

RT: 6.50 min Scan# 750

Delta R.T. -0.00 min

Lab File: BF118173.D

Acq: 10 Dec 2019 19:58

Instrument :

BNA_F

ClientSampled :


Tot Ion: 99 Resp: 624928

Ion Ratio Lower Upper




99 100

42 17.6 14.1 21.1

71 37.3 29.7 44.5

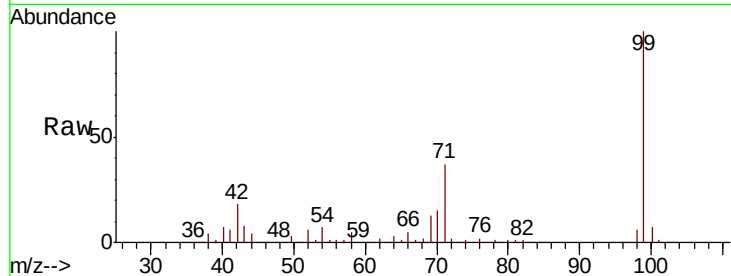

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

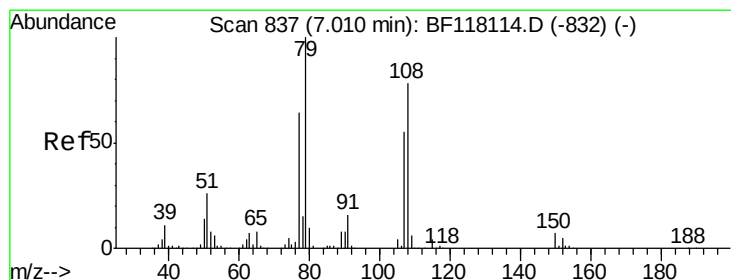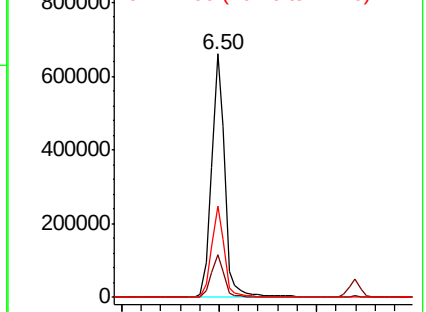

#15

Benzyl Alcohol

Concen: 2.029 ng

RT: 7.03 min Scan# 840

Delta R.T. 0.02 min

Lab File: BF118173.D

Acq: 10 Dec 2019 19:58


Tgt Ion: 79 Resp: 8136

Ion Ratio Lower Upper



79 100




108 33.8 62.7 94.1#

77 105.5 51.4 77.2#



Abundance Ion 79.00 (78.70 to 79.70): BF1
Ion 108.00 (107.70 to 108.70): BF1
Ion 77.00 (76.70 to 77.70): BF1




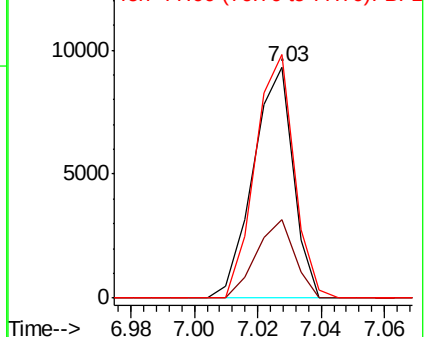


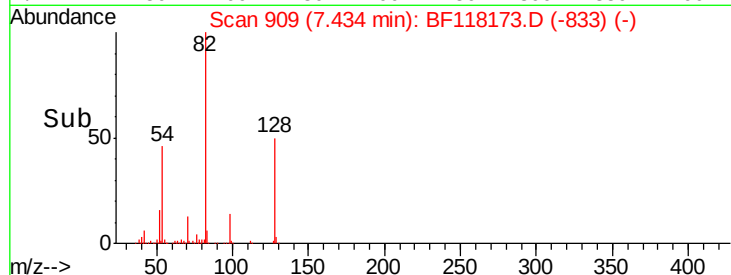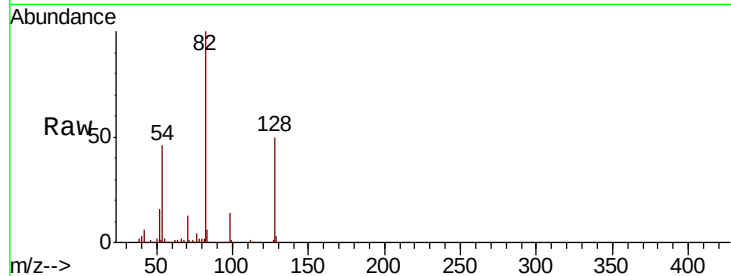

#19
n-Nitroso-di-n-propylamine
Concen: 19.196 ng
RT: 7.43 min Scan# 909
Delta R.T. 0.15 min
Lab File: BF118173.D
Acq: 10 Dec 2019 19:58


Instrument :
BNA_F
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
70	100		
42	44.5	43.2	64.8
101	0.0	8.1	12.1
130	2.2	19.8	29.8

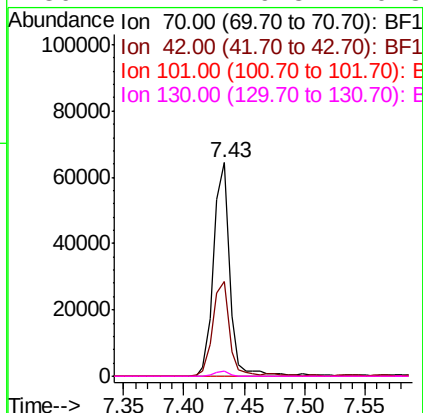

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.16 min Scan# 1032
Delta R.T. -0.00 min
Lab File: BF118173.D
Acq: 10 Dec 2019 19:58

Tgt Ion	Ratio	Lower	Upper
136	100		
137	10.8	9.0	13.6
54	5.6	5.0	7.6
68	4.0	3.8	5.8

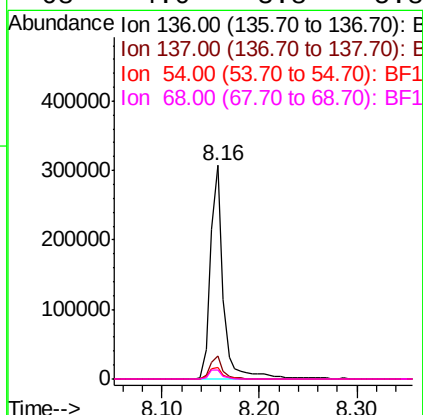


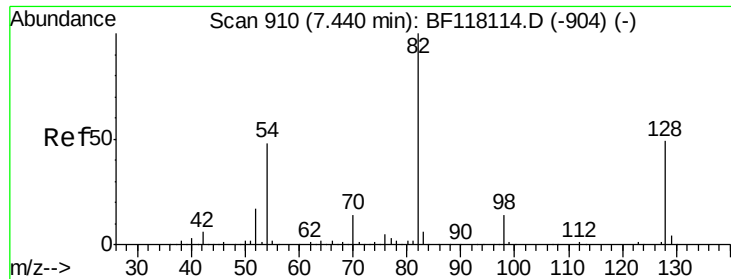




#23
Nitrobenzene-d5
Concen: 89.078 ng
RT: 7.43 min Scan# 909
Delta R.T. -0.01 min
Lab File: BF118173.D
Acq: 10 Dec 2019 19:58

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
82	100		
128	49.6	39.1	58.7
54	46.2	38.2	57.2

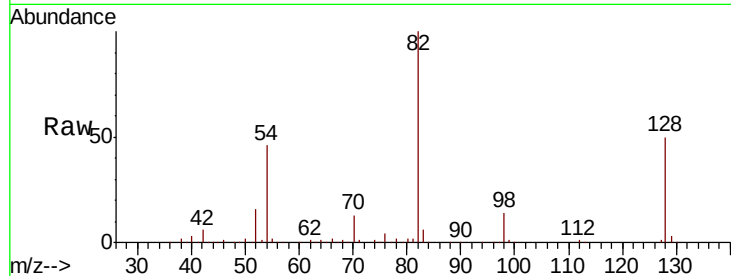


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): BF1
Ion 54.00 (53.70 to 54.70): BF1


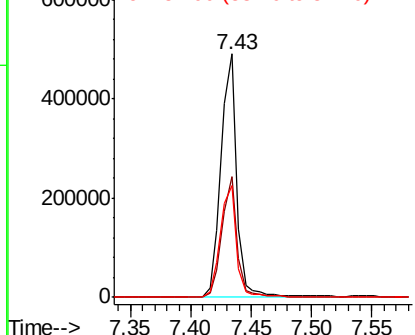



#25
Isophorone
Concen: 51.937 ng
RT: 7.43 min Scan# 909
Delta R.T. -0.26 min
Lab File: BF118173.D
Acq: 10 Dec 2019 19:58

Tgt Ion	Ratio	Lower	Upper
82	100		
95	0.0	6.3	9.5#
138	0.0	16.3	24.5#



Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 95.00 (94.70 to 95.70): BF1
Ion 138.00 (137.70 to 138.70): BF1

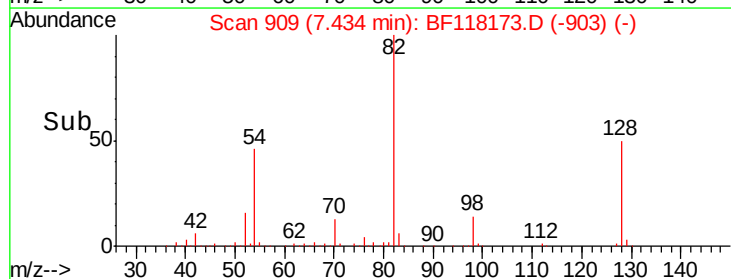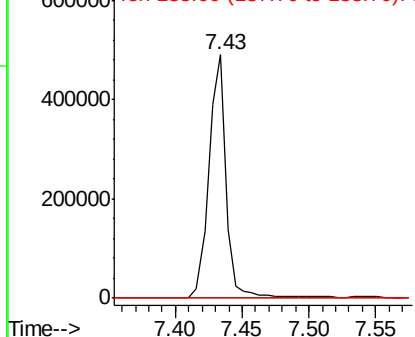


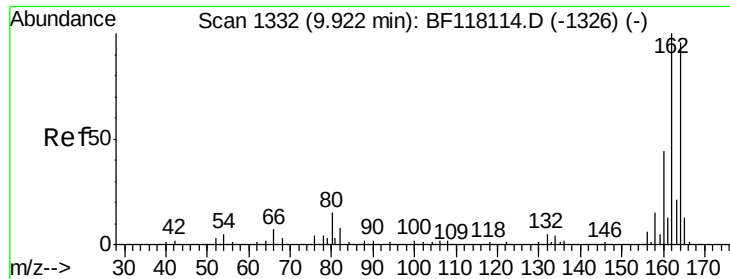




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.92 min Scan# 1331
Delta R.T. -0.01 min
Lab File: BF118173.D
Acq: 10 Dec 2019 19:58

Instrument :
BNA_F
ClientSampleId :

Tot Ion:164 Resp: 136952
Ion Ratio Lower Upper
164 100
162 104.7 83.4 125.0
160 45.4 36.6 54.8

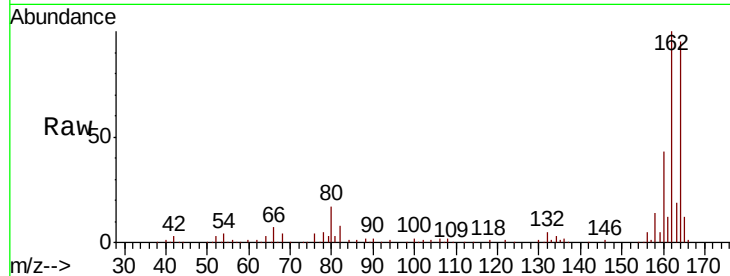


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

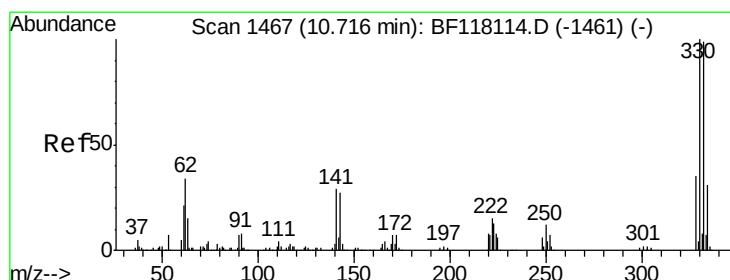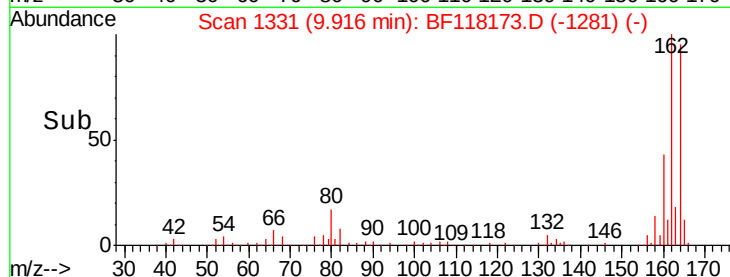
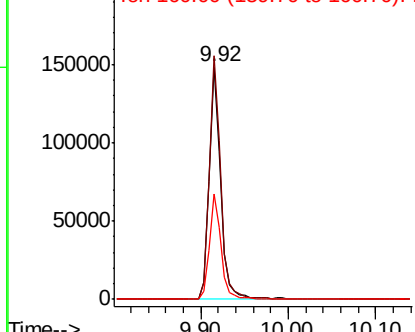



#42
2,4,6-Tribromophenol
Concen: 129.465 ng
RT: 10.71 min Scan# 1466
Delta R.T. -0.01 min
Lab File: BF118173.D
Acq: 10 Dec 2019 19:58

Tgt Ion:330 Resp: 215393
Ion Ratio Lower Upper
330 100
332 97.9 78.1 117.1
141 33.6 26.9 40.3

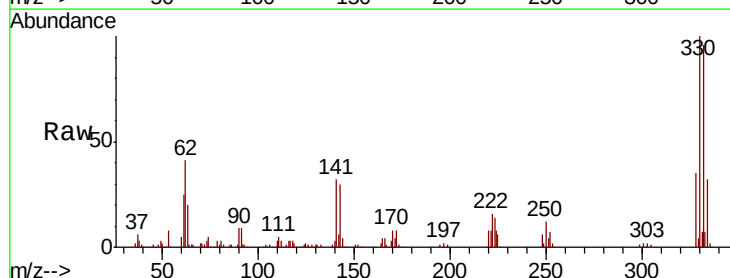

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

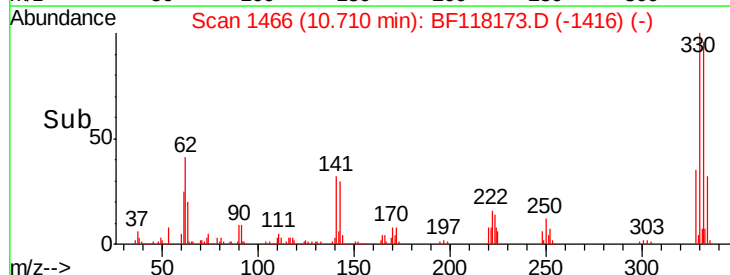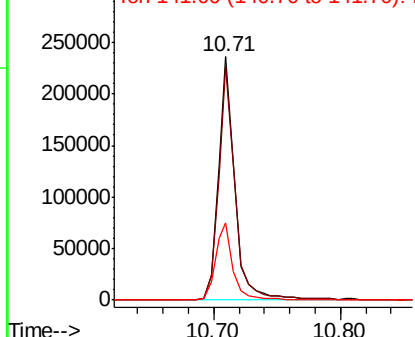







#45
 2-Fluorobiphenyl
 Concen: 98.912 ng
 RT: 9.23 min Scan# 1215
 Delta R.T. -0.01 min
 Lab File: BF118173.D
 Acq: 10 Dec 2019 19:58

Instrument :
 BNA_F
 ClientSampled :

Tot Ion:172 Resp: 890234
 Ion Ratio Lower Upper
 172 100
 171 36.4 29.2 43.8
 170 23.8 19.4 29.2




Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

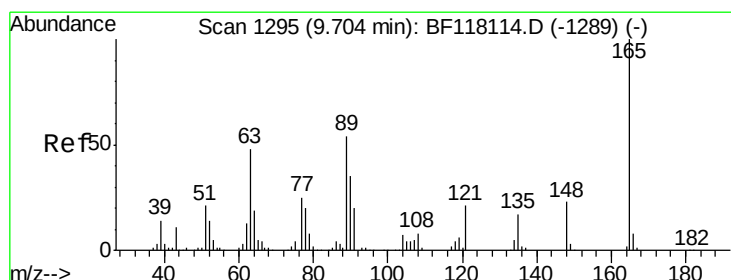
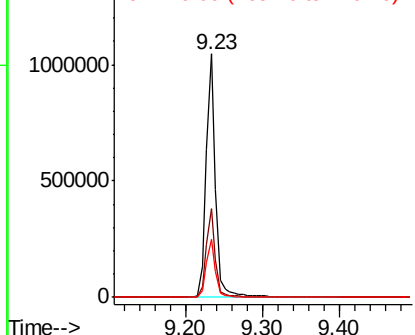



#51
 2,6-Dinitrotoluene
 Concen: 7.583 ng
 RT: 9.92 min Scan# 1331
 Delta R.T. 0.21 min
 Lab File: BF118173.D
 Acq: 10 Dec 2019 19:58

Tgt Ion:165 Resp: 16679
 Ion Ratio Lower Upper
 165 100
 63 2.2 41.4 62.0#
 89 1.7 42.9 64.3#



Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF1
 Ion 89.00 (88.70 to 89.70): BF1




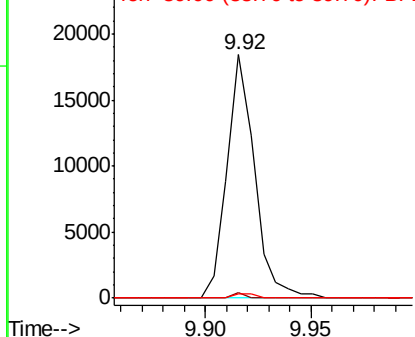


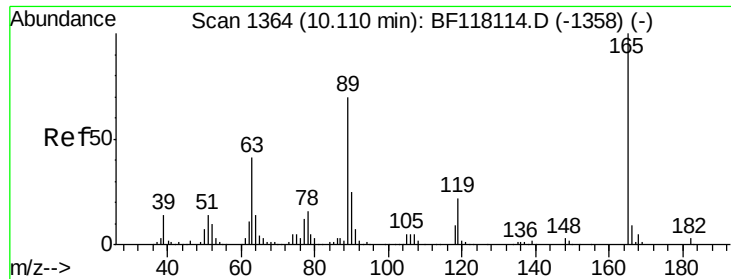

#57
 2,4-Dinitrotoluene
 Concen: 5.681 ng
 RT: 9.92 min Scan# 1331
 Delta R.T. -0.19 min
 Lab File: BF118173.D
 Acq: 10 Dec 2019 19:58




Instrument :
 BNA_F
 ClientSampled :


Tot Ion	Ratio	Lower	Upper
165	100		
63	2.2	32.6	49.0#
89	1.7	56.1	84.1#
182	0.0	2.1	3.1#

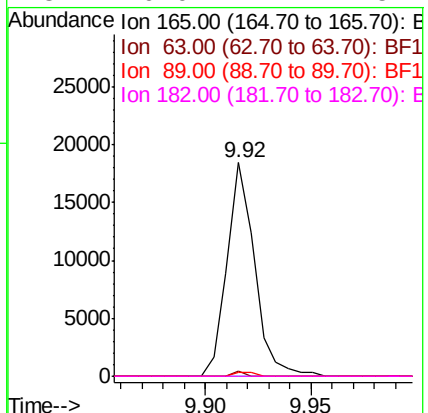

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.41 min Scan# 1585
 Delta R.T. -0.00 min
 Lab File: BF118173.D
 Acq: 10 Dec 2019 19:58

Tgt Ion	Ratio	Lower	Upper
188	100		
94	8.3	7.1	10.7
80	8.2	7.9	11.9

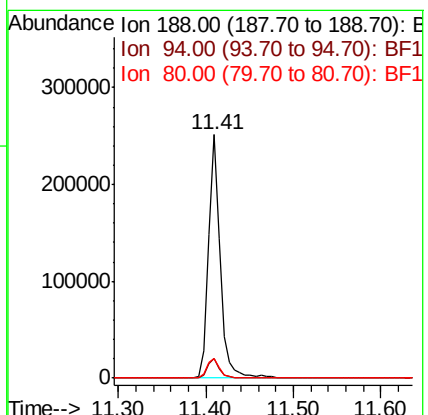


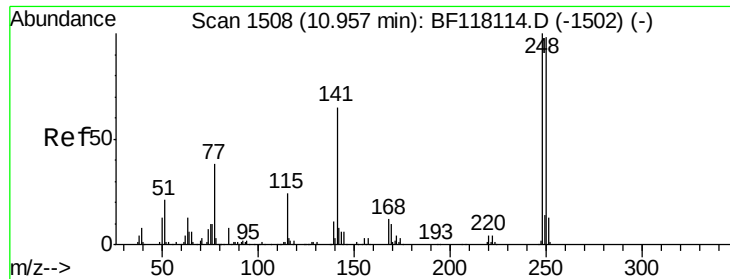




#67
4-Bromophenyl-phenylether
Concen: 4.849 ng
RT: 10.71 min Scan# 1466
Delta R.T. -0.25 min
Lab File: BF118173.D
Acq: 10 Dec 2019 19:58

Instrument :
BNA_F
ClientSampleId :

Tot Ion:248 Resp: 13120
Ion Ratio Lower Upper
248 100
250 184.8 78.3 117.5#
141 489.3 52.2 78.4#

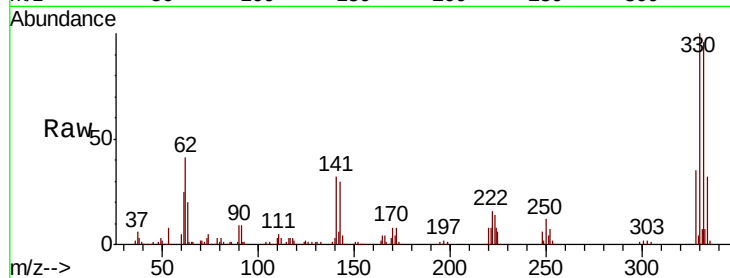


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

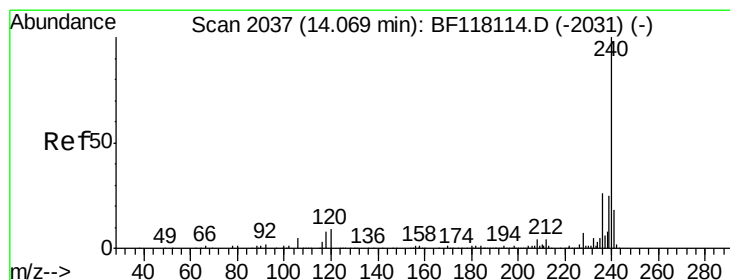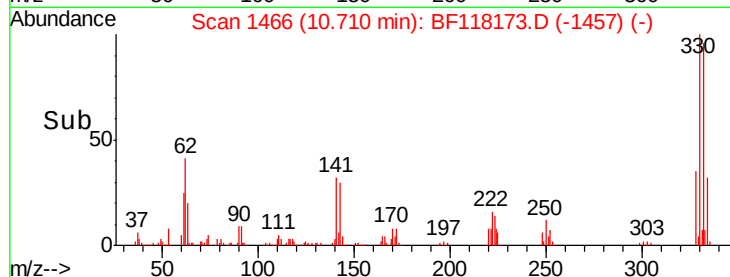
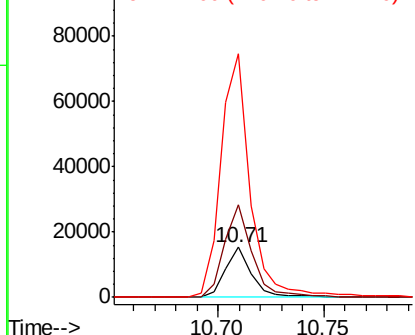



#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.06 min Scan# 2036
Delta R.T. -0.01 min
Lab File: BF118173.D
Acq: 10 Dec 2019 19:58

Tgt Ion:240 Resp: 188539
Ion Ratio Lower Upper
240 100
120 9.9 7.1 10.7
236 27.2 21.0 31.6

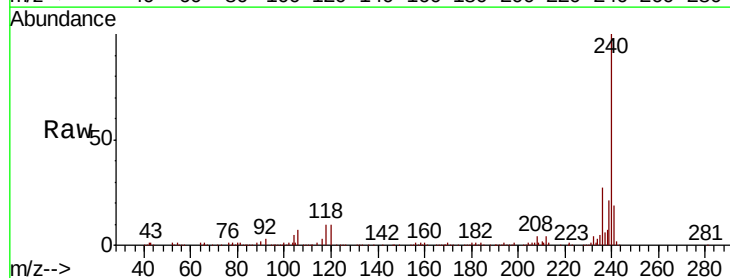

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

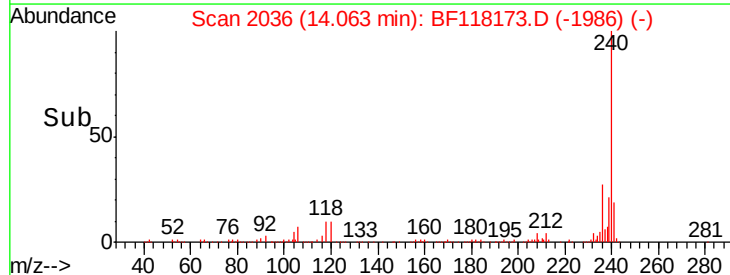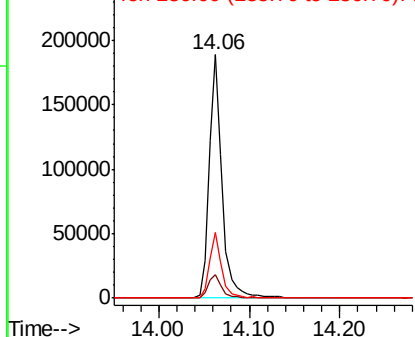



#77

Benzidine

Concen: 2.611 ng

RT: 13.00 min Scan# 1855

Delta R.T. 0.25 min

Lab File: BF118173.D

Acq: 10 Dec 2019 19:58

Instrument :

BNA_F

ClientSampleId :


Tot Ion:184 Resp: 12960

Ion Ratio Lower Upper




184 100

185 14.6 12.3 18.5

183 5.9 9.9 14.9#

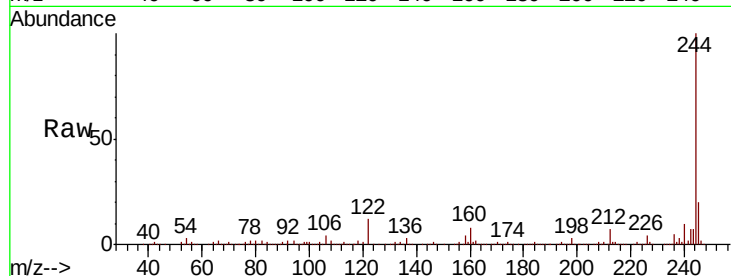

Abundance Ion 184.00 (183.70 to 184.70): E
Ion 185.00 (184.70 to 185.70): E
Ion 183.00 (182.70 to 183.70): E

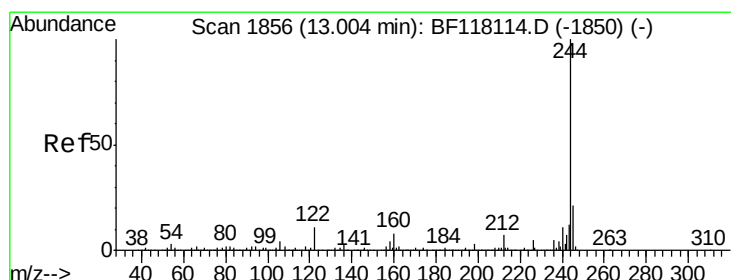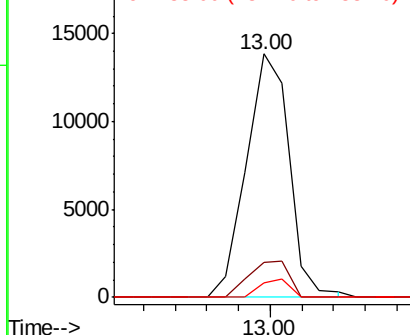

#79

Terphenyl-d14

Concen: 85.109 ng

RT: 13.00 min Scan# 1855

Delta R.T. -0.01 min

Lab File: BF118173.D

Acq: 10 Dec 2019 19:58


Tgt Ion:244 Resp: 933134

Ion Ratio Lower Upper



244 100


212 7.0 5.9 8.9

122 12.1 9.0 13.6



Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

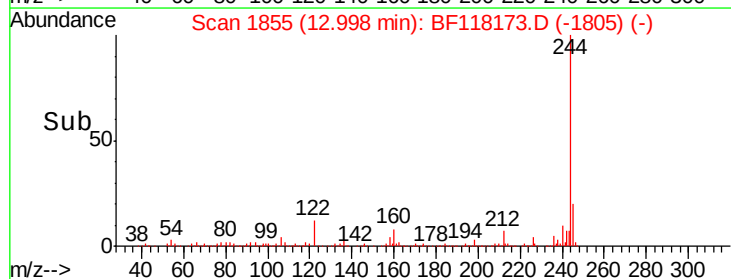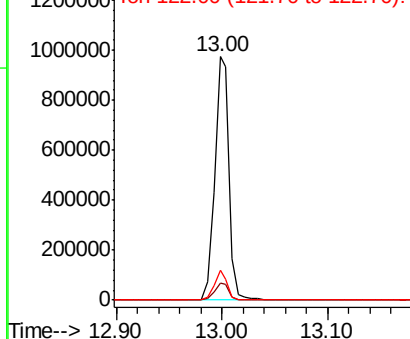

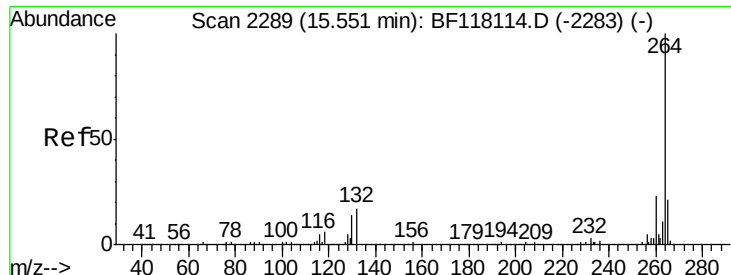

#87
Pervlene-d12
Concen: 20.000 ng
RT: 15.56 min Scan# 2290
Delta R.T. 0.01 min
Lab File: BF118173.D
Acq: 10 Dec 2019 19:58

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	22.5	18.6	28.0
265	20.2	16.8	25.2

