
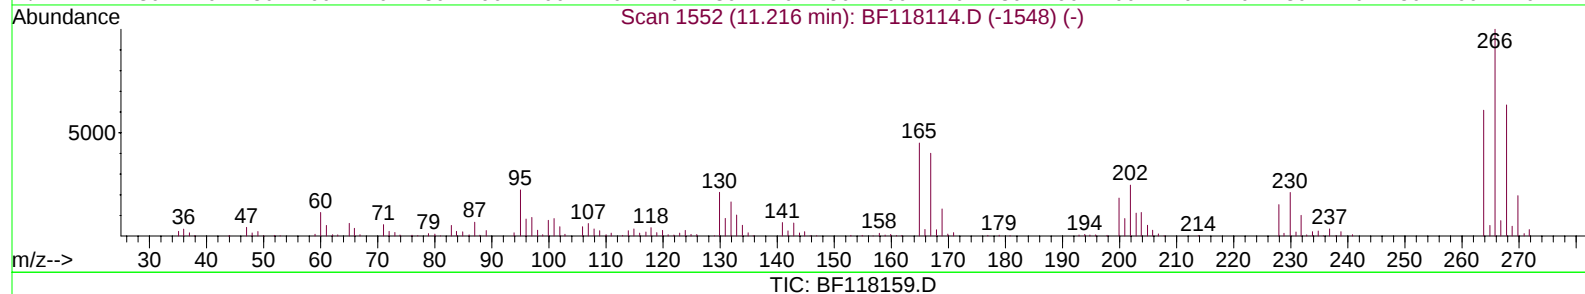
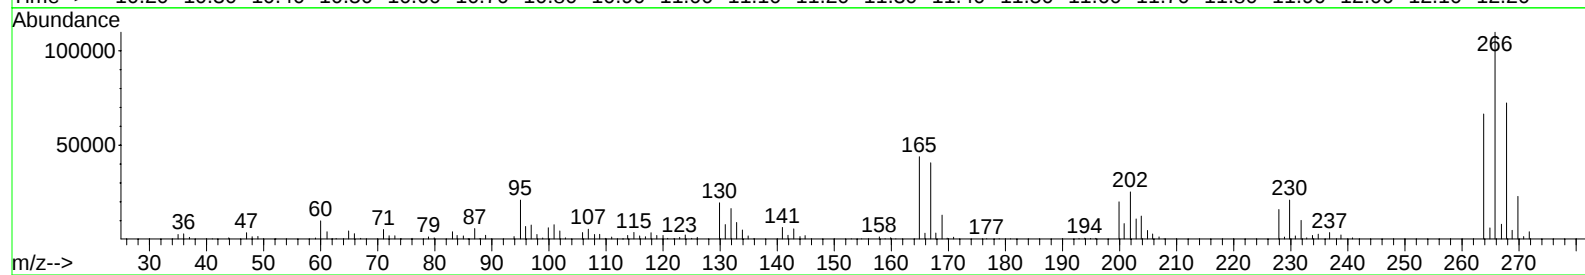


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF121019\
Data File : BF118159.D
Acq On : 10 Dec 2019 10:29
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 10 17:17:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF120619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 17:34:43 2019
Response via : Initial Calibration

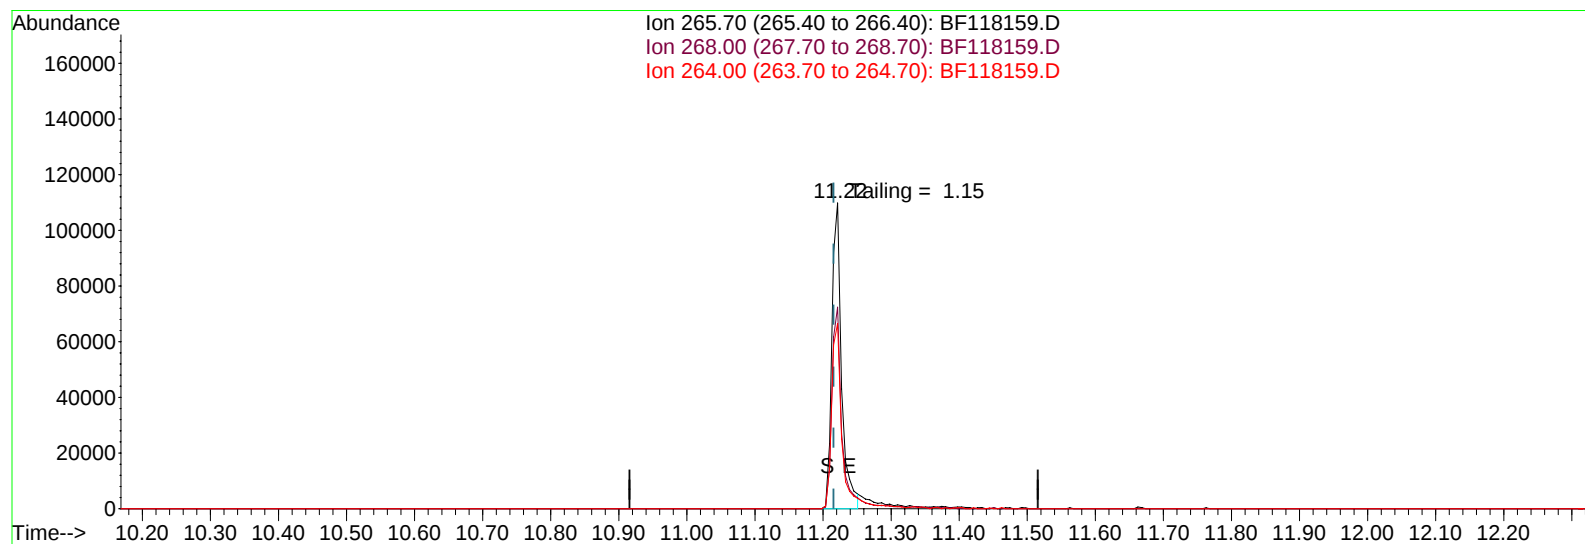

(70) Pentachlorophenol (C)




11.221min (+0.006) 39769.98ng

response 117603

Ion	Exp%	Act%
265.70	100	100
268.00	63.40	65.91
264.00	60.90	60.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF121019\
Data File : BF118159.D
Acq On : 10 Dec 2019 10:29
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 10 17:17:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF120619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 17:34:43 2019
Response via : Initial Calibration

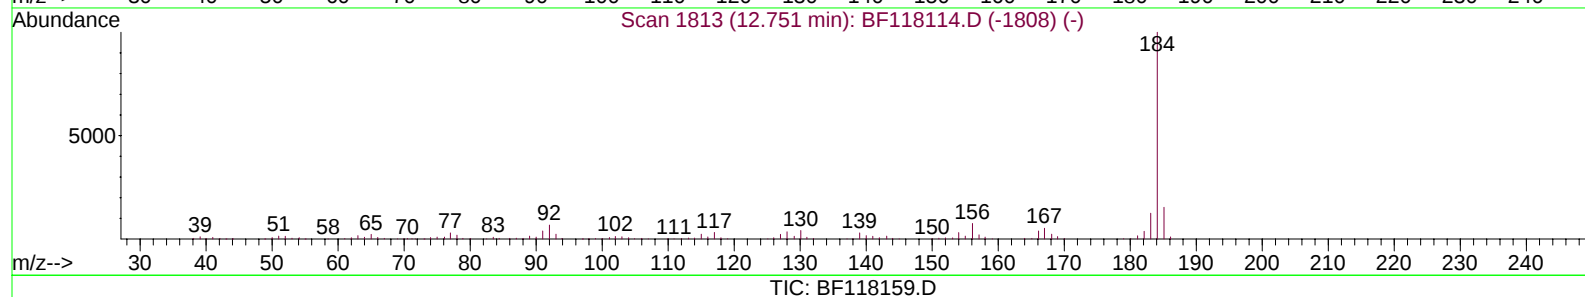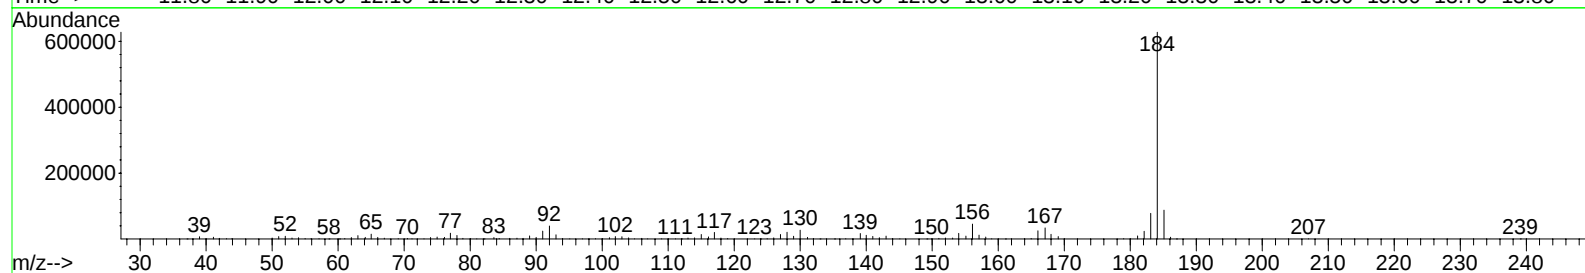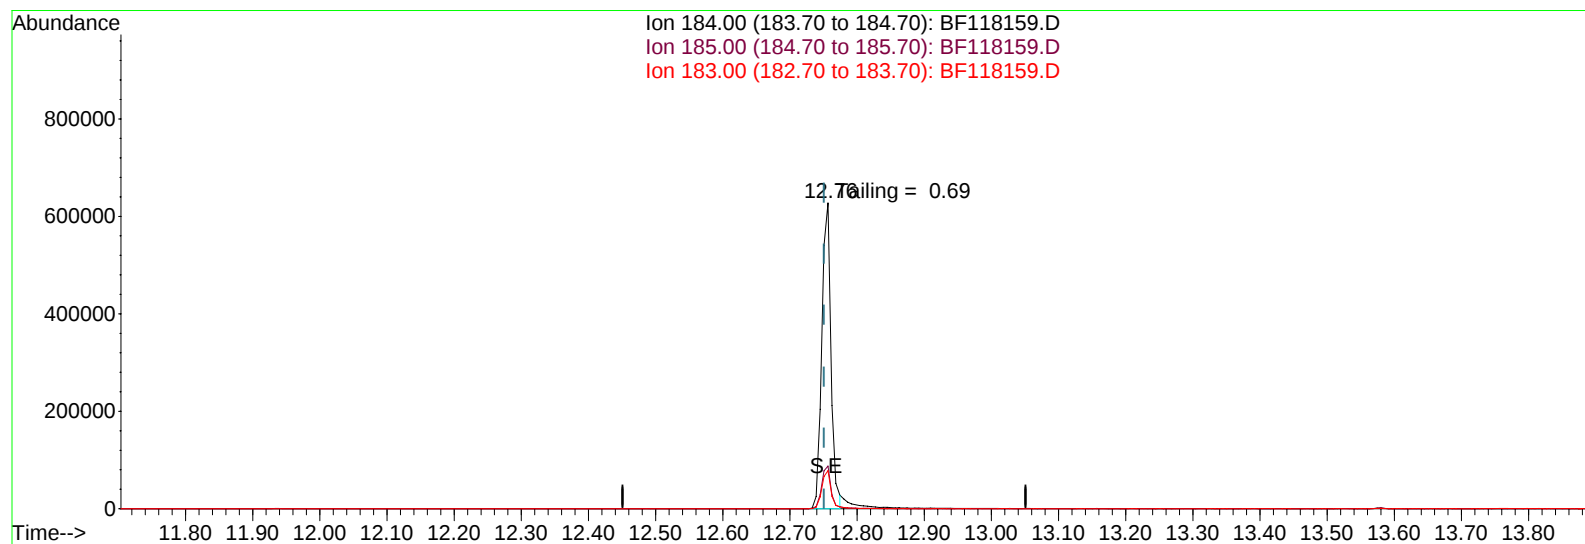

TIC: BF118159.D

(77) Benzidine

12.757min (+0.006) 143411.94ng

response 630482

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	13.99
183.00	12.40	12.46
0.00	0.00	0.00