


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF121019\
Data File : BF118159.D
Acq On : 10 Dec 2019 10:29
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120619.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 06 17:34:43 2019

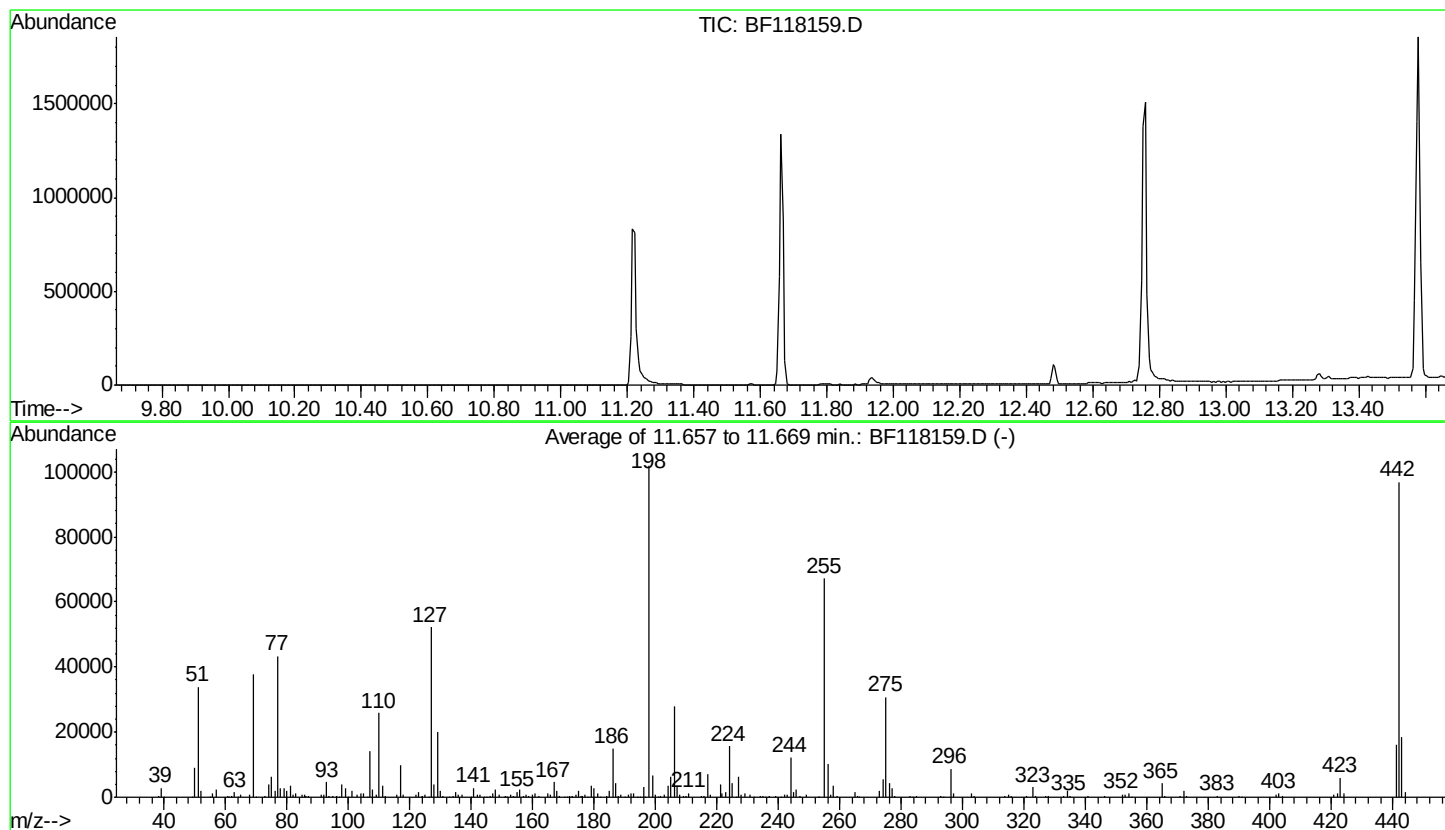

AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	33928	PASS
68	69	0.00	2	2.0	767	PASS
69	198	0.00	100	37.2	37840	PASS
70	69	0.00	2	0.3	123	PASS
127	198	10	80	51.3	52213	PASS
197	198	0.00	2	0.2	170	PASS
198	198	100	100	100.0	101856	PASS
199	198	5	9	6.5	6663	PASS
275	198	10	60	30.2	30728	PASS
365	198	1	100	4.2	4291	PASS
441	198	0.01	100	15.8	16091	PASS
442	198	50	100	95.1	96869	PASS
443	442	15	24	19.0	18444	PASS