
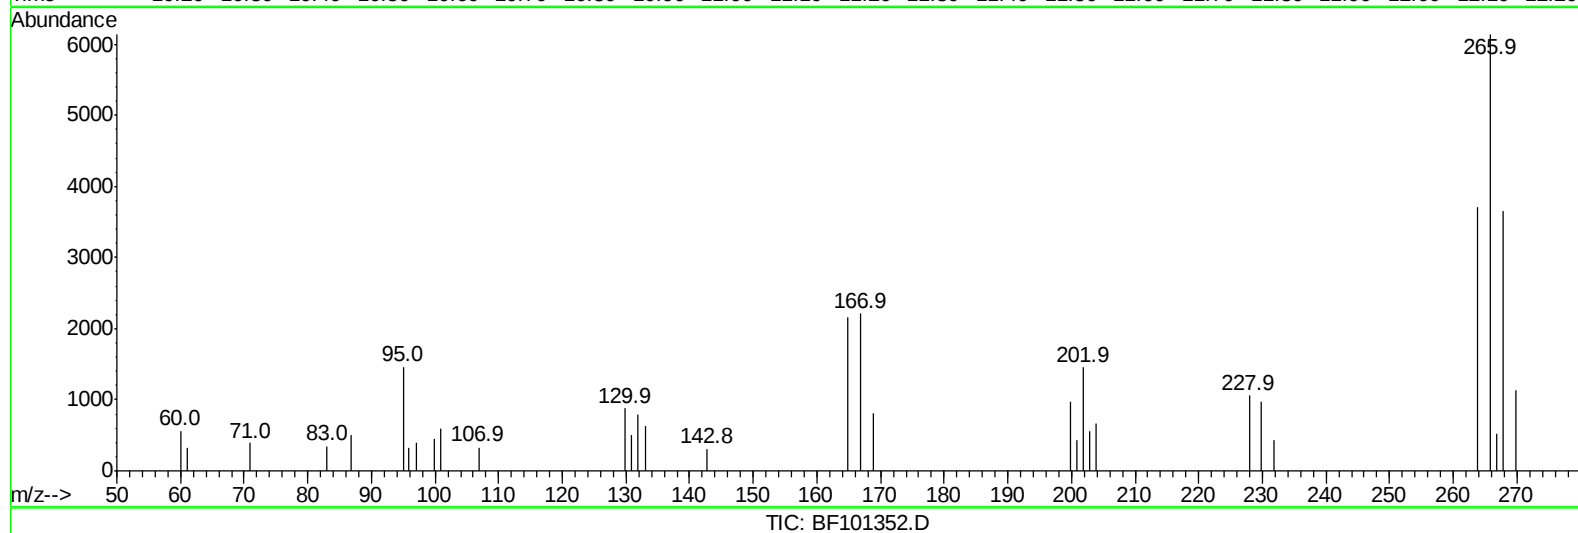


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121217\
Data File : BF101352.D
Acq On : 13 Dec 2017 2:16
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 13 07:39:08 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 08 18:17:31 2017
Response via : Initial Calibration

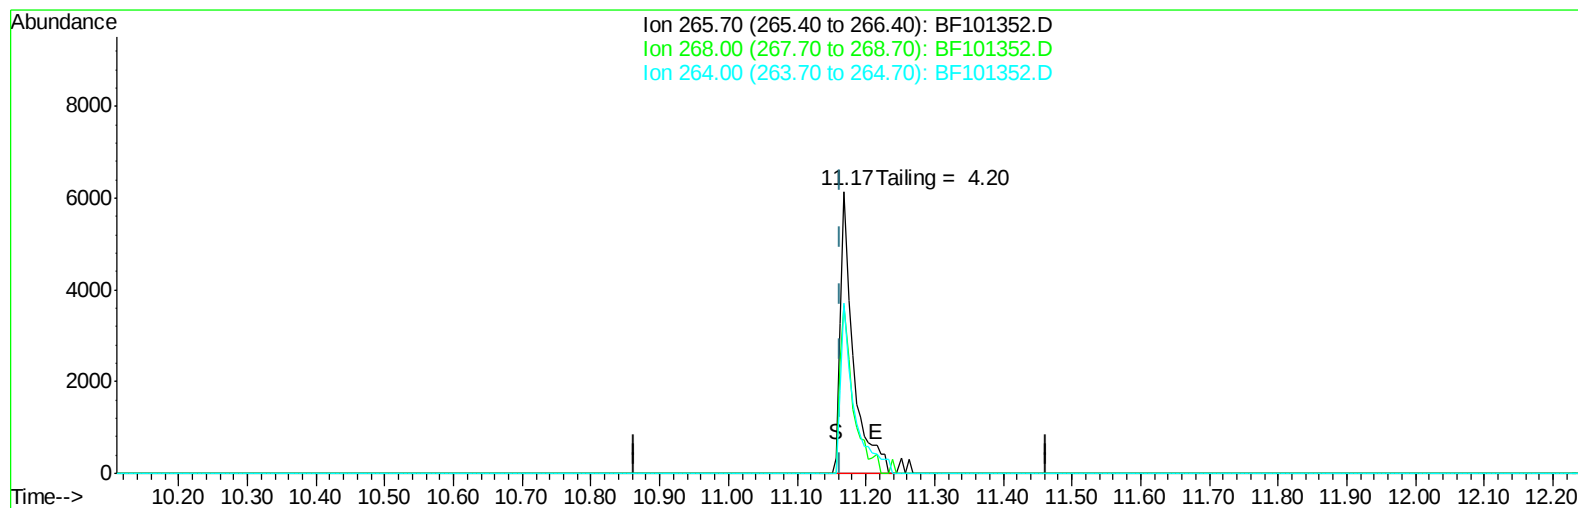

TIC: BF101352.D

(69) Pentachlorophenol (C)



11.169min (+0.006) 0.00ng

response 7874

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.44
264.00	61.90	60.40
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121217\
Data File : BF101352.D
Acq On : 13 Dec 2017 2:16
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 13 07:39:08 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 08 18:17:31 2017
Response via : Initial Calibration

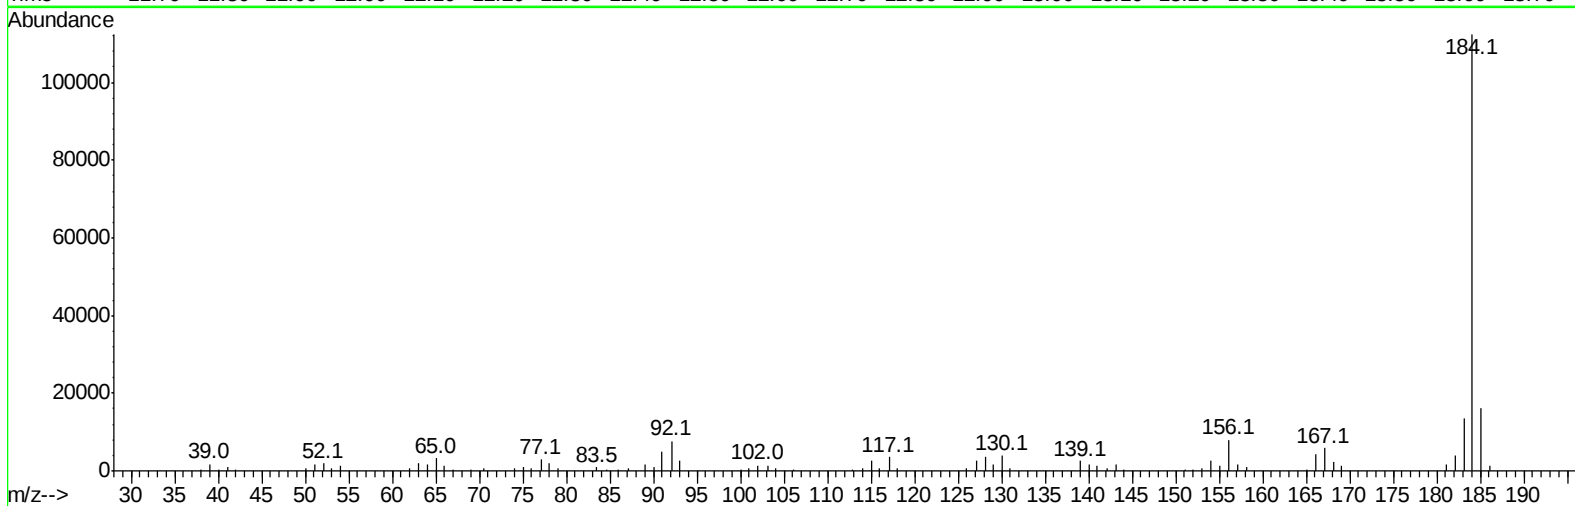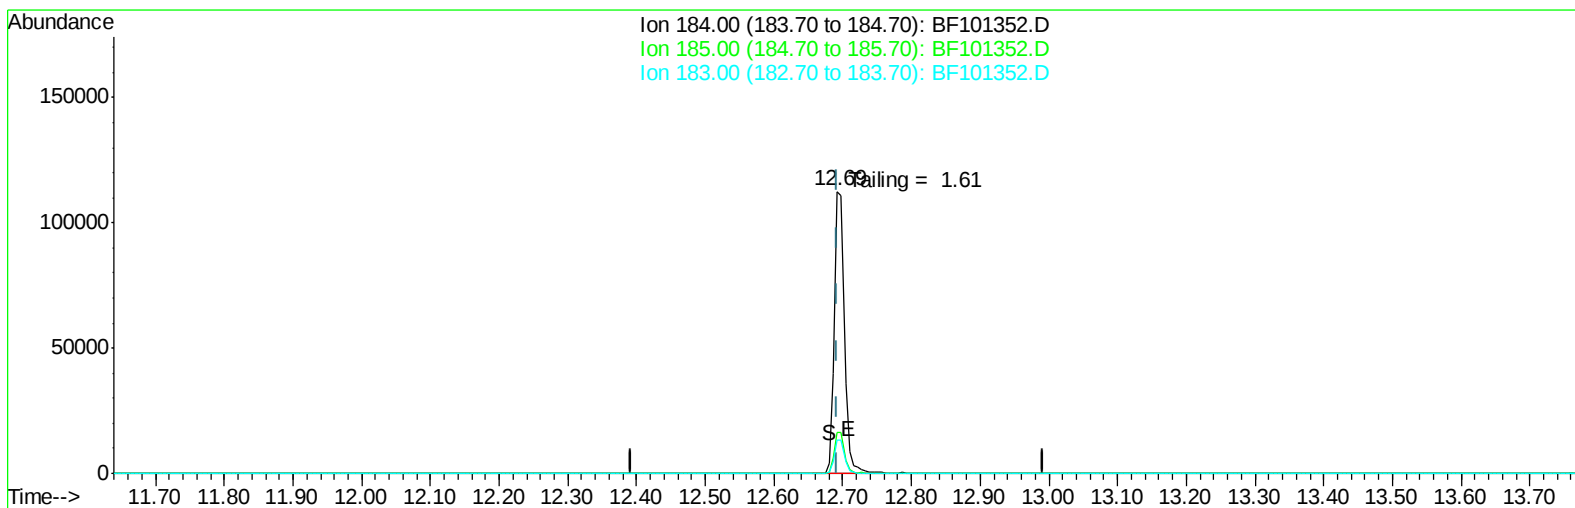

TIC: BF101352.D

(76) Benzidine

12.692min (+0.000) 0.00ng m

response 113627

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.49
183.00	11.60	11.99
0.00	0.00	0.00