


Data Path : Z:\HPCHEM1\BNA F\Data\BF121217\
 Data File : BF101352.D
 Acq On : 13 Dec 2017 2:16
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 08 18:17:31 2017

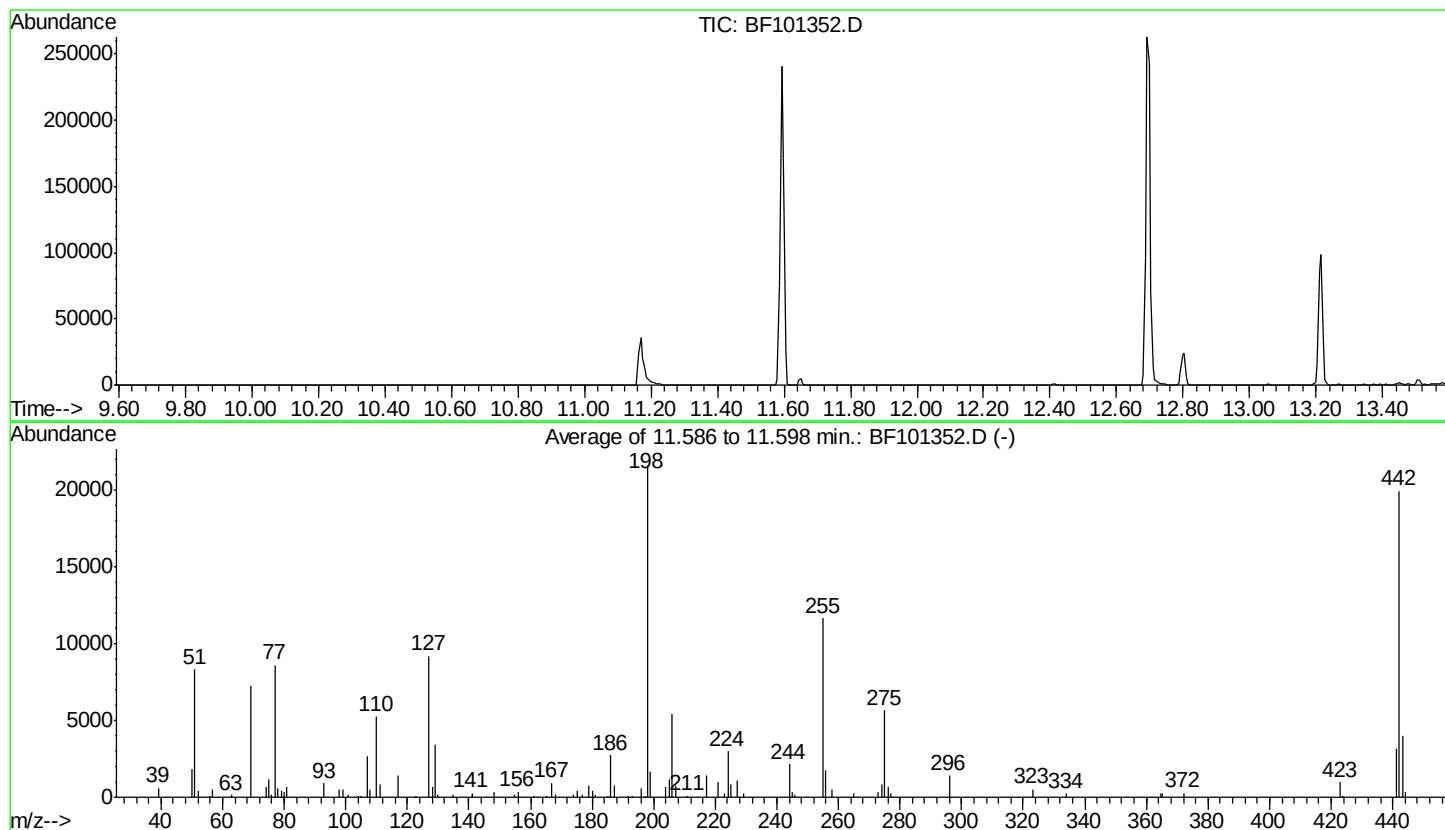

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1611

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	8334	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.5	7230	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.5	9170	PASS
197	198	0.00	2	0.5	107	PASS
198	198	100	100	100.0	21590	PASS
199	198	5	9	7.7	1652	PASS
275	198	10	60	26.1	5637	PASS
365	198	1	100	1.3	279	PASS
441	443	0.01	100	77.7	3130	PASS
442	198	50	100	92.4	19954	PASS
443	442	15	24	20.2	4026	PASS