
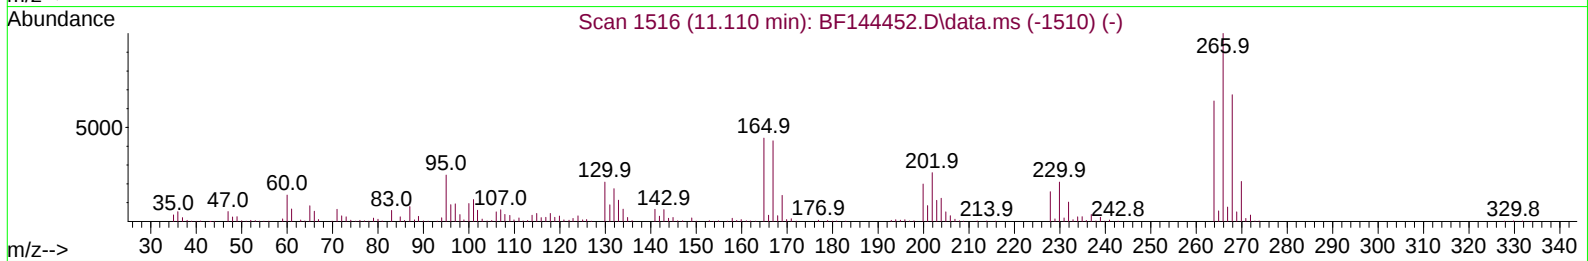
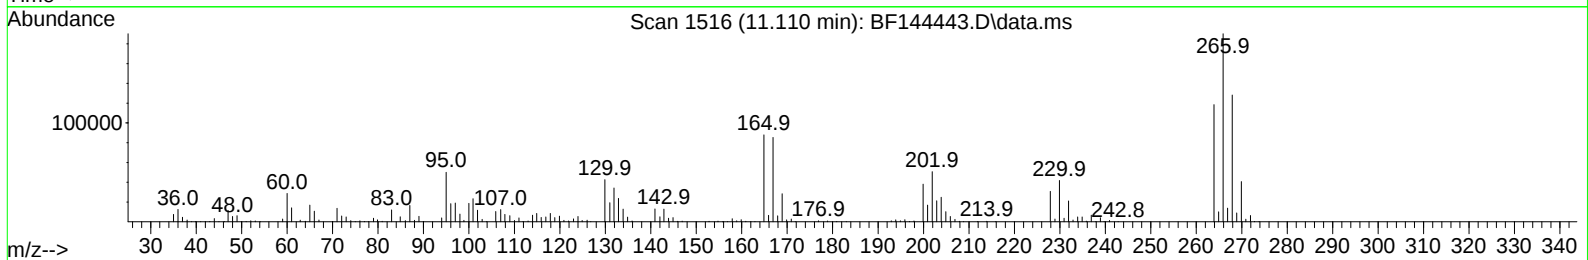


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121225\
Data File : BF144443.D
Acq On : 12 Dec 2025 10:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 12 17:05:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 15:57:03 2025
Response via : Initial Calibration

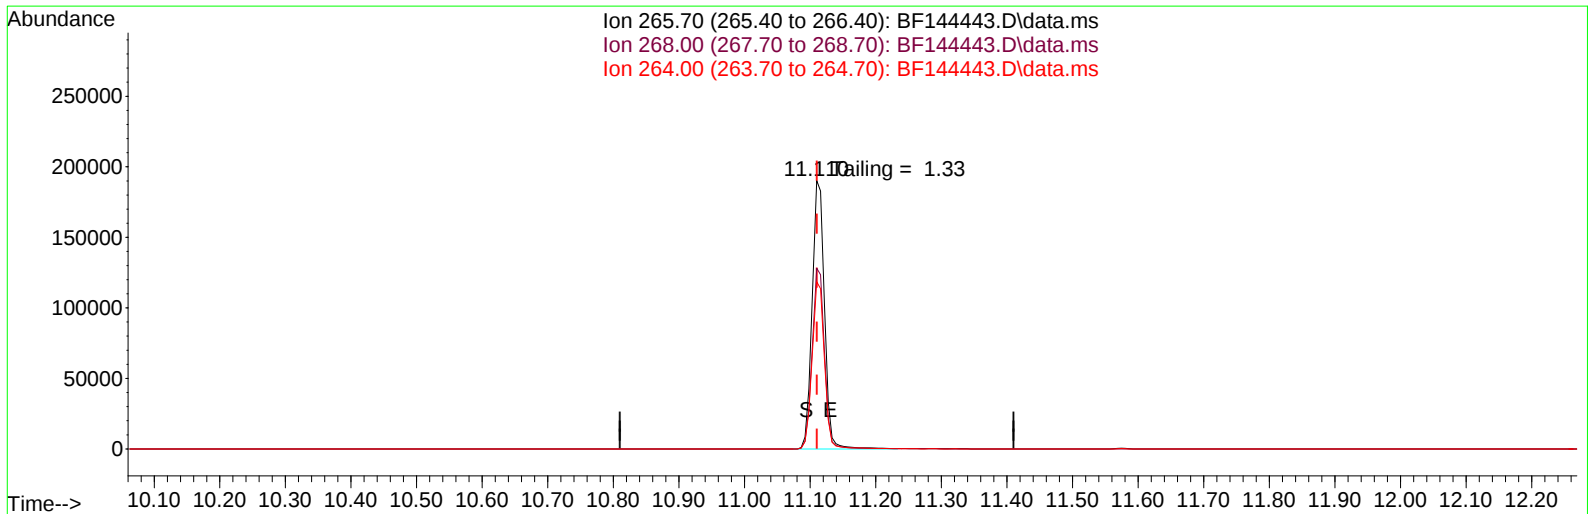

TIC: BF144443.D\data.ms

(70) Pentachlorophenol (C)




11.110min (-0.000) 22971.43 ng

response 249570

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.30	67.36
264.00	64.00	62.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121225\
Data File : BF144443.D
Acq On : 12 Dec 2025 10:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 12 17:05:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 15:57:03 2025
Response via : Initial Calibration

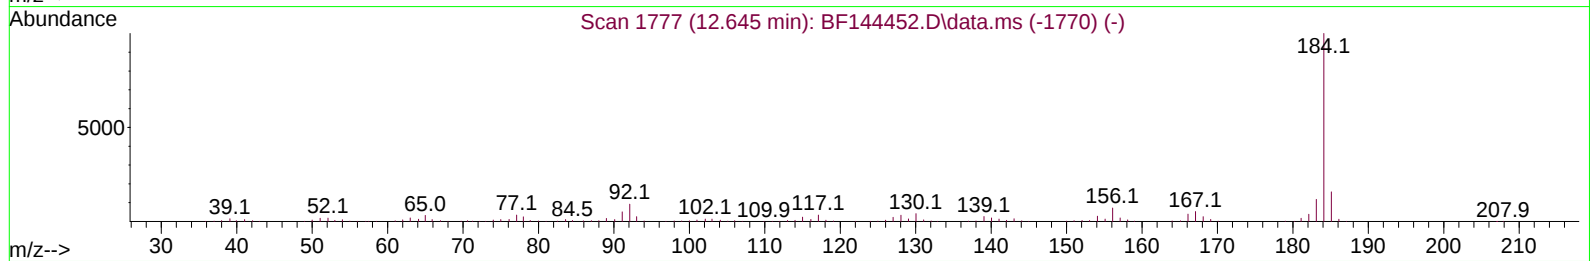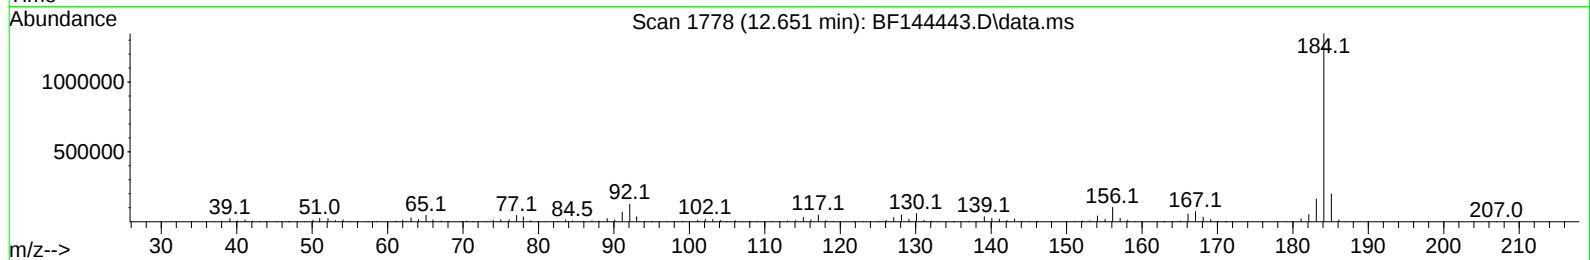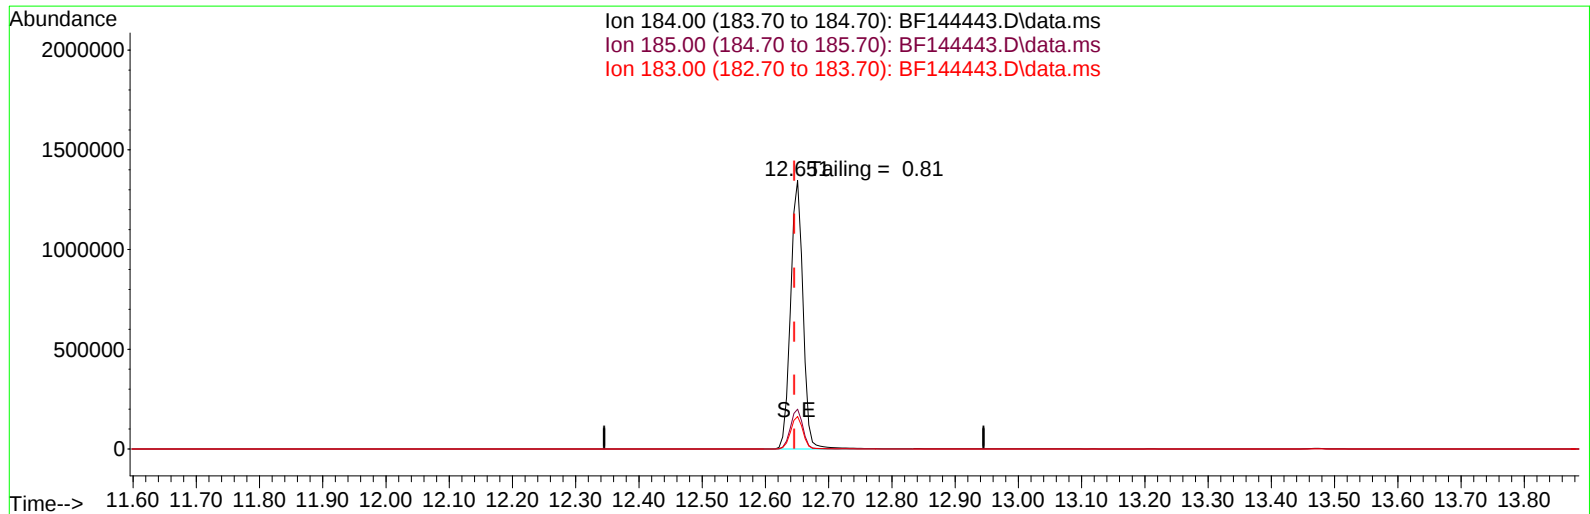

TIC: BF144443.D\data.ms

(77) Benzidine

12.651min (+ 0.006) 0.00 ng

response 1848697

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.80
183.00	11.70	12.11
0.00	0.00	0.00