


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121225\
Data File : BF144443.D
Acq On : 12 Dec 2025 10:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 12 15:57:03 2025

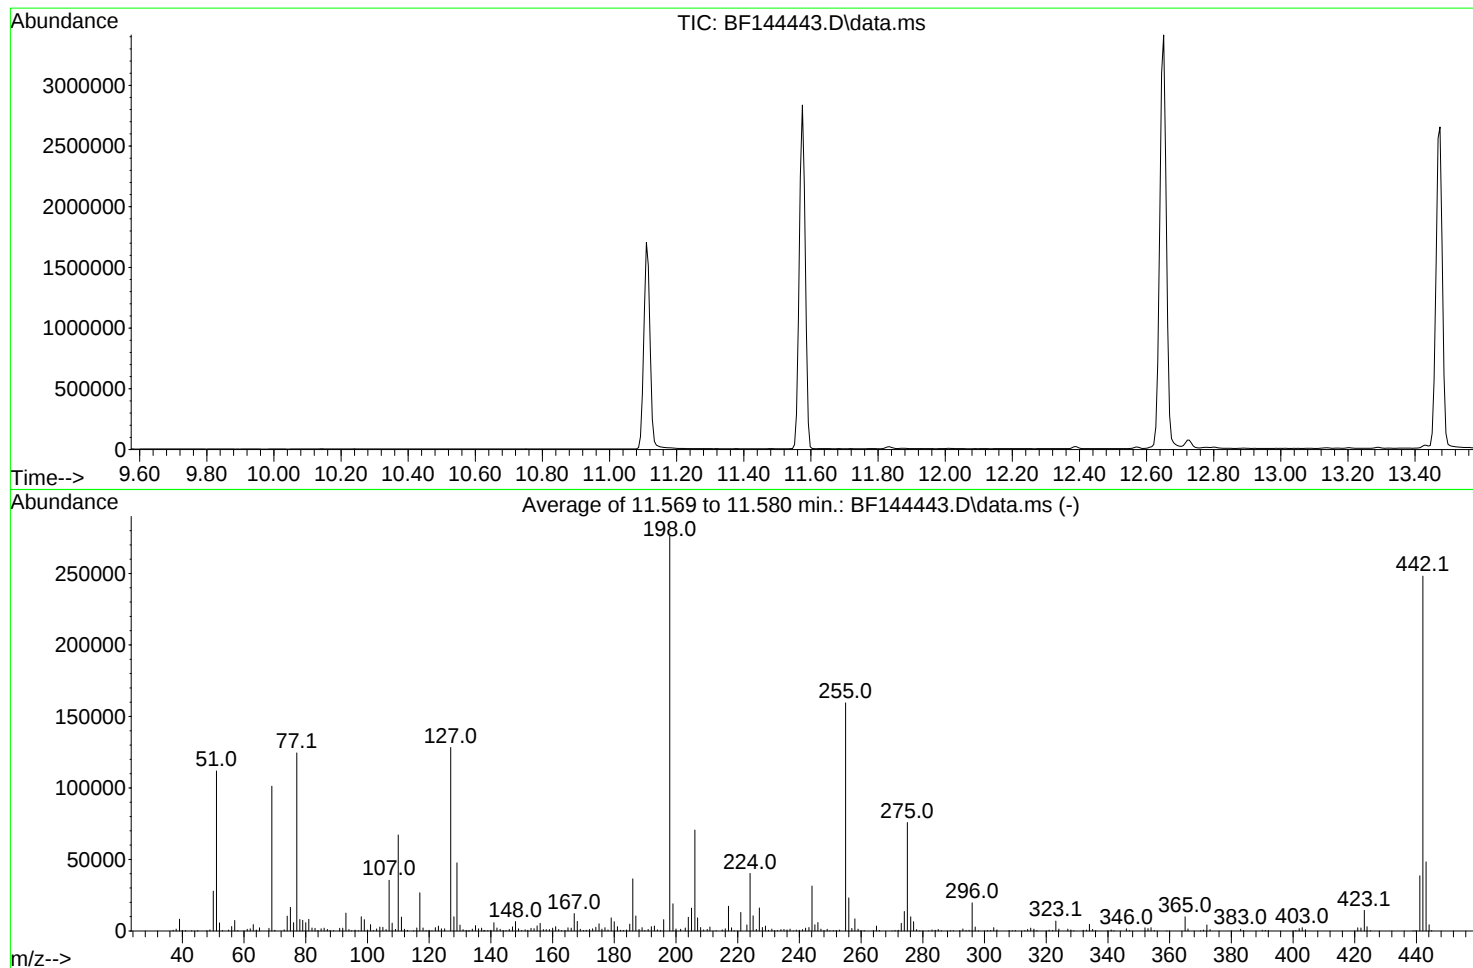




AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1587

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.9	1890	PASS
69	69	100	100	100.0	101219	PASS
70	69	0.00	2	0.5	513	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	276160	PASS
199	198	5	9	6.9	18955	PASS
365	198	1	100	3.6	9856	PASS
441	443	0.01	150	79.8	38533	PASS
442	442	100	100	100.0	248192	PASS
443	442	15	24	19.4	48267	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121225\
Data File : BF144443.D
Acq On : 12 Dec 2025 10:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 12 17:05:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 15:57:03 2025
Response via : Initial Calibration

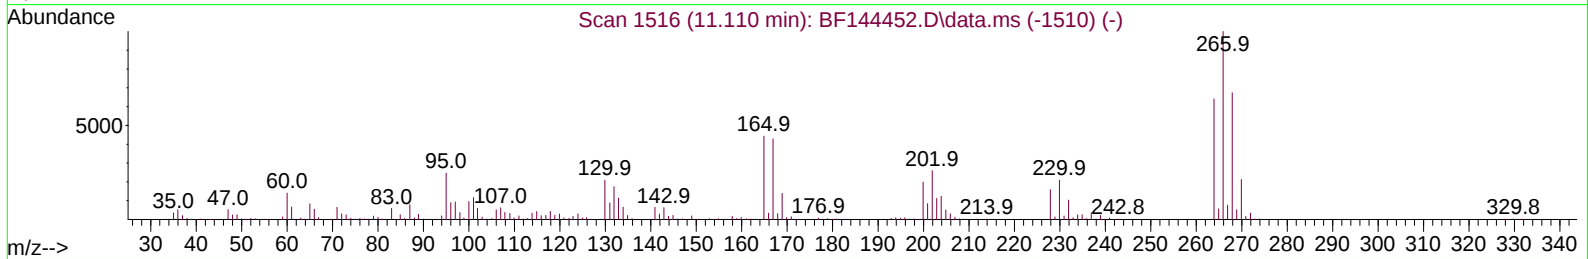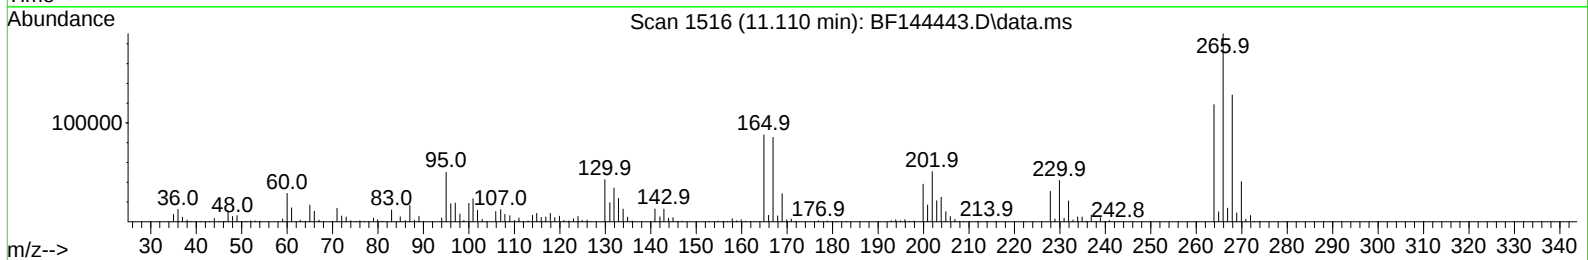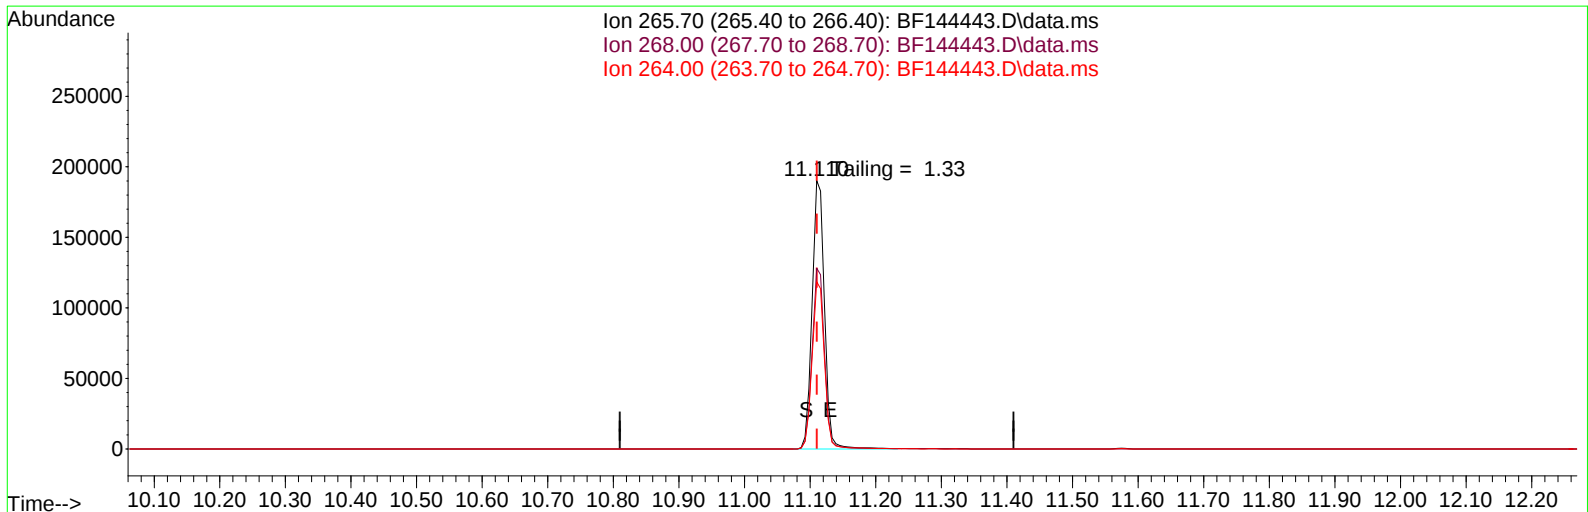

TIC: BF144443.D\data.ms

(70) Pentachlorophenol (C)

11.110min (-0.000) 22971.43 ng




response 249570

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.30	67.36
264.00	64.00	62.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121225\
Data File : BF144443.D
Acq On : 12 Dec 2025 10:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 12 17:05:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 15:57:03 2025
Response via : Initial Calibration

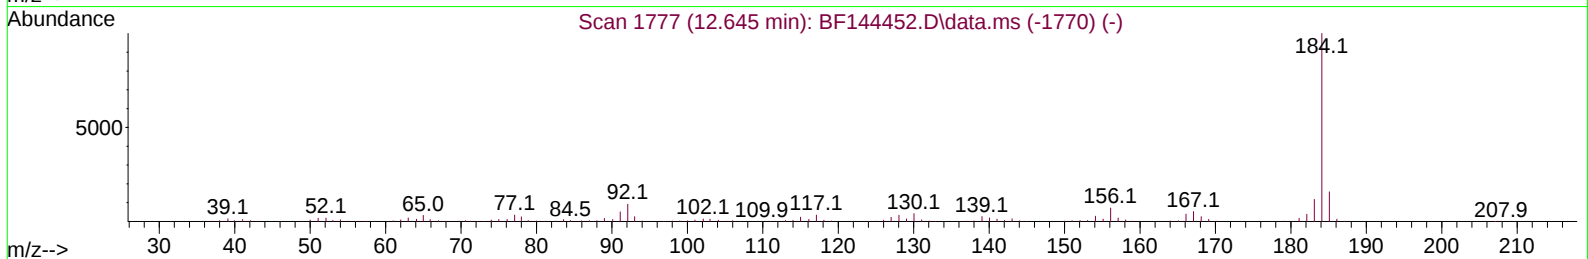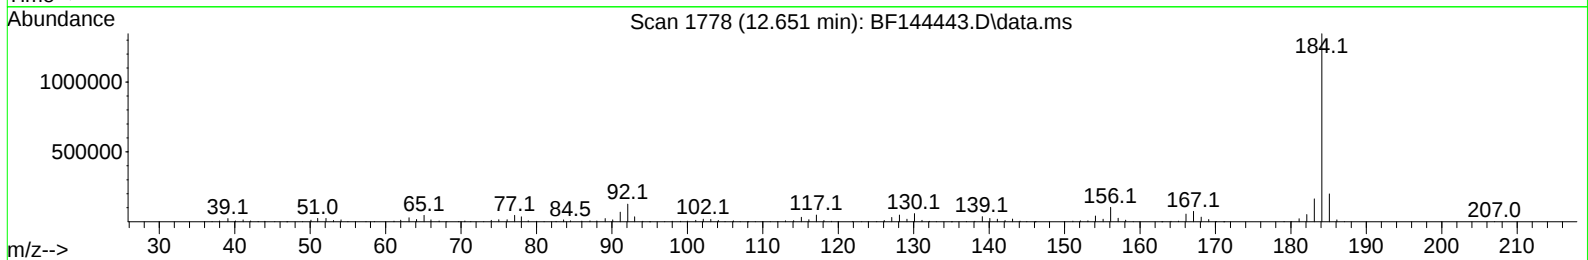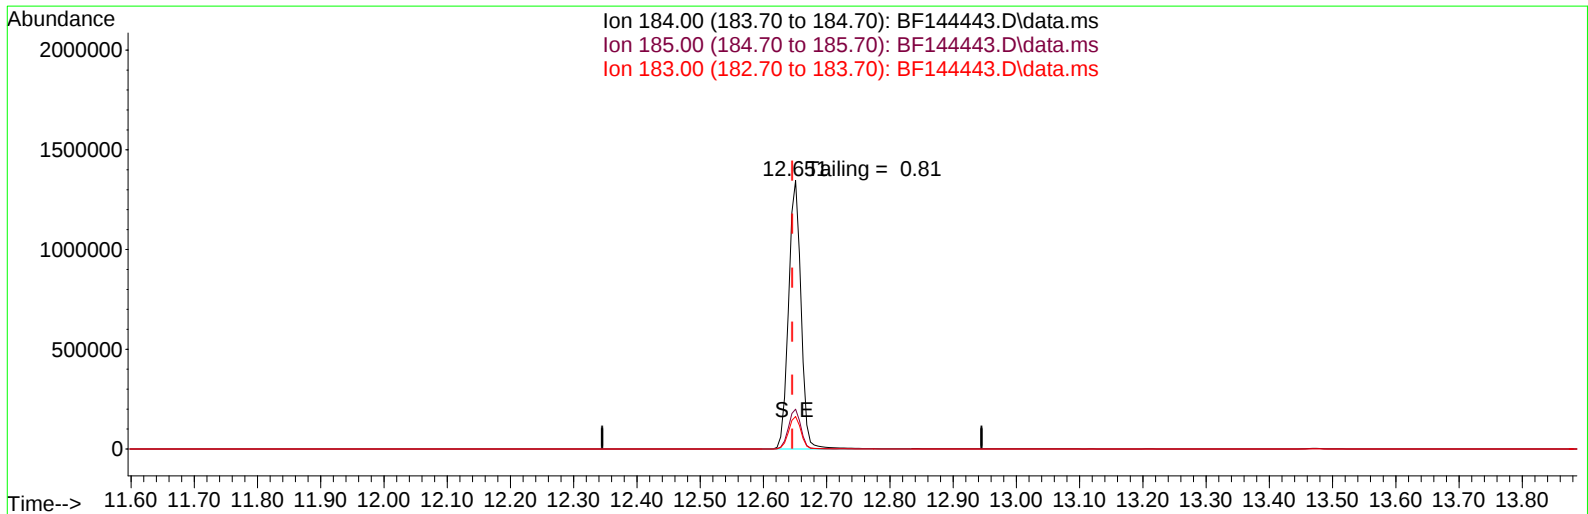

TIC: BF144443.D\data.ms

(77) Benzidine

12.651min (+ 0.006) 0.00 ng

response 1848697

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.80
183.00	11.70	12.11
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/12/2025	BNA_F	<u>BF144443.D</u>
Compound Name	Response	Retention Time
DDT	530974	13.474
DDD	2194	13.204
DDE	8450	11.574
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10644	541618	1.97

Instrument :
BNA_F
ClientSampleId :
DFTPP