
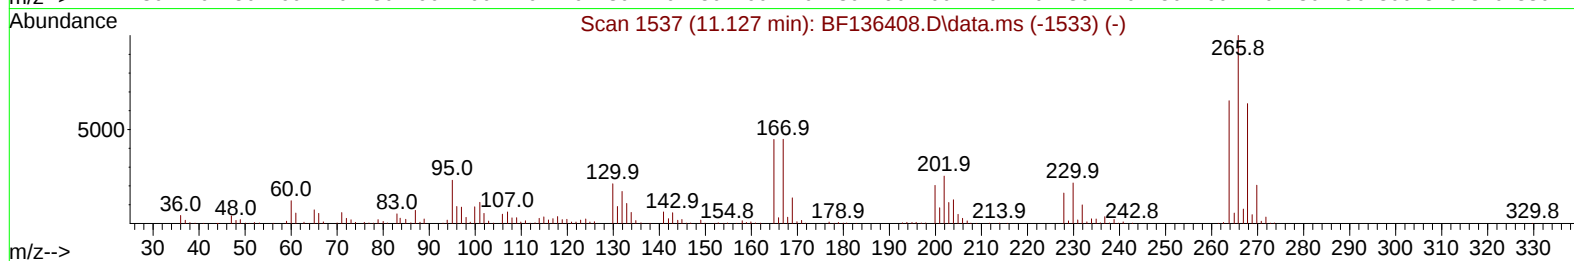
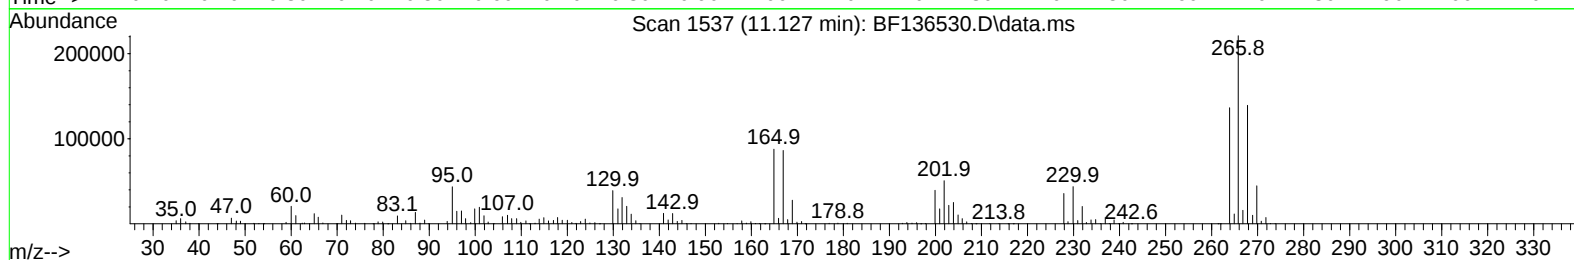


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121323\
Data File : BF136530.D
Acq On : 13 Dec 2023 10:50
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 13 12:05:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 06 09:40:27 2023
Response via : Initial Calibration

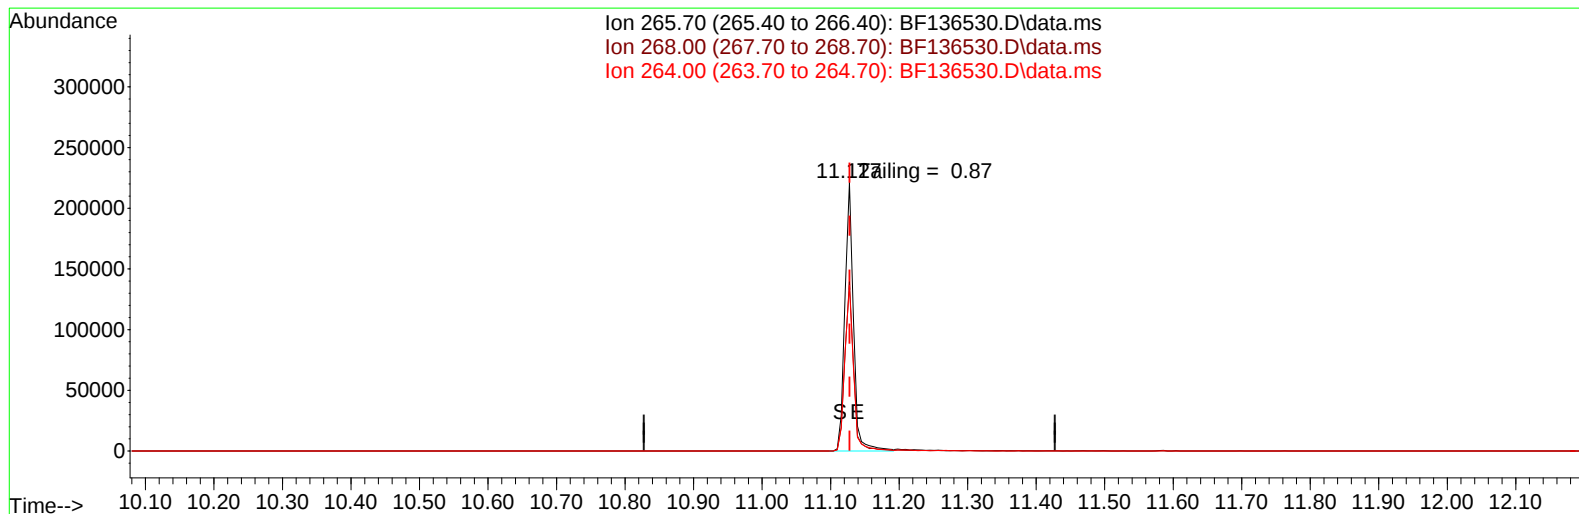

TIC: BF136530.D\data.ms

(70) Pentachlorophenol (C)




11.127min (-0.000) 23588.07 ng

response 192488

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.01
264.00	65.30	61.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121323\
Data File : BF136530.D
Acq On : 13 Dec 2023 10:50
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 13 12:05:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 06 09:40:27 2023
Response via : Initial Calibration

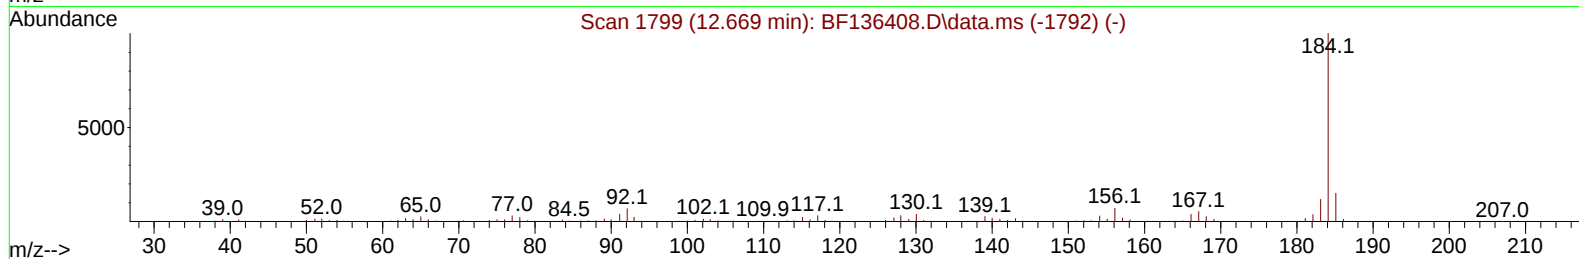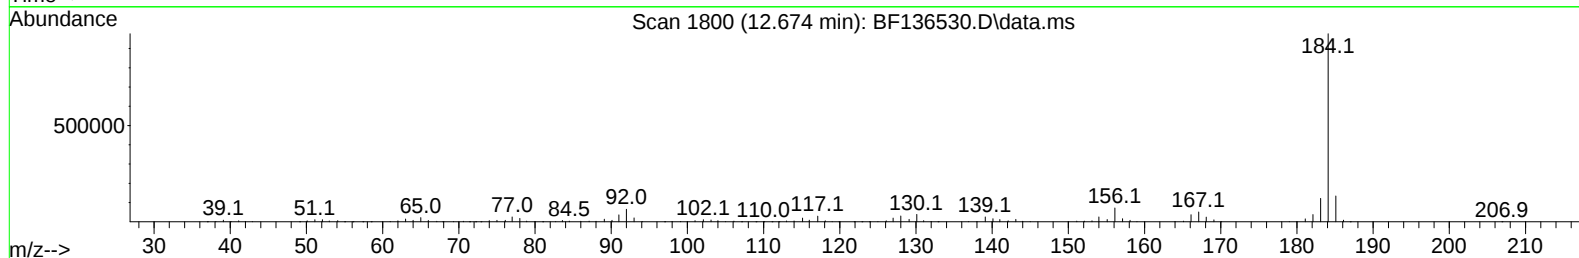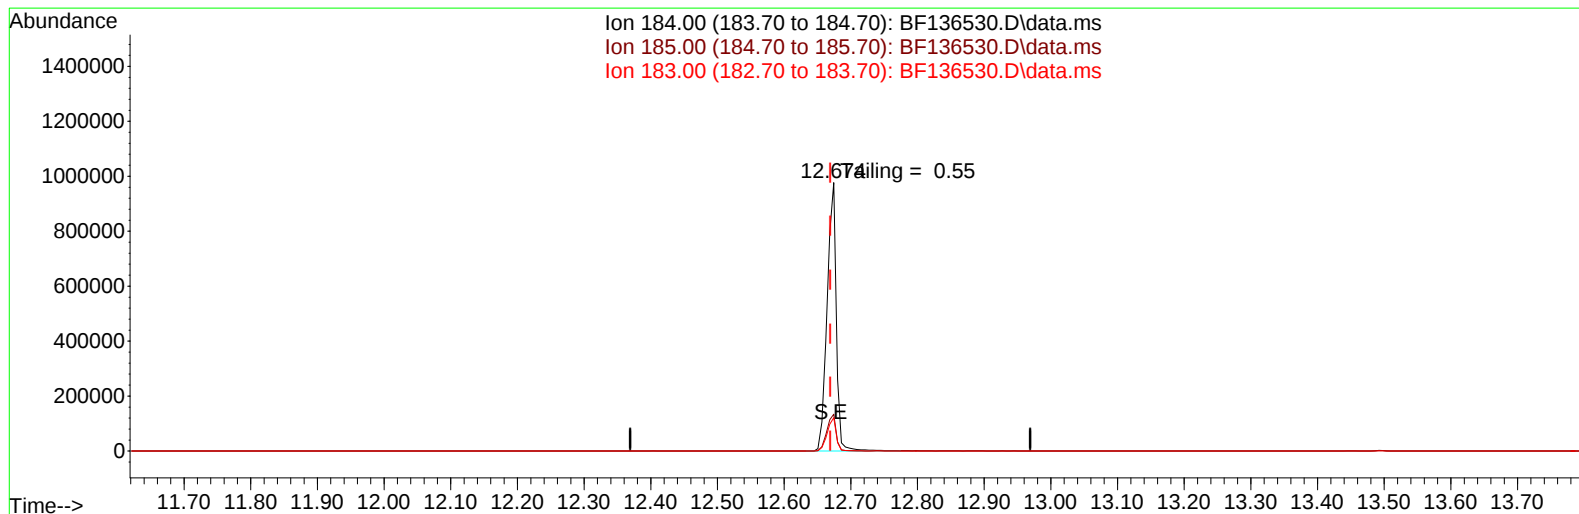

TIC: BF136530.D\data.ms

(77) Benzidine**12.674min (+ 0.005) 1638.06 ng****response 932869**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.71
183.00	11.70	12.44
0.00	0.00	0.00