
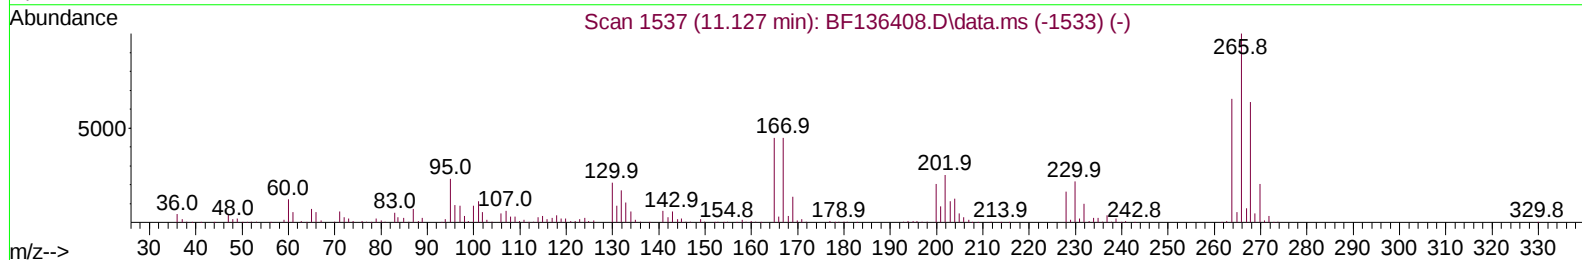
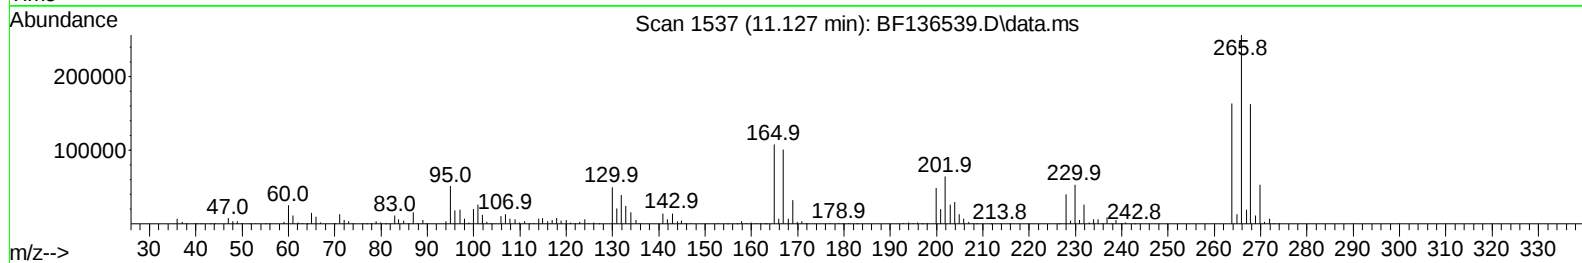


Quant Time: Dec 14 02:39:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : wed Dec 06 09:40:27 2023
Response via : Initial Calibration

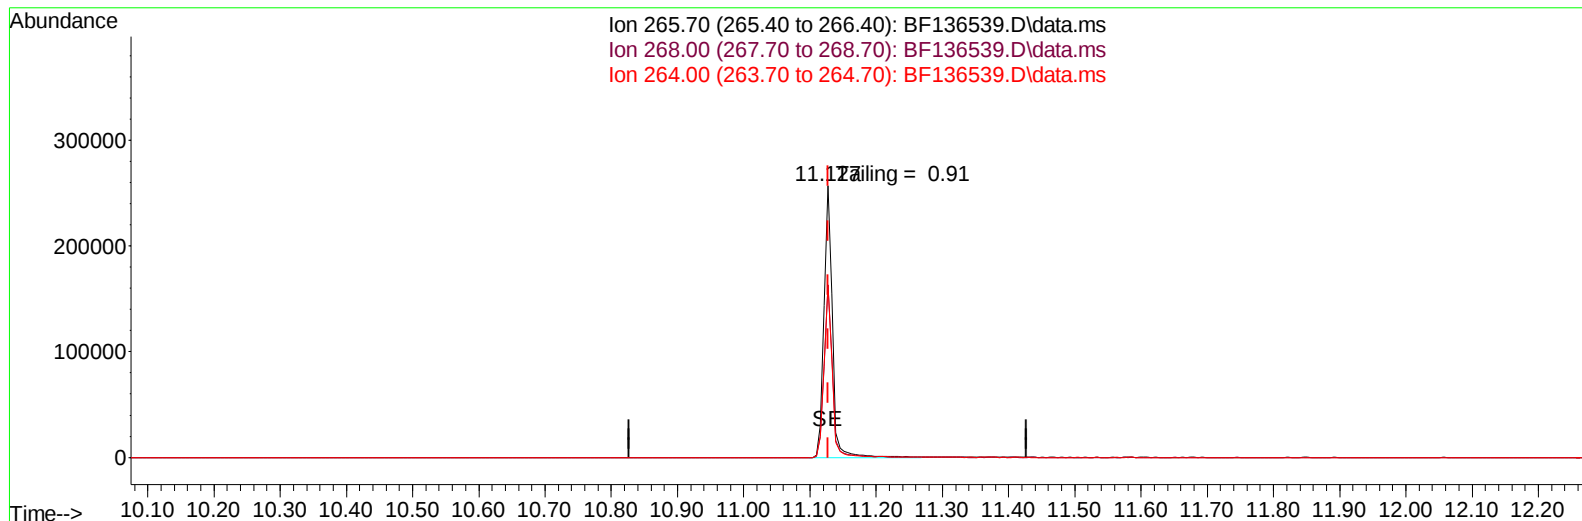

TIC: BF136539.D\data.ms

(70) Pentachlorophenol (C)




11.127min (-0.000) 23107.60 ng

response 230802

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.58
264.00	65.30	63.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121323\
Data File : BF136539.D
Acq On : 13 Dec 2023 15:58
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 02:39:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 06 09:40:27 2023
Response via : Initial Calibration

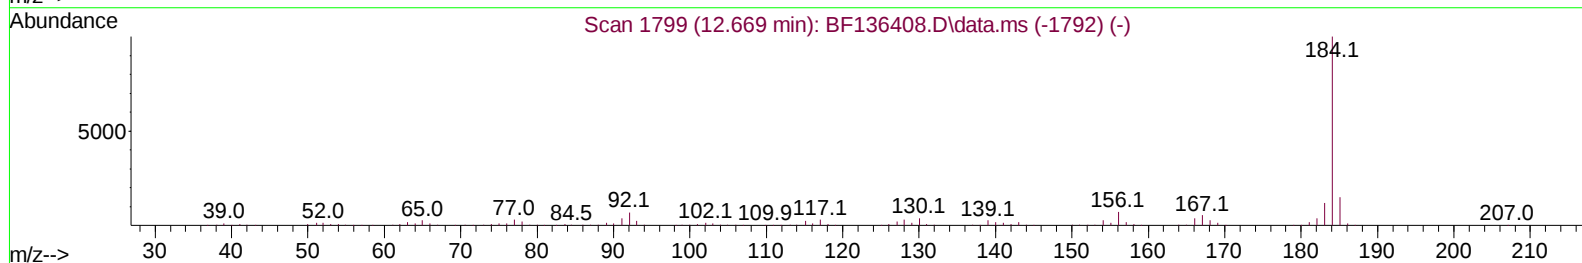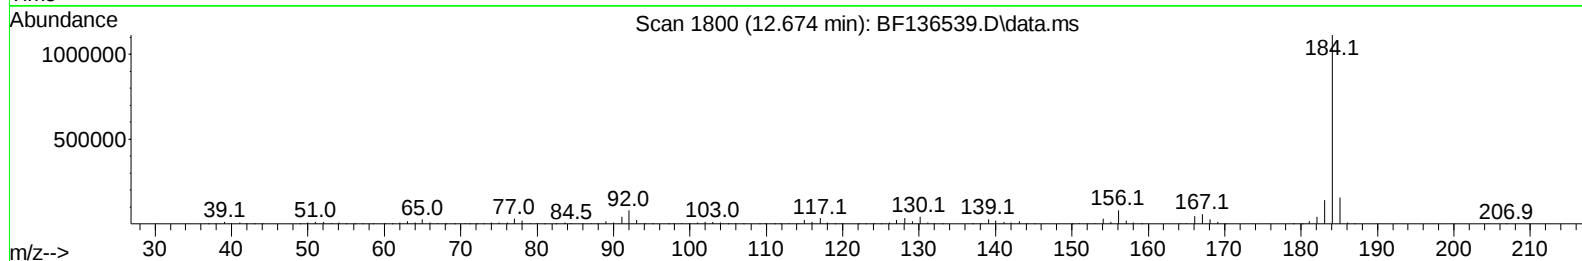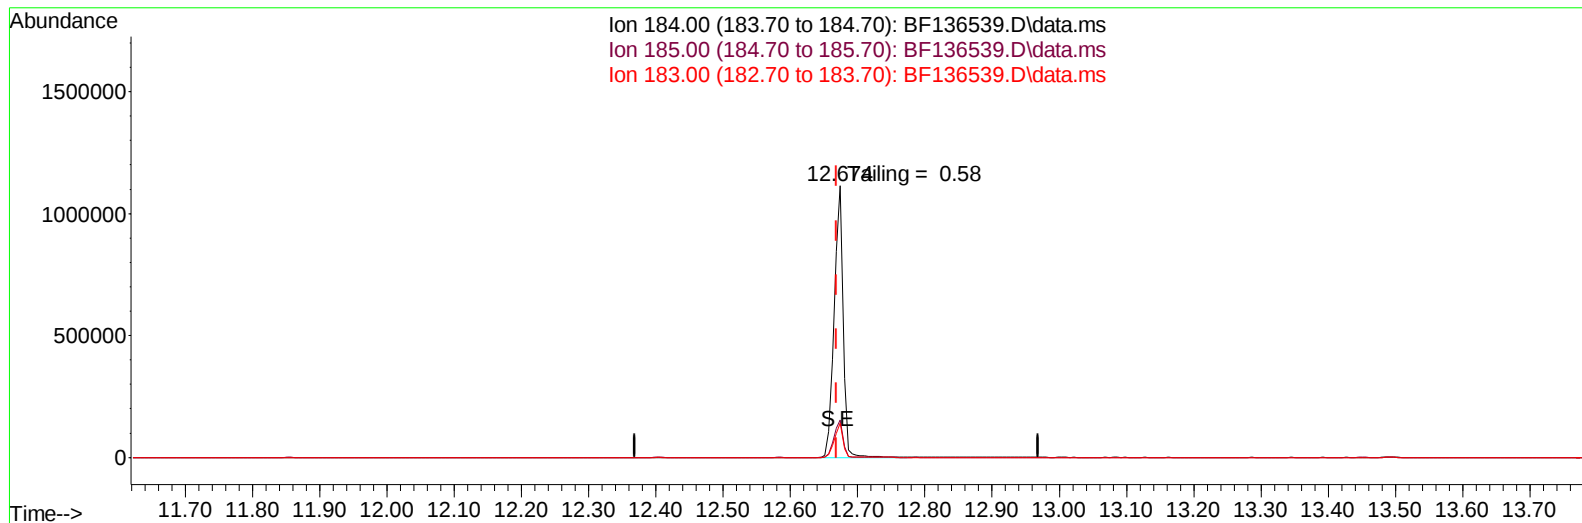

TIC: BF136539.D\data.ms

(77) Benzidine**12.674min (+ 0.005) 1419.26 ng****response 1024476**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.87
183.00	11.70	12.58
0.00	0.00	0.00