

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121323\
 Data File : BF136536.D
 Acq On : 13 Dec 2023 14:09
 Operator : CG\JU
 Sample : 05737-01 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SU-02-12082023

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136536.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.869	299	303	310	rVB2	21804	29043	3.96%	0.546%
2	5.428	564	568	577	rBV	292566	255989	34.92%	4.813%
3	6.434	735	739	746	rBV	274071	246116	33.57%	4.627%
4	6.792	796	800	804	rBV	680313	570551	77.82%	10.726%
5	7.351	891	895	899	rBV	192291	154546	21.08%	2.905%
6	8.069	1013	1017	1021	rBV	855527	715037	97.53%	13.443%
7	9.145	1197	1200	1209	rBV	382648	302806	41.30%	5.693%
8	9.828	1312	1316	1332	rBV	899445	733138	100.00%	13.783%
9	10.616	1447	1450	1457	rBV	143907	131638	17.96%	2.475%
10	11.322	1566	1570	1573	rBV	648533	602014	82.11%	11.318%
11	11.851	1653	1660	1665	rBV2	24065	28769	3.92%	0.541%
12	12.416	1751	1756	1762	rBV8	12983	20096	2.74%	0.378%
13	12.504	1767	1771	1774	rBV6	6030	9733	1.33%	0.183%
14	12.539	1774	1777	1779	rVB	14396	12935	1.76%	0.243%
15	12.639	1789	1794	1797	rBV5	12605	16986	2.32%	0.319%
16	12.769	1813	1816	1818	rBV	11985	11487	1.57%	0.216%
17	12.792	1818	1820	1823	rVB3	12214	9763	1.33%	0.184%
18	12.910	1837	1840	1844	rBV	269168	240544	32.81%	4.522%
19	13.098	1866	1872	1875	rBV6	13225	22750	3.10%	0.428%
20	13.151	1879	1881	1886	rVB5	14997	18162	2.48%	0.341%
21	13.268	1899	1901	1904	rBV4	8039	11174	1.52%	0.210%
22	13.498	1937	1940	1942	rBV2	25899	32068	4.37%	0.603%
23	13.827	1994	1996	1999	rBV3	16159	13849	1.89%	0.260%
24	13.968	2017	2020	2024	rBV	584277	576535	78.64%	10.839%
25	15.451	2268	2272	2278	rBV	437575	553460	75.49%	10.405%




Sum of corrected areas: 5319189

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121323\
Data File : BF136536.D
Acq On : 13 Dec 2023 14:09
Operator : CG\JU
Sample : 05737-01 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SU-02-12082023

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

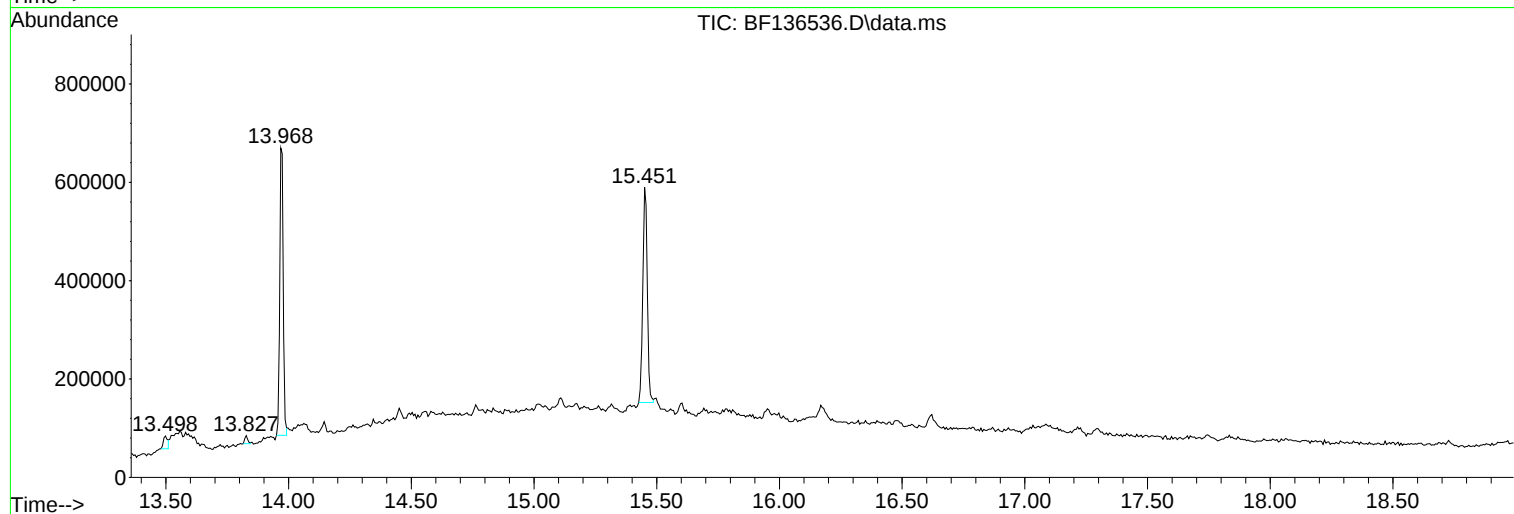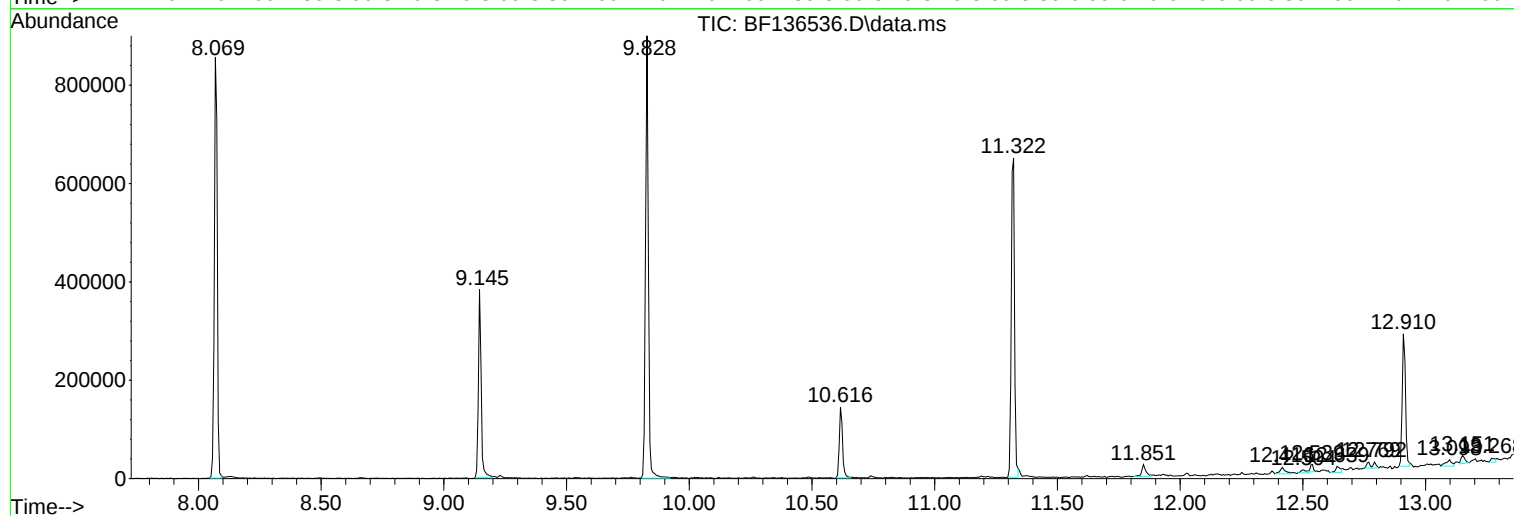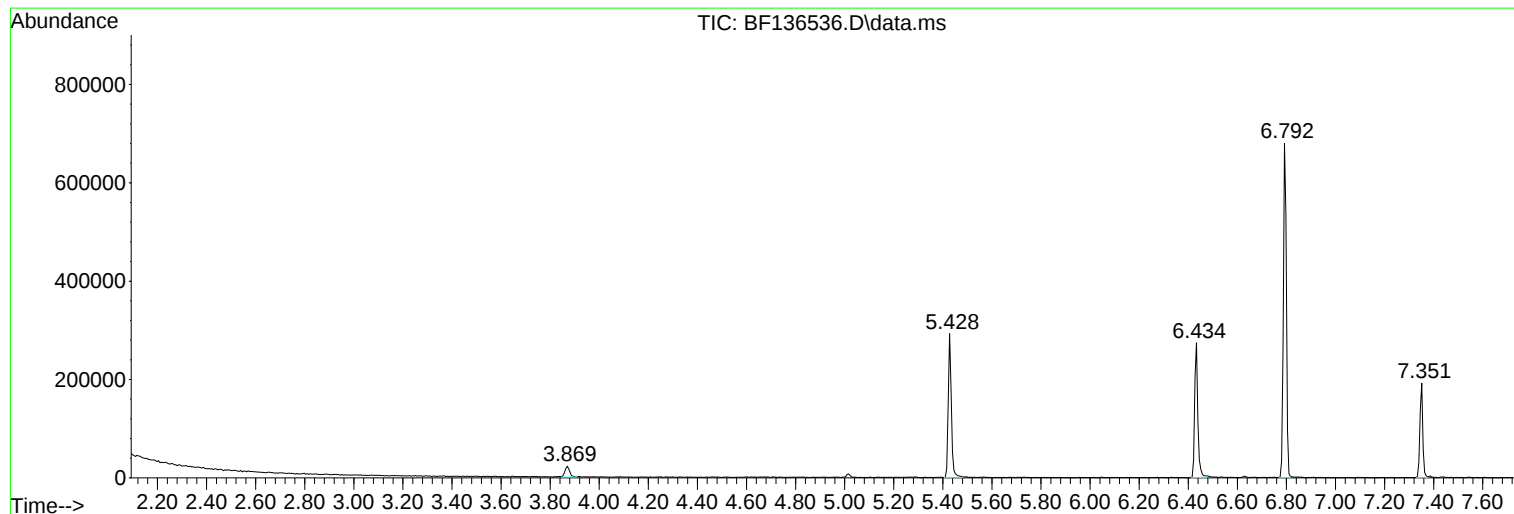

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121323\
Data File : BF136536.D
Acq On : 13 Dec 2023 14:09
Operator : CG\JU
Sample : 05737-01 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SU-02-12082023

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121323\
Data File : BF136536.D
Acq On : 13 Dec 2023 14:09
Operator : CG\JU
Sample : 05737-01 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SU-02-12082023

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------