

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121323\
 Data File : BF136561.D
 Acq On : 14 Dec 2023 03:38
 Operator : CG\JU
 Sample : 05588-01 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TUDOR

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136561.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.863	297	302	307	rVB	3998	6385	1.34%	0.148%
2	5.016	494	498	503	rVB	8003	8030	1.69%	0.186%
3	5.428	564	568	577	rVB	295518	258355	54.22%	5.970%
4	6.434	735	739	749	rVB	279828	251074	52.69%	5.801%
5	6.792	797	800	804	rBV	407637	357455	75.02%	8.259%
6	7.351	891	895	900	rBV	197857	153087	32.13%	3.537%
7	8.075	1014	1018	1021	rBV	453824	399748	83.89%	9.237%
8	9.145	1197	1200	1208	rBV	324481	278691	58.49%	6.439%
9	9.827	1313	1316	1320	rBV	495643	394892	82.88%	9.124%
10	10.616	1447	1450	1459	rBV	133725	125262	26.29%	2.894%
11	10.745	1469	1472	1475	rBV4	5942	7935	1.67%	0.183%
12	11.321	1566	1570	1573	rBV	512916	426603	89.53%	9.857%
13	11.786	1644	1649	1651	rBV5	4035	6470	1.36%	0.149%
14	11.851	1657	1660	1666	rBV4	19451	19761	4.15%	0.457%
15	11.933	1672	1674	1677	rVB3	9294	6988	1.47%	0.161%
16	12.198	1714	1719	1720	rBV5	4373	6025	1.26%	0.139%
17	12.374	1747	1749	1752	rBV3	12847	12545	2.63%	0.290%
18	12.416	1752	1756	1761	rVV8	9956	17553	3.68%	0.406%
19	12.463	1761	1764	1768	rVB4	9449	11716	2.46%	0.271%
20	12.539	1773	1777	1780	rBV	94163	85493	17.94%	1.975%
21	12.739	1809	1811	1812	rBV2	15924	10071	2.11%	0.233%
22	12.768	1812	1816	1819	rVV	100279	95953	20.14%	2.217%
23	12.815	1822	1824	1826	rBV3	7181	6800	1.43%	0.157%
24	12.915	1837	1841	1849	rBV	343407	332461	69.77%	7.682%
25	13.204	1887	1890	1894	rVB2	14690	18464	3.88%	0.427%
26	13.415	1920	1926	1930	rBV2	121671	182412	38.28%	4.215%
27	13.974	2016	2021	2024	rBV2	477109	476487	100.00%	11.010%
28	13.998	2024	2025	2028	rVB	56655	31325	6.57%	0.724%
29	15.021	2196	2199	2201	rBV2	53145	67170	14.10%	1.552%
30	15.456	2269	2273	2277	rBV	217160	272663	57.22%	6.300%




Sum of corrected areas: 4327874

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121323\
Data File : BF136561.D
Acq On : 14 Dec 2023 03:38
Operator : CG\JU
Sample : 05588-01 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TUDOR

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

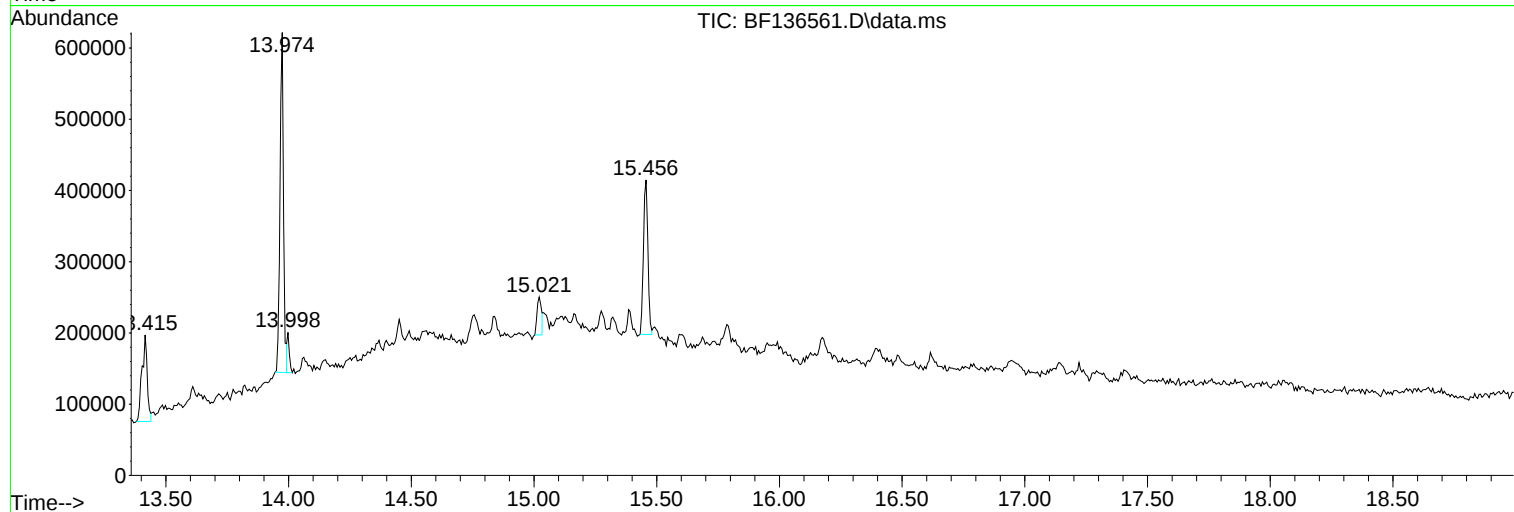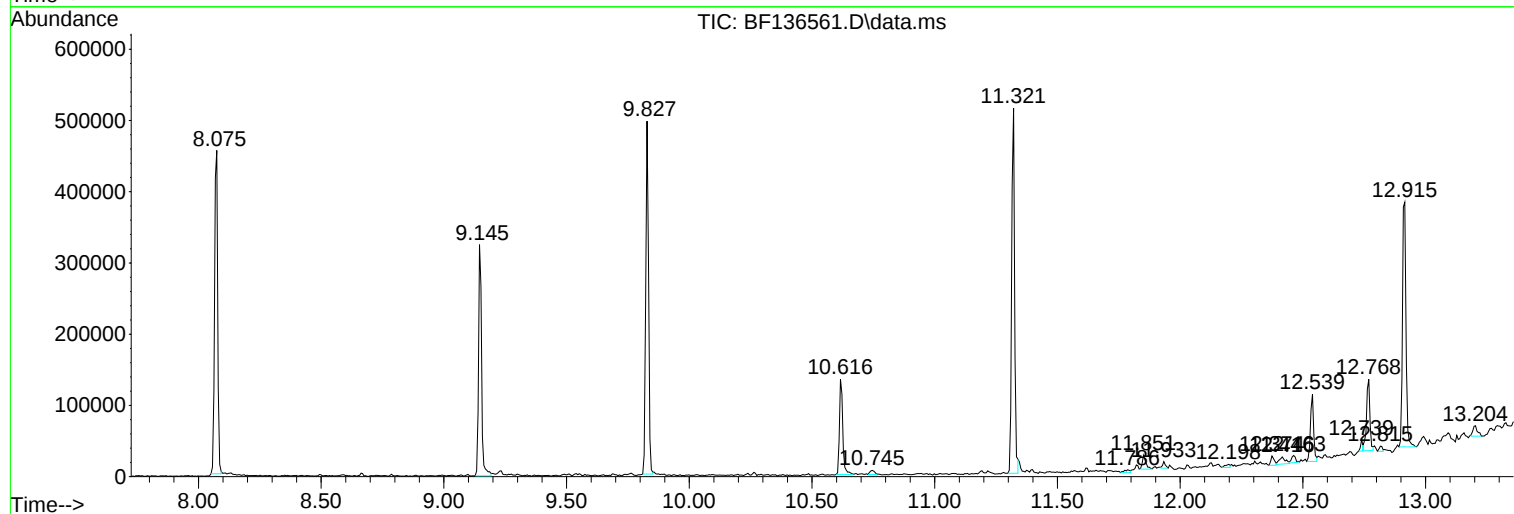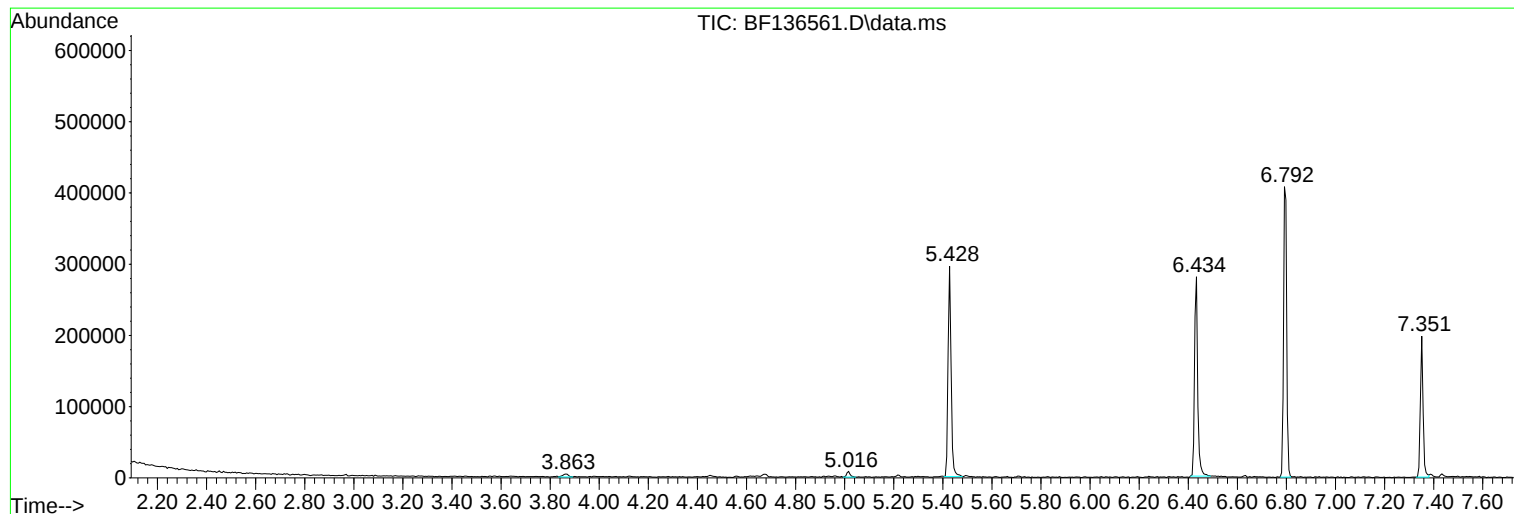

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121323\
Data File : BF136561.D
Acq On : 14 Dec 2023 03:38
Operator : CG\JU
Sample : 05588-01 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TUDOR

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121323\
Data File : BF136561.D
Acq On : 14 Dec 2023 03:38
Operator : CG\JU
Sample : 05588-01 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TUDOR

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------