


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121323\
Data File : BF136539.D
Acq On : 13 Dec 2023 15:58
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 06 09:40:27 2023

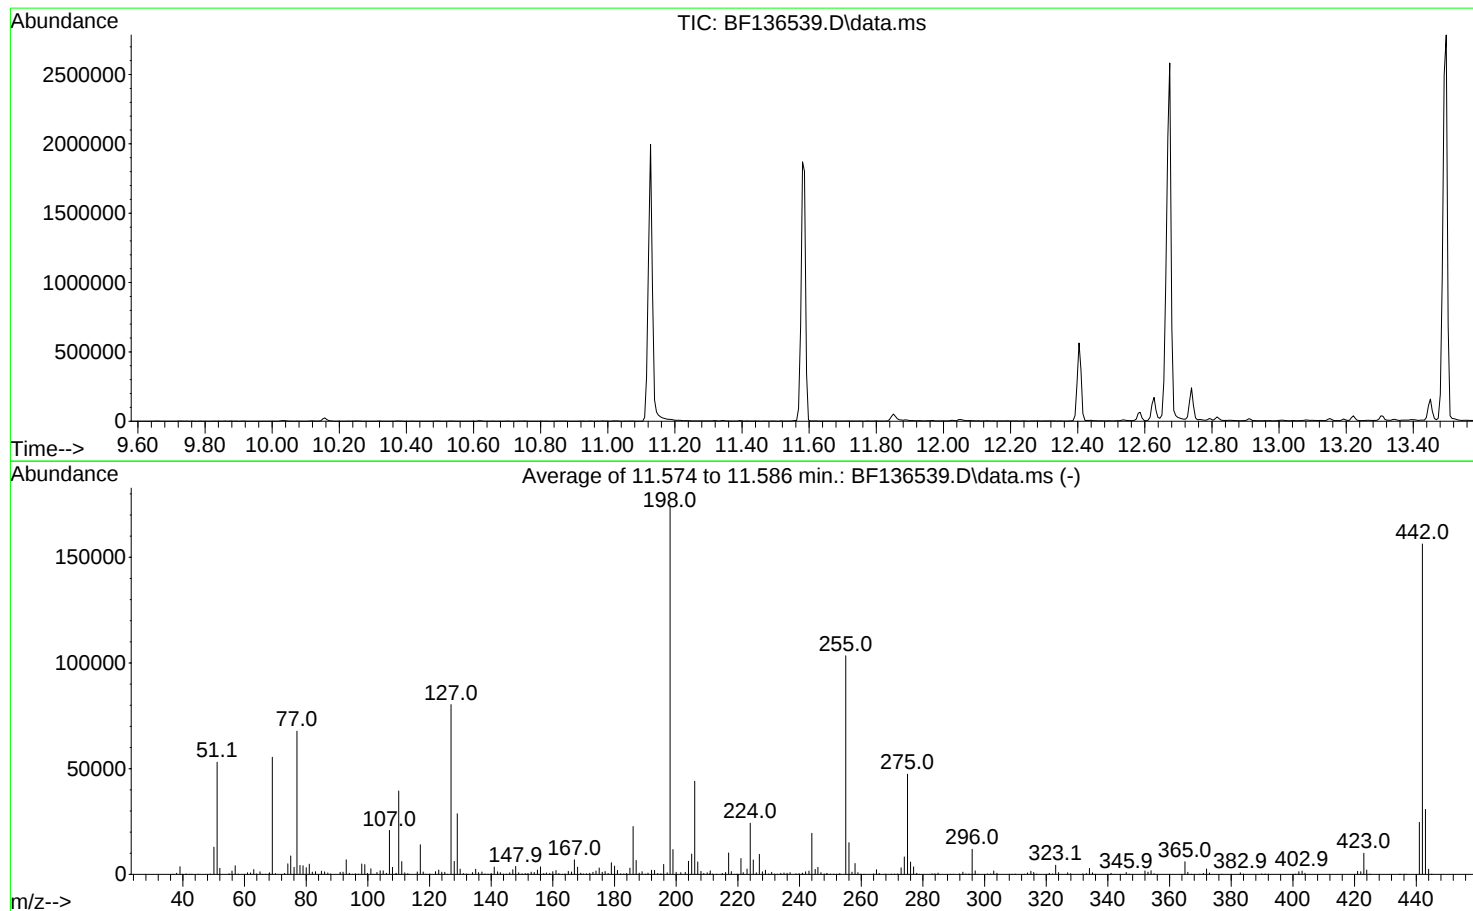

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	53045	PASS
68	69	0.00	2	1.4	770	PASS
69	198	0.00	100	31.9	55437	PASS
70	69	0.00	2	0.7	368	PASS
127	198	10	80	46.2	80355	PASS
197	198	0.00	2	0.4	770	PASS
198	198	100	100	100.0	174040	PASS
199	198	5	9	6.7	11735	PASS
275	198	10	60	27.2	47376	PASS
365	198	1	100	3.4	5965	PASS
441	198	0.01	100	14.1	24625	PASS
442	442	50	100	100.0	156293	PASS
443	442	15	24	19.6	30706	PASS

Instrument :
BNA_F
ClientSampleId :
DFTPP


Abundance

Ion 265.70 (265.40 to 266.40): BF136539.D\data.ms
Ion 268.00 (267.70 to 268.70): BF136539.D\data.ms
Ion 264.00 (263.70 to 264.70): BF136539.D\data.ms

11.17
Tail = 0.91

SE

Time--> 10.10 10.20 10.30 10.40 10.50 10.60 10.70 10.80 10.90 11.00 11.10 11.20 11.30 11.40 11.50 11.60 11.70 11.80 11.90 12.00 12.10 12.20






Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.58
264.00	65.30	63.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121323\
Data File : BF136539.D
Acq On : 13 Dec 2023 15:58
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 14 02:39:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 06 09:40:27 2023
Response via : Initial Calibration

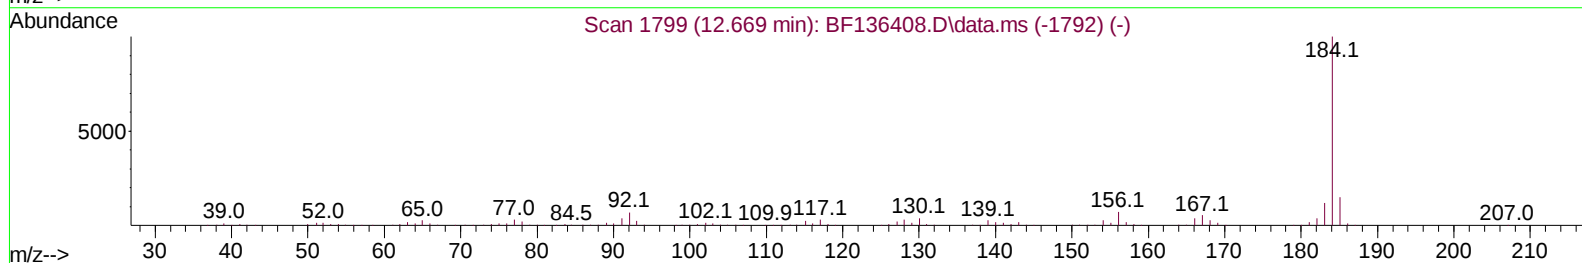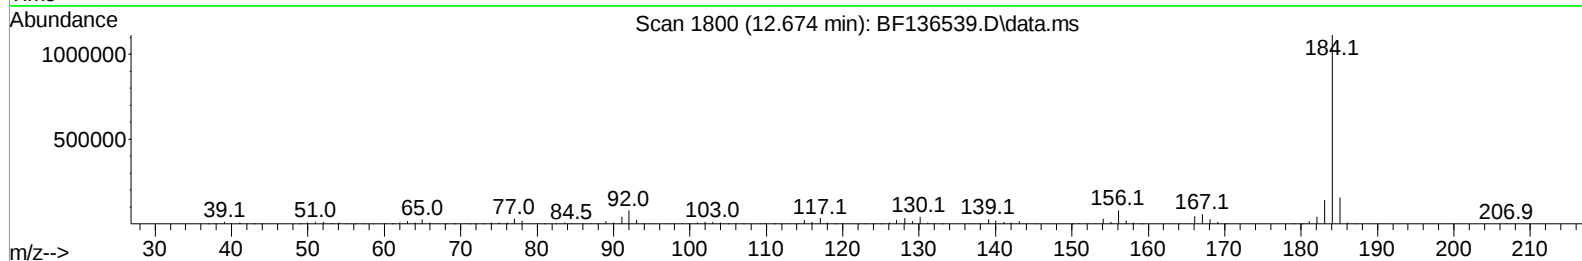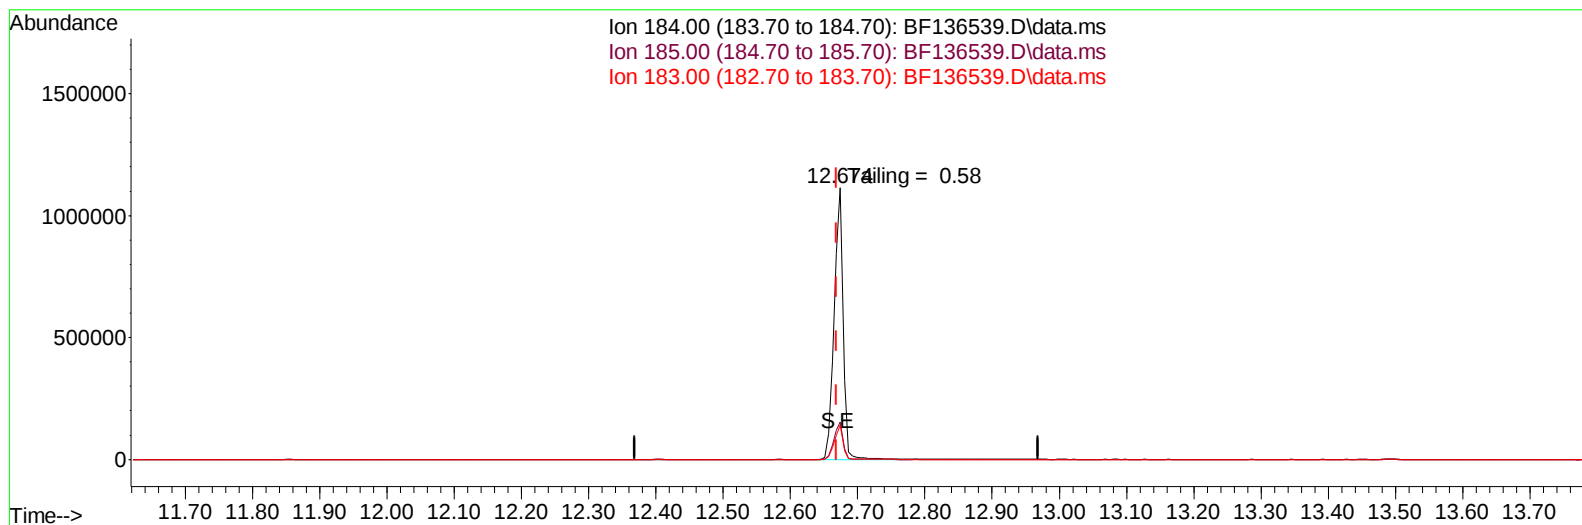

TIC: BF136539.D\data.ms

(77) Benzidine

12.674min (+ 0.005) 1419.26 ng

response 1024476

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.87
183.00	11.70	12.58
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/13/2023	BNA_F	<u>BF136539.D</u>
Compound Name	Response	Retention Time
DDT	533559	13.498
DDD	7739	13.221
DDE	556	12.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8295	541854	1.53

Instrument :
BNA_F
ClientSampleId :
DFTPP