
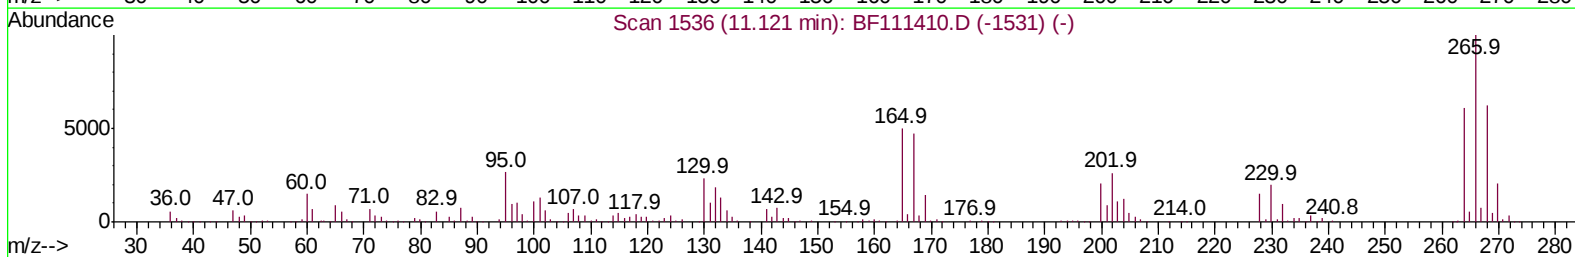
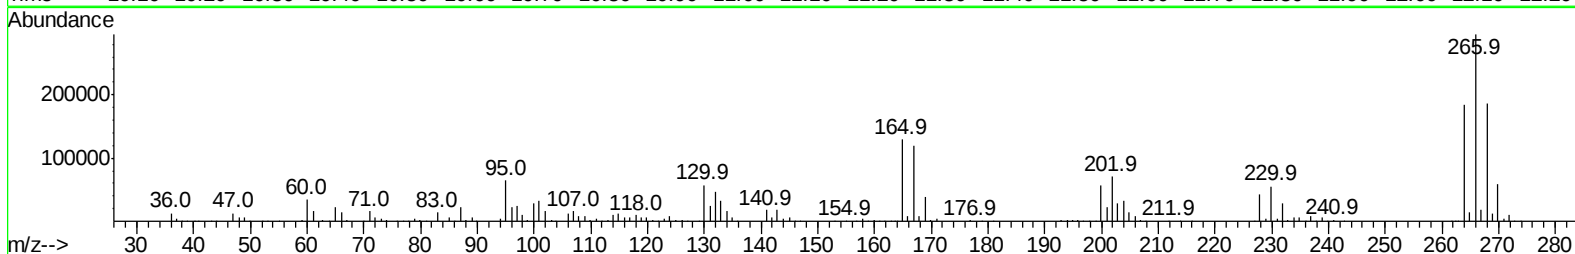


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF121418\
Data File : BF111406.D
Acq On : 14 Dec 2018 9:17
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 14:03:47 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF121418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 14 13:26:17 2018
Response via : Initial Calibration

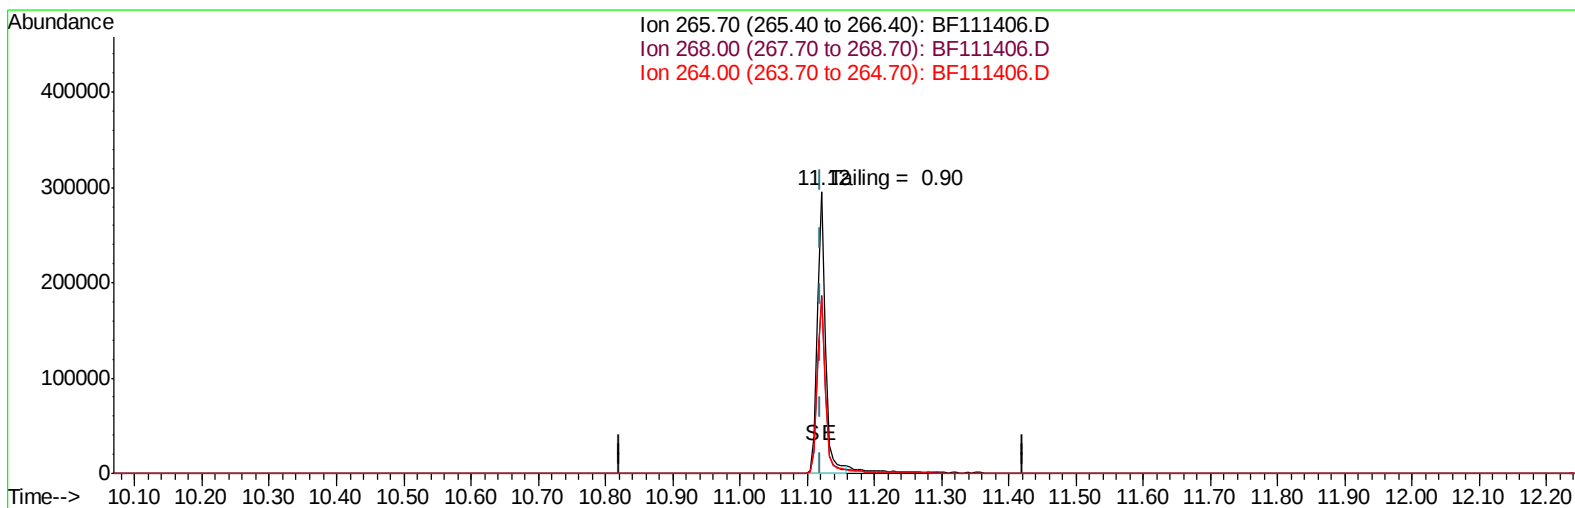

TIC: BF111406.D

(70) Pentachlorophenol (C)

11.122min (+0.000) 39027.41ng

response 268308

Ion	Exp%	Act%
265.70	100	100
268.00	59.90	63.15
264.00	61.40	62.31
0.00	0.00	0.00

