


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF121418\
 Data File : BF111406.D
 Acq On : 14 Dec 2018 9:17
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 14 13:26:17 2018

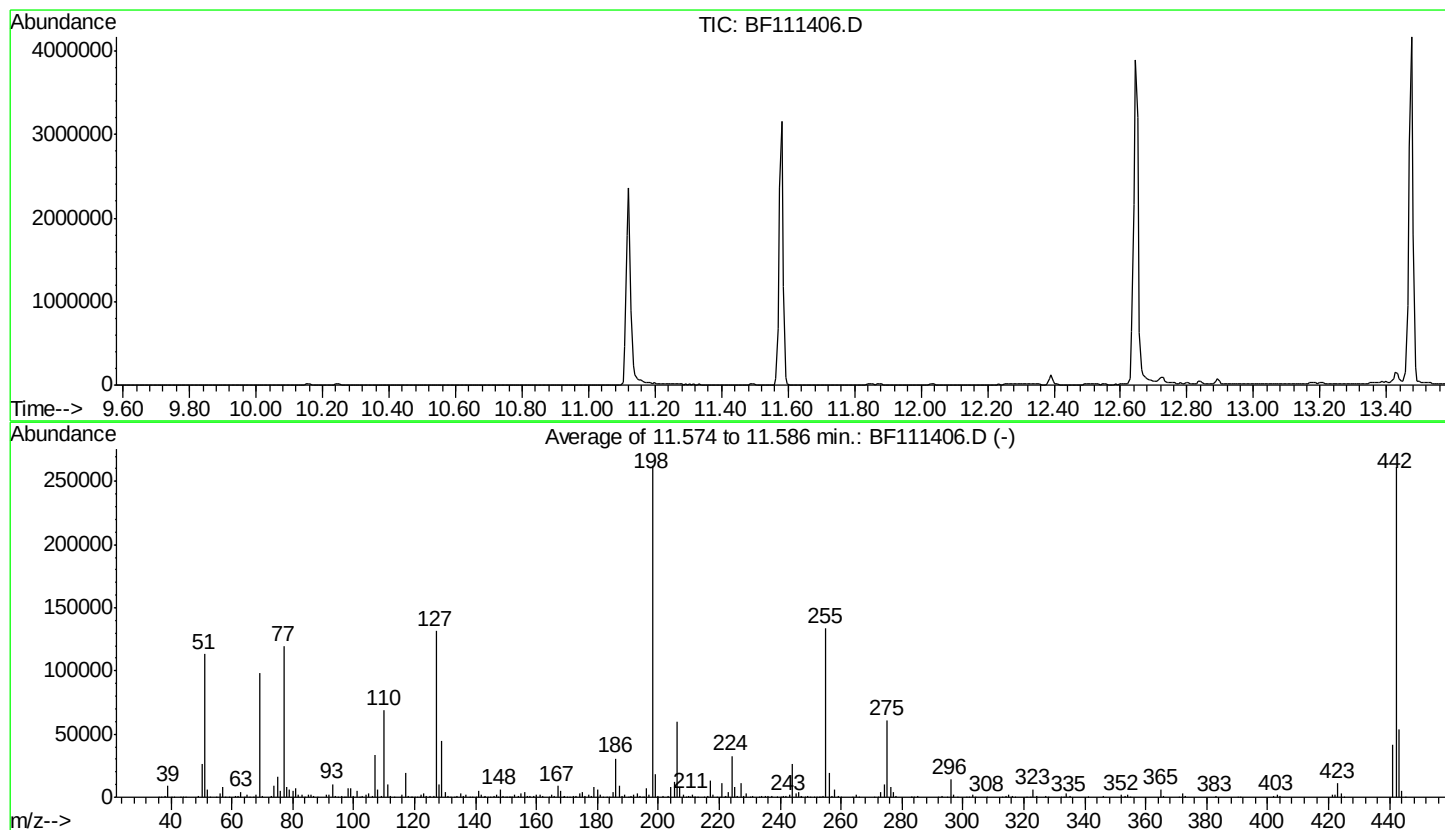

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.2	113301	PASS
68	69	0.00	2	1.7	1705	PASS
69	198	0.00	100	37.4	98082	PASS
70	69	0.00	2	0.8	812	PASS
127	198	10	80	50.0	131360	PASS
197	198	0.00	2	0.8	2004	PASS
198	198	100	100	100.0	262549	PASS
199	198	5	9	6.8	17859	PASS
275	198	10	60	23.0	60338	PASS
365	198	1	100	2.3	6033	PASS
441	198	0.01	100	15.9	41872	PASS
442	198	50	100	99.8	261909	PASS
443	442	15	24	20.4	53336	PASS