


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF121418\
 Data File : BF111415.D
 Acq On : 14 Dec 2018 13:33
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 14 13:26:17 2018

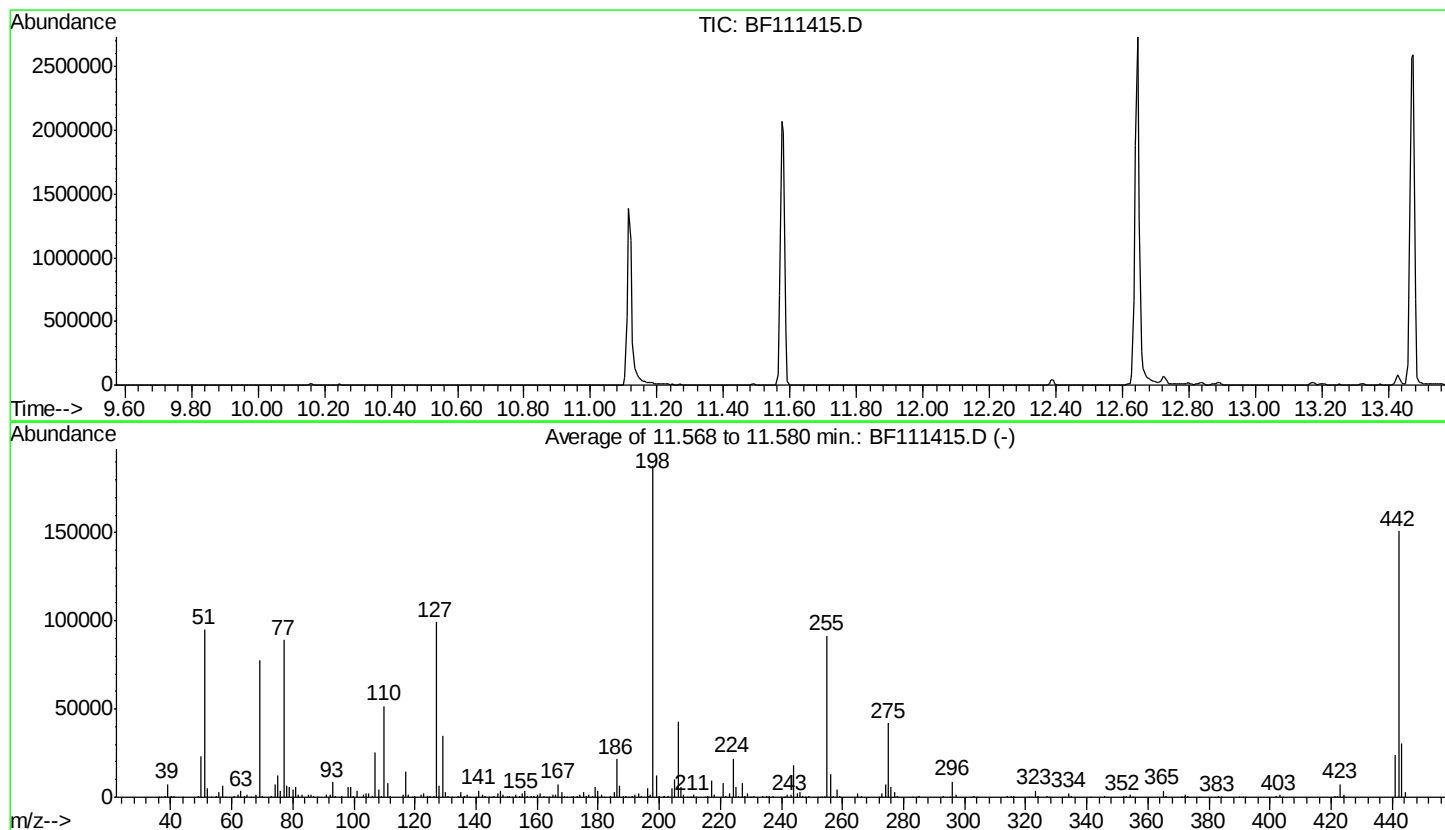

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.5	94954	PASS
68	69	0.00	2	1.6	1237	PASS
69	198	0.00	100	41.5	77925	PASS
70	69	0.00	2	0.6	441	PASS
127	198	10	80	52.7	99157	PASS
197	198	0.00	2	0.8	1484	PASS
198	198	100	100	100.0	187976	PASS
199	198	5	9	6.7	12612	PASS
275	198	10	60	22.3	41939	PASS
365	198	1	100	1.9	3636	PASS
441	198	0.01	100	12.7	23827	PASS
442	198	50	100	80.1	150637	PASS
443	442	15	24	20.1	30255	PASS