


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF121418\
Data File : BF111442.D
Acq On : 15 Dec 2018 2:31
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121418.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 14 13:26:17 2018

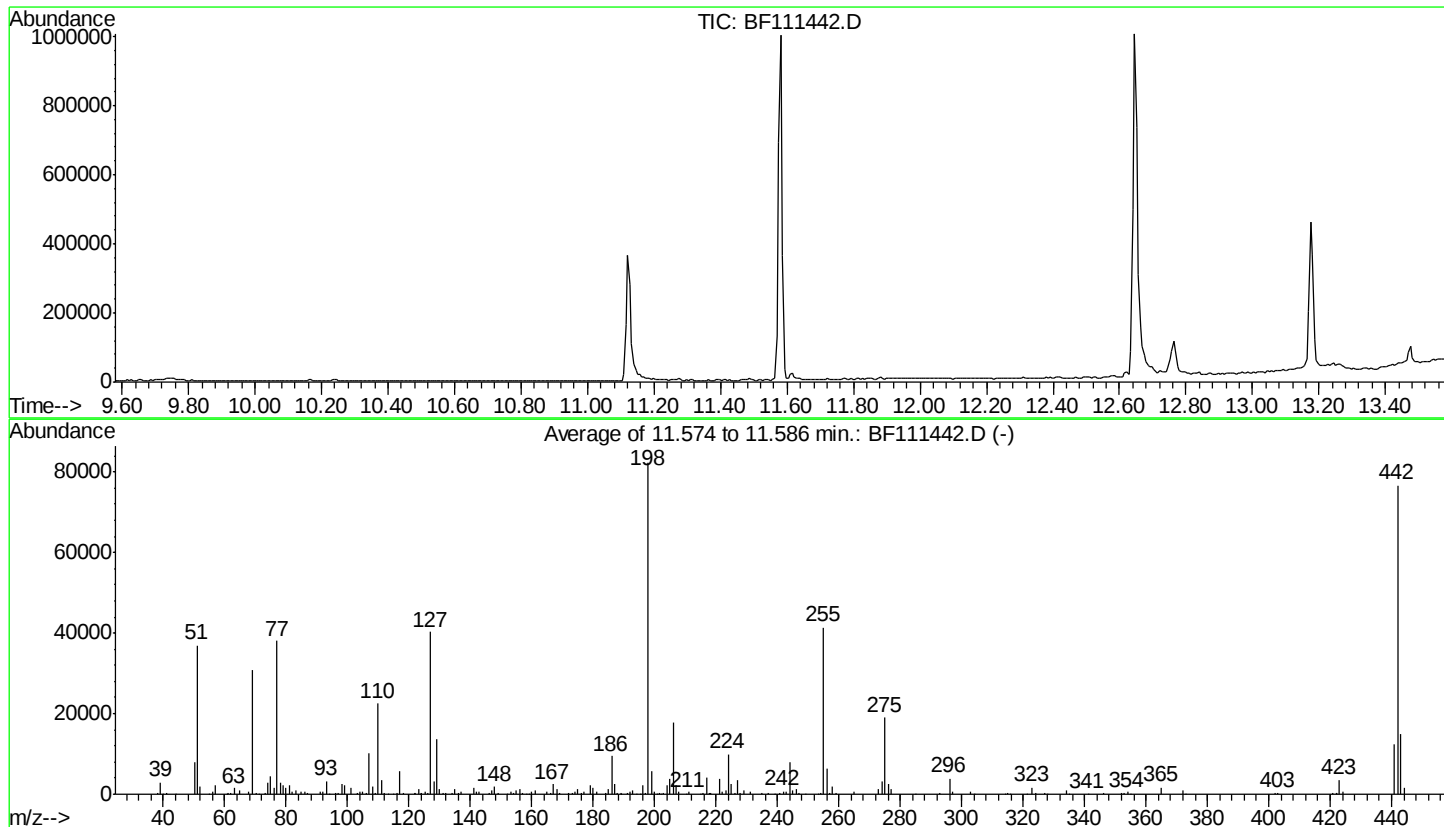

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.9	36923	PASS
68	69	0.00	2	1.9	590	PASS
69	198	0.00	100	37.3	30673	PASS
70	69	0.00	2	0.8	235	PASS
127	198	10	80	48.9	40255	PASS
197	198	0.00	2	0.5	407	PASS
198	198	100	100	100.0	82296	PASS
199	198	5	9	7.0	5731	PASS
275	198	10	60	23.0	18954	PASS
365	198	1	100	2.1	1718	PASS
441	198	0.01	100	15.0	12370	PASS
442	198	50	100	93.1	76592	PASS
443	442	15	24	19.3	14814	PASS