


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121422\
 Data File : BF131628.D
 Acq On : 14 Dec 2022 13:40
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 15 12:12:03 2022

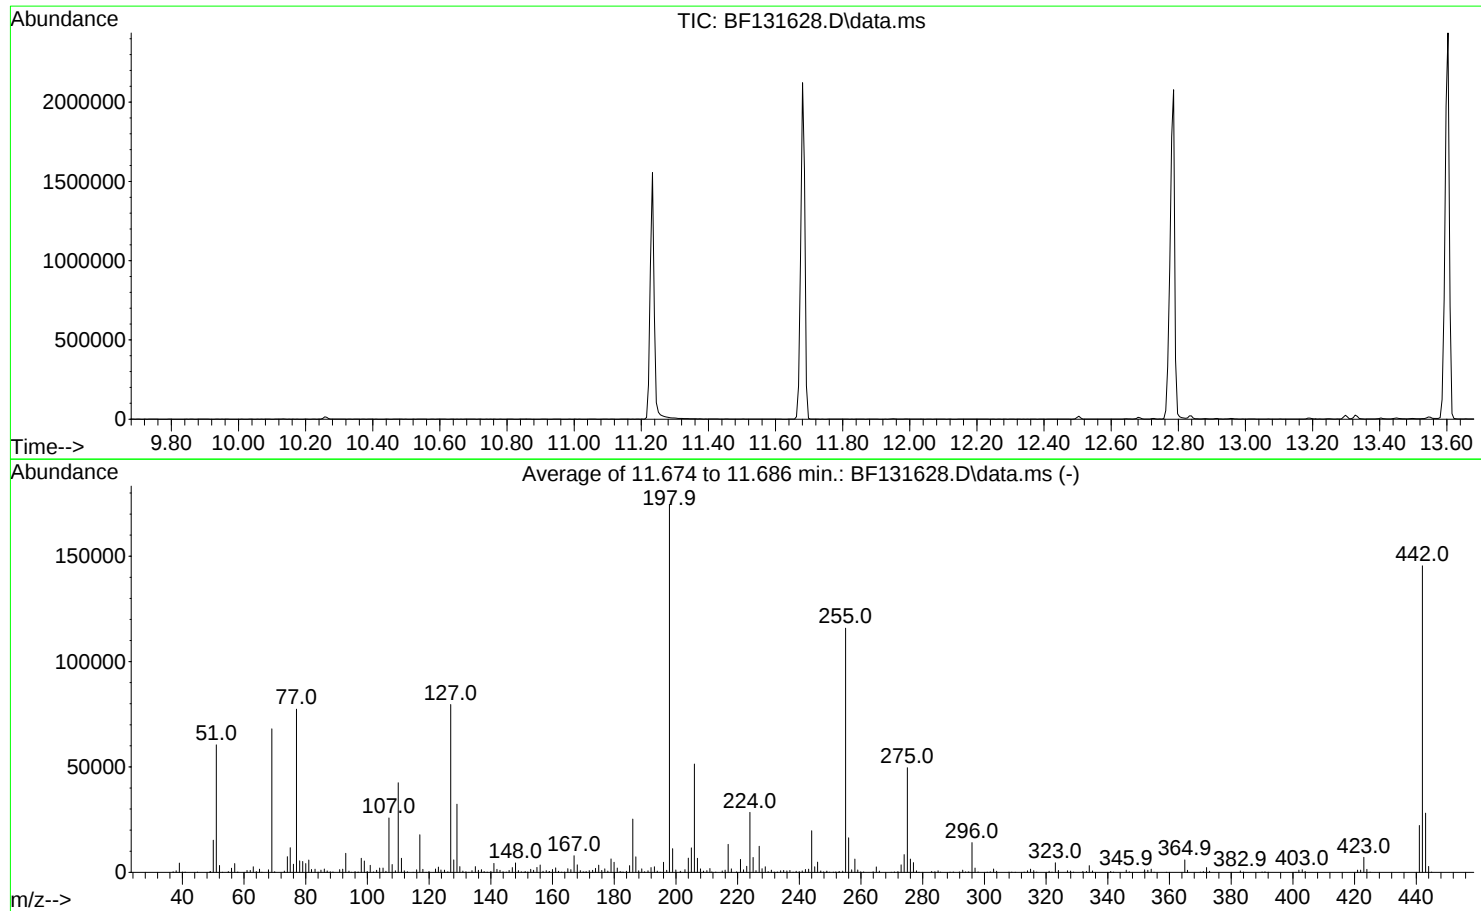




AutoFind: Scans 1630, 1631, 1632; Background Corrected with Scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	60523	PASS
68	69	0.00	2	1.7	1176	PASS
69	198	0.00	100	39.0	68072	PASS
70	69	0.00	2	0.4	251	PASS
127	198	10	80	45.6	79619	PASS
197	198	0.00	2	0.6	987	PASS
198	198	100	100	100.0	174579	PASS
199	198	5	9	6.4	11207	PASS
275	198	10	60	28.4	49595	PASS
365	198	1	100	3.4	5922	PASS
441	198	0.01	100	12.7	22180	PASS
442	442	50	100	100.0	145467	PASS
443	442	15	24	19.3	28096	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121422\
 Data File : BF131628.D
 Acq On : 14 Dec 2022 13:40
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Dec 15 05:30:53 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 14 03:22:29 2022
 Response via : Initial Calibration

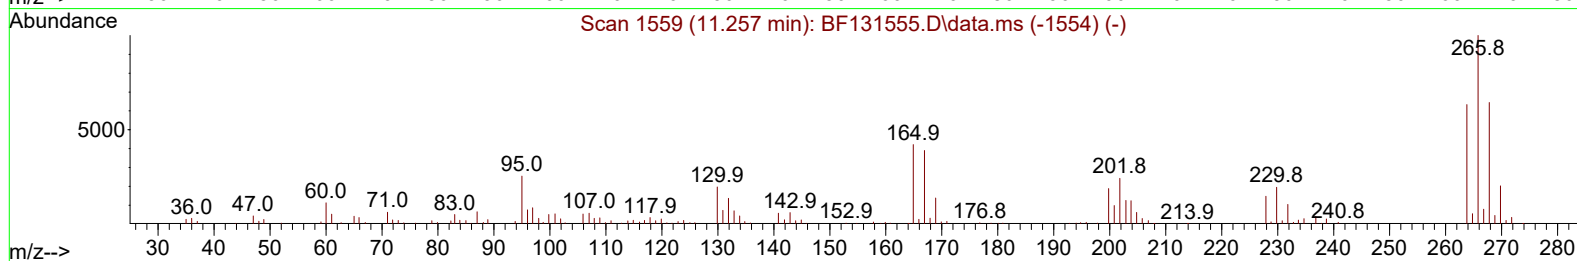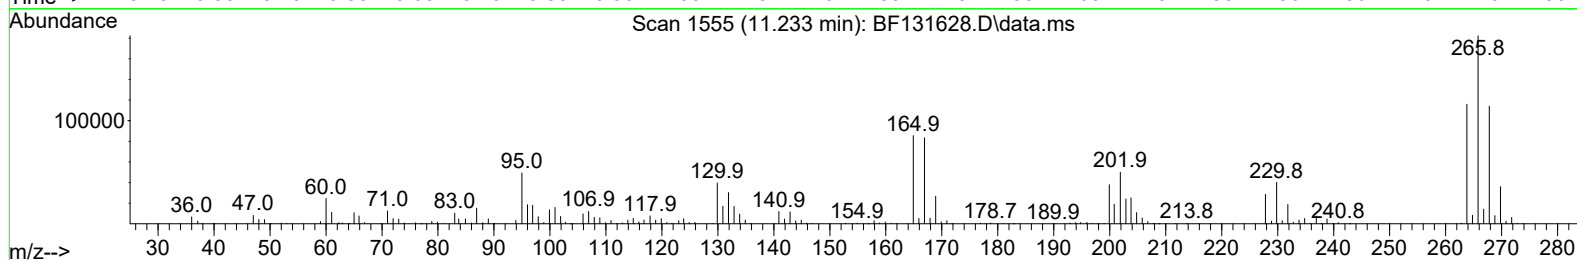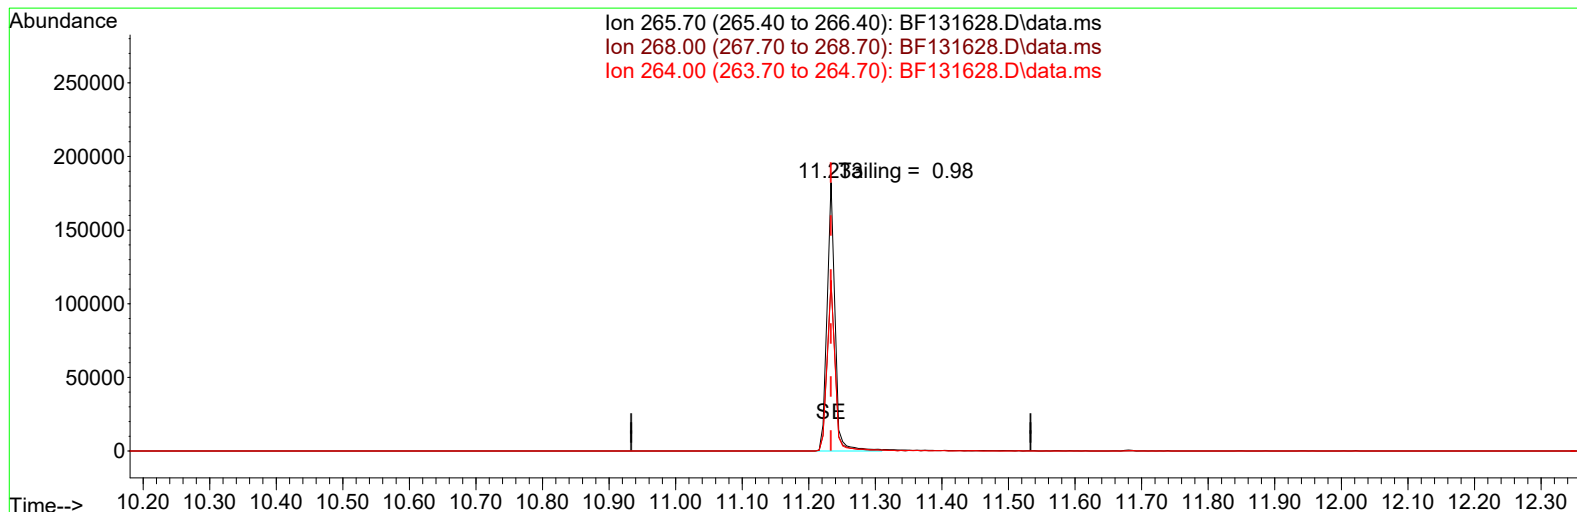

TIC: BF131628.D\data.ms

(70) Pentachlorophenol (C)

11.233min (+ 0.000) 167115.89 ng




response 154430

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	62.63
264.00	63.40	63.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121422\
Data File : BF131628.D
Acq On : 14 Dec 2022 13:40
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 15 05:30:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 14 03:22:29 2022
Response via : Initial Calibration

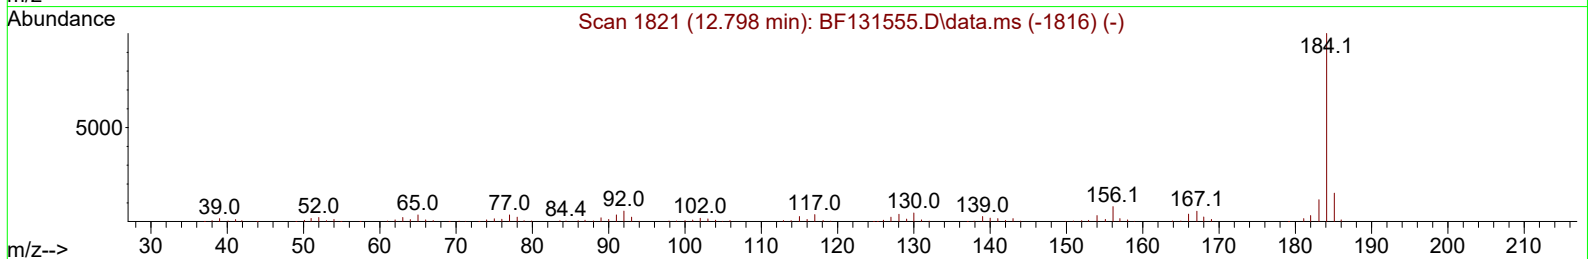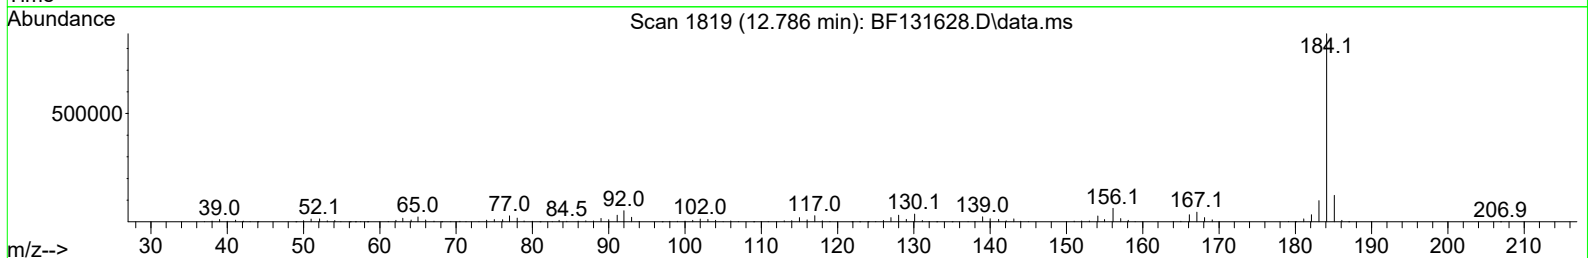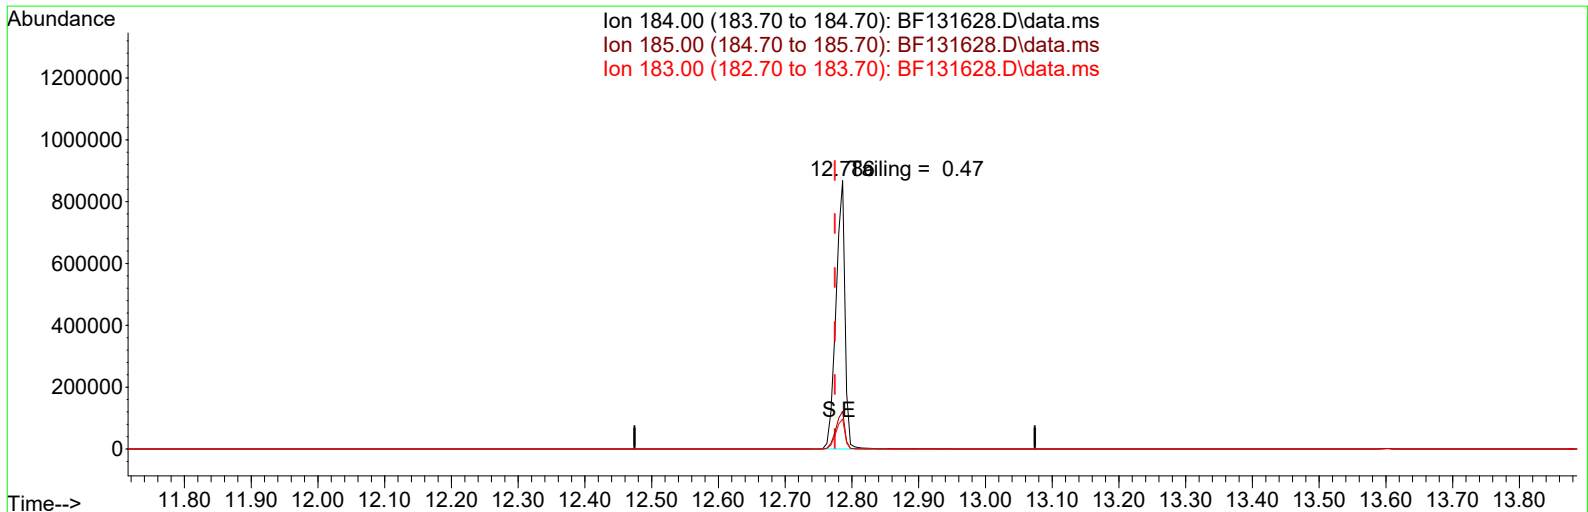

TIC: BF131628.D\data.ms

(77) Benzidine

12.786min (+ 0.012) 228453.23 ng

response 814112

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.04
183.00	11.60	11.24
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/14/2022	BNA_F	<u>BF131628.D</u>
Compound Name	Response	Retention Time
DDT	422049	13.604
DDD	8168	13.298
DDE	900	12.957
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9068	431117	2.10

Instrument :
BNA_F
ClientSampleId :
DFTPP