

Data File : BF111492.D
Acq On : 16 Dec 2018 3:39
Operator : JU/SJ
Sample : J6376-06
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TEST-PIT-2

Quant Time: Dec 17 00:57:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 14 13:26:17 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.79	152	119594	20.00	ng	0.00
21) Naphthalene-d8	8.07	136	428547	20.00	ng	0.00
39) Acenaphthene-d10	9.83	164	159672	20.00	ng	0.00
64) Phenanthrene-d10	11.31	188	270918	20.00	ng	0.00
76) Chrysene-d12	13.95	240	264118	20.00	ng	0.00
87) Perylene-d12	15.39	264	174853	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.43	112	867376	120.69	ng	0.01
7) Phenol-d6	6.43	99	924201	96.68	ng	0.00
23) Nitrobenzene-d5	7.35	82	677434	94.13	ng	0.00
42) 2,4,6-Tribromophenol	10.62	330	191128	133.63	ng	0.00
45) 2-Fluorobiphenyl	9.15	172	1182858	114.43	ng	0.00
79) Terphenyl-d14	12.90	244	1138014	101.18	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.35	70	88406	14.017	ng	# 84
25) Isophorone	7.35	82	677535	55.642	ng	# 64
51) 2,6-Dinitrotoluene	9.83	165	19550	7.553	ng	# 30
57) 2,4-Dinitrotoluene	9.83	165	19550	5.755	ng	# 25
67) 4-Bromophenyl-phenylether	10.62	248	12048	4.126	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BF111492.D
Acq On : 16 Dec 2018 3:39
Operator : JU/SJ
Sample : J6376-06
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TEST-PIT-2

Quant Time: Dec 17 00:57:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 14 13:26:17 2018
Response via : Initial Calibration

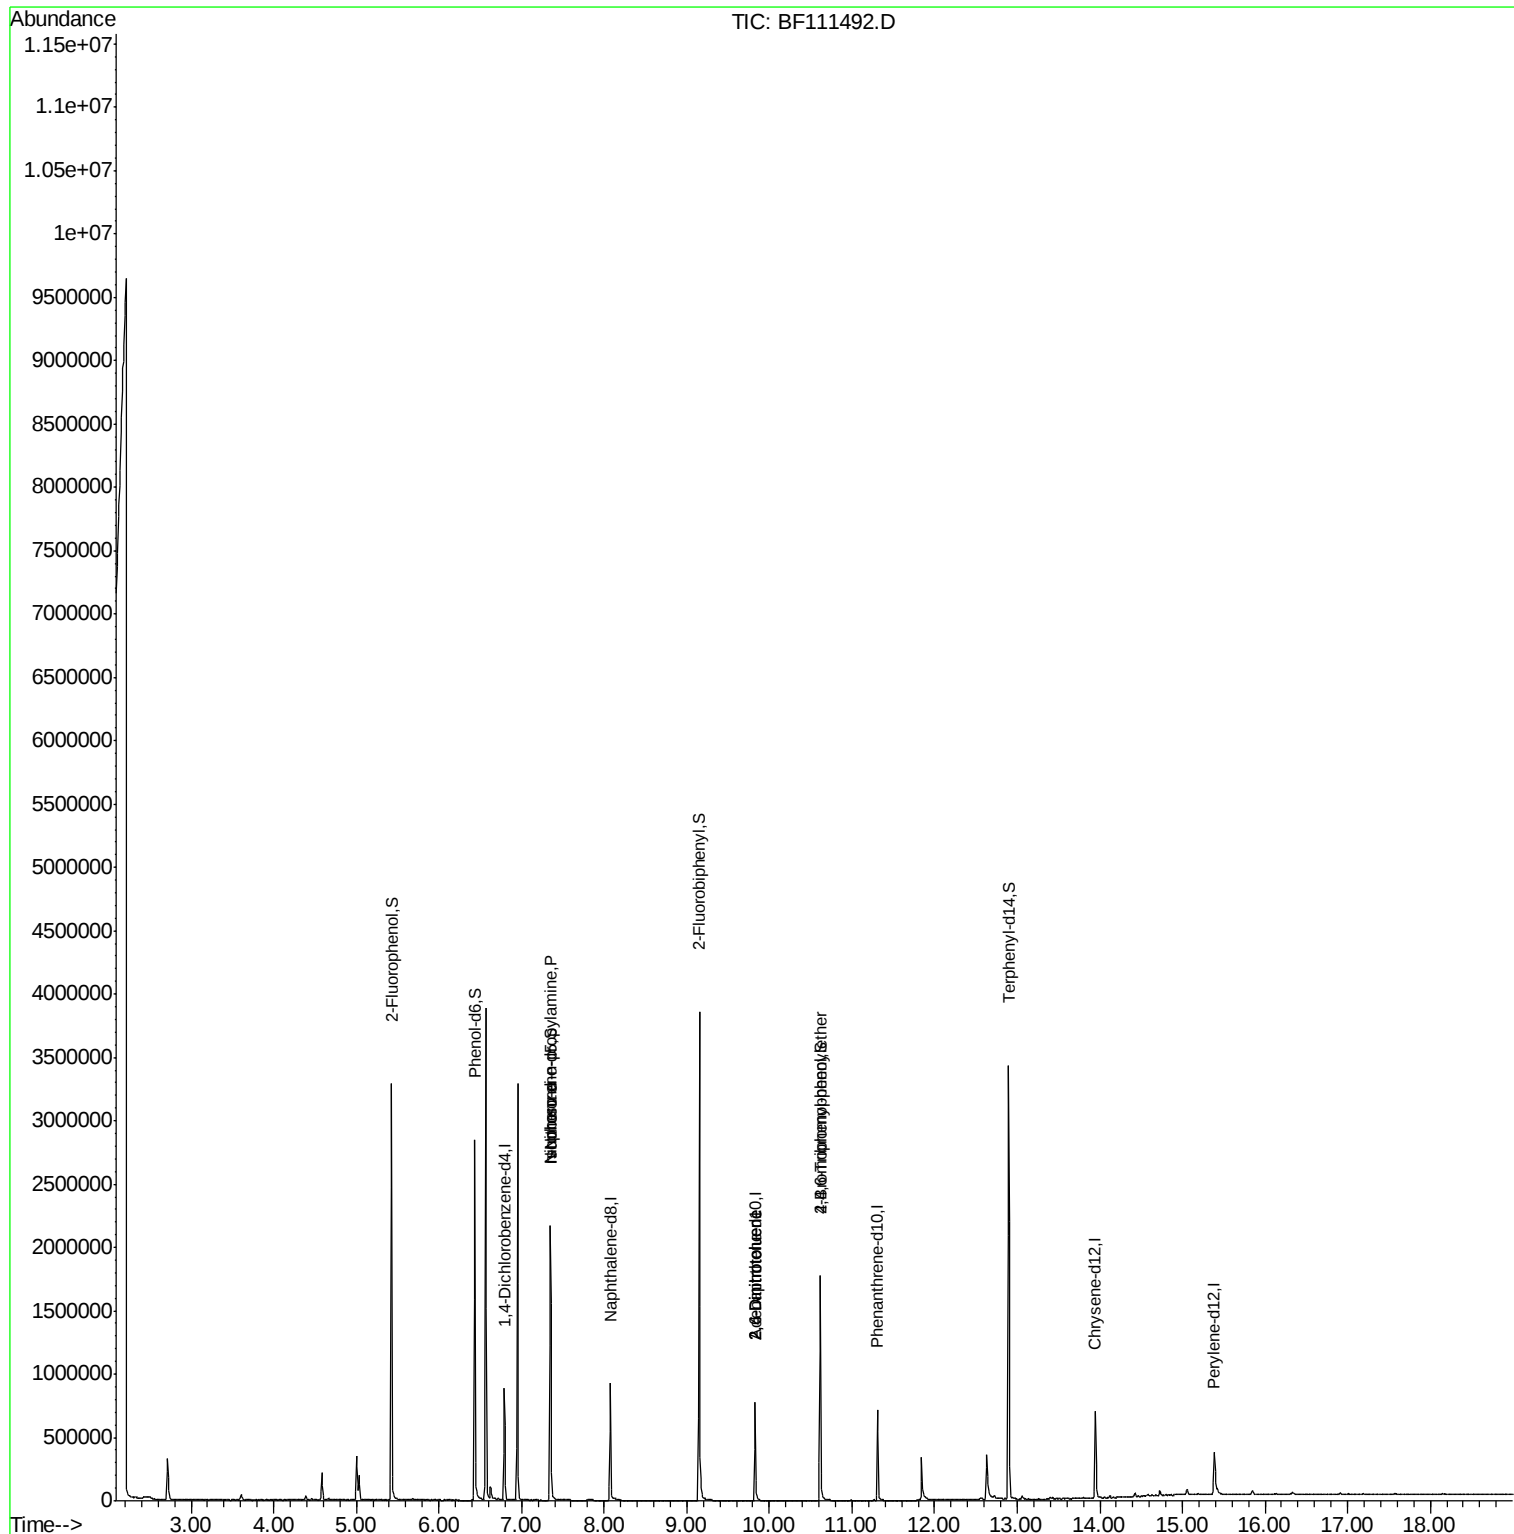




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.79 min Scan# 800
Delta R.T. -0.00 min
Lab File: BF111492.D
Acq: 16 Dec 2018 3:39

Instrument :
BNA_F
ClientSampleId :
TEST-PIT-2

Tgt Ion:152 Resp: 119594
Ion Ratio Lower Upper
152 100
150 157.2 126.6 189.8
115 62.7 50.7 76.1

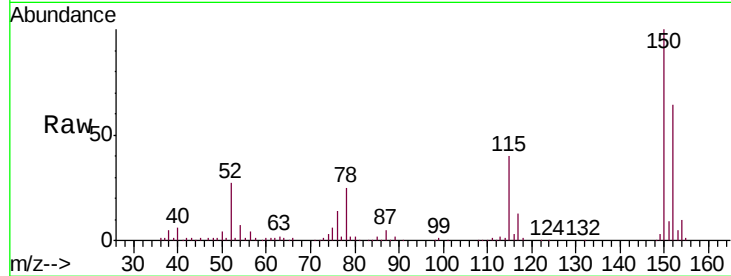


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

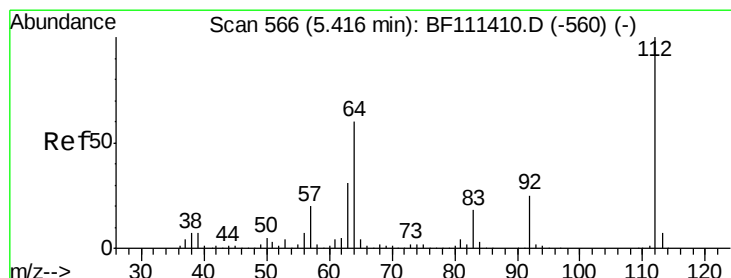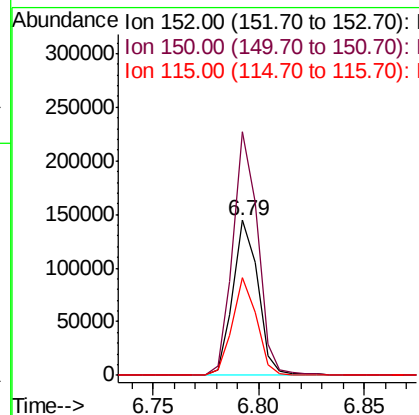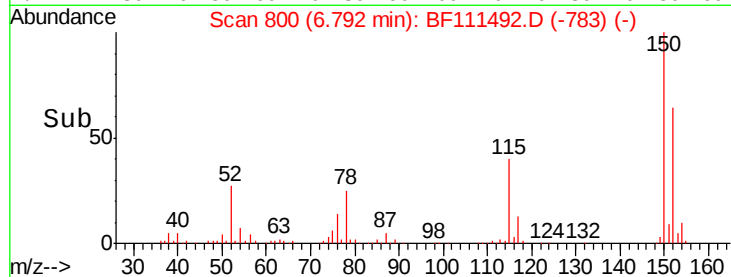



#5

2-Fluorophenol
Concen: 120.689 ng
RT: 5.43 min Scan# 568
Delta R.T. 0.01 min
Lab File: BF111492.D
Acq: 16 Dec 2018 3:39

Tgt Ion:112 Resp: 867376
Ion Ratio Lower Upper
112 100
64 58.7 51.8 77.6
63 30.7 26.8 40.2

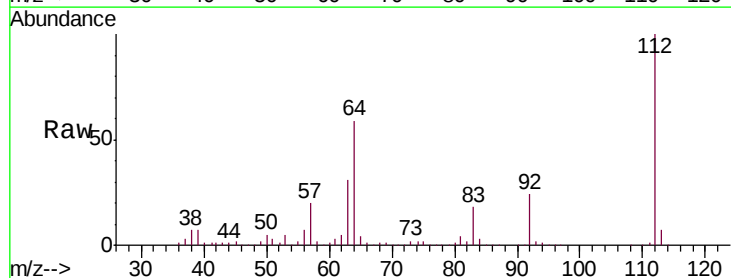

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

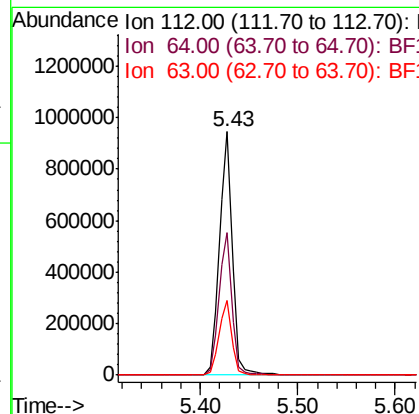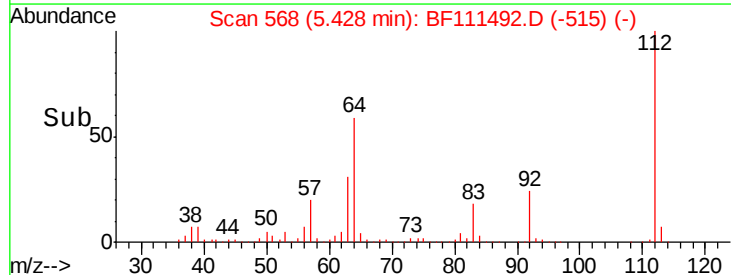



#7

Phenol-d6

Concen: 96.676 ng

RT: 6.43 min Scan# 739

Delta R.T. -0.01 min

Lab File: BF111492.D

Acq: 16 Dec 2018 3:39

Instrument :

BNA_F

ClientSampleId :

TEST-PIT-2





Tgt Ion: 99 Resp: 924201

Ion Ratio Lower Upper

99 100

42 22.4 17.4 26.0

71 33.5 26.1 39.1

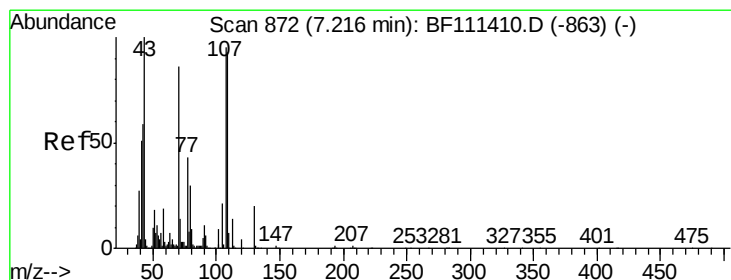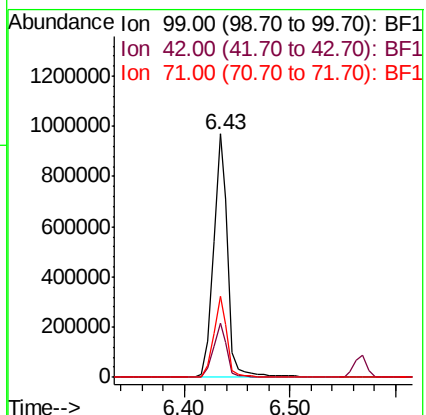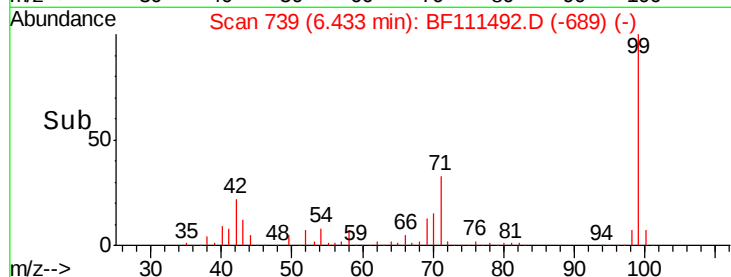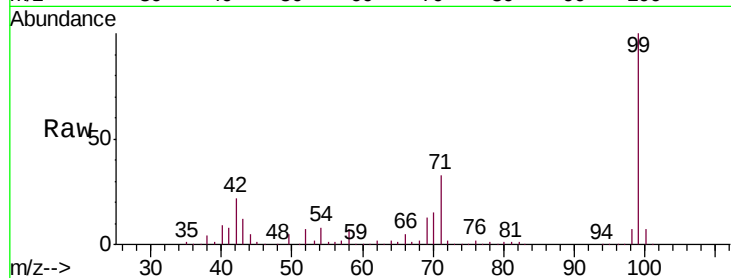

#19

n-Nitroso-di-n-propylamine

Concen: 14.017 ng

RT: 7.35 min Scan# 895

Delta R.T. 0.14 min

Lab File: BF111492.D

Acq: 16 Dec 2018 3:39

Tgt Ion: 70 Resp: 88406




Ion Ratio Lower Upper


70 100

42 62.2 53.2 79.8

101 0.0 8.2 12.4#

130 2.0 18.1 27.1#


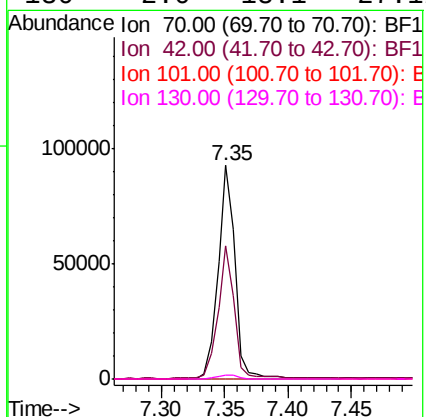
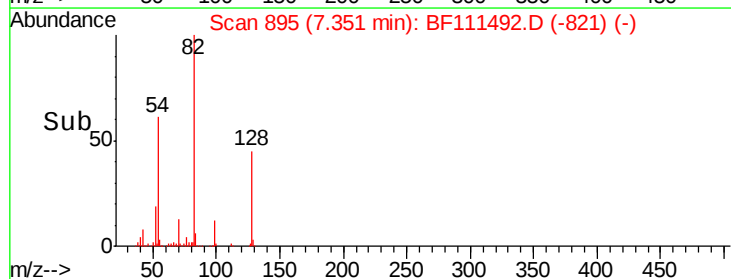
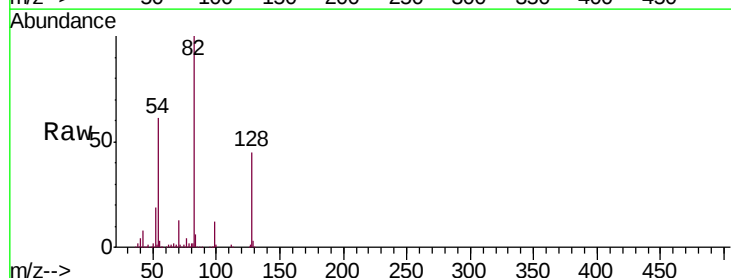


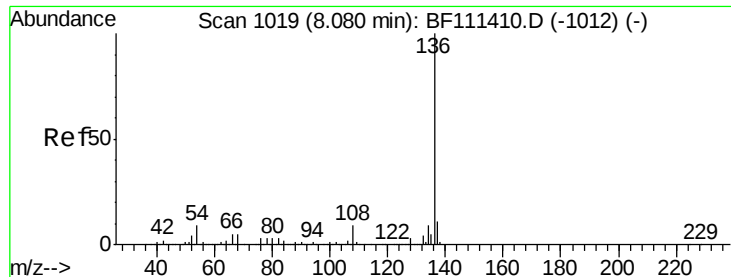

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.07 min Scan# 1018
Delta R.T. -0.01 min
Lab File: BF111492.D
Acq: 16 Dec 2018 3:39




Instrument :
BNA_F
ClientSampleId :
TEST-PIT-2


Tgt Ion:	136	Resp:	428547
Ion	Ratio	Lower	Upper
136	100		
137	10.3	9.1	13.7
54	8.3	7.7	11.5
68	4.4	4.9	7.3#

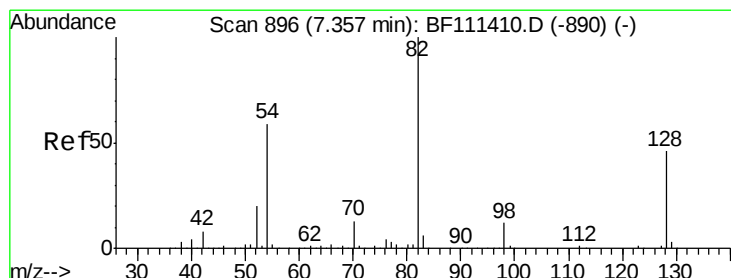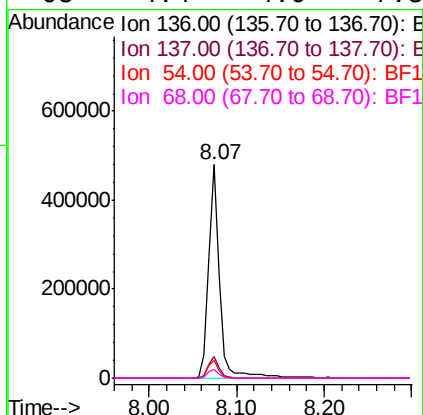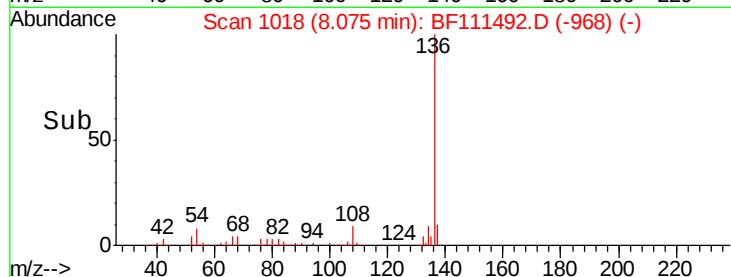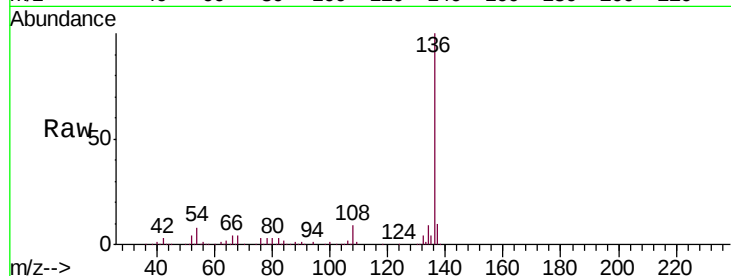

#23
Nitrobenzene-d5
Concen: 94.133 ng
RT: 7.35 min Scan# 895
Delta R.T. -0.01 min
Lab File: BF111492.D
Acq: 16 Dec 2018 3:39

Tgt Ion:	82	Resp:	677434
Ion	Ratio	Lower	Upper
82	100		
128	44.8	37.4	56.2
54	60.8	47.6	71.4


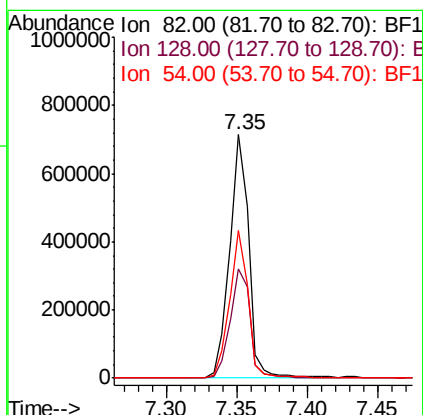
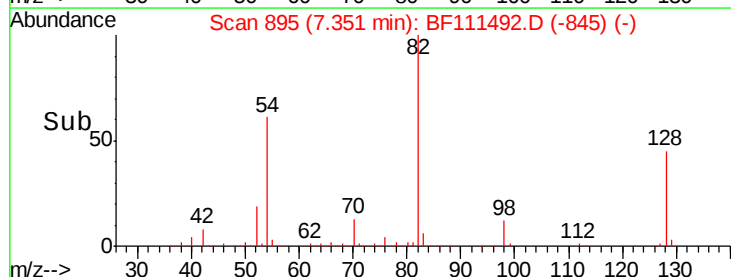
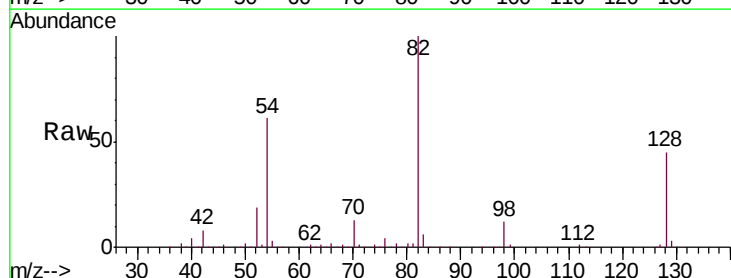


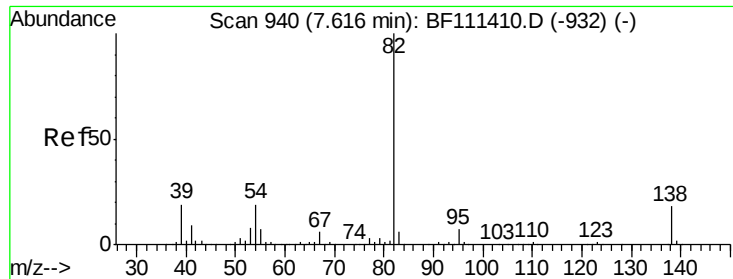

#25
Isophorone
Concen: 55.642 ng
RT: 7.35 min Scan# 895
Delta R.T. -0.26 min
Lab File: BF111492.D
Acq: 16 Dec 2018 3:39




Instrument :
BNA_F
ClientSampleId :
TEST-PIT-2


Tgt Ion: 82 Resp: 677535
Ion Ratio Lower Upper
82 100
95 0.0 5.4 8.2#
138 0.0 15.1 22.7#

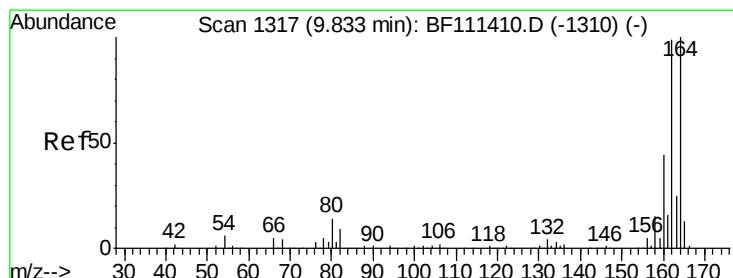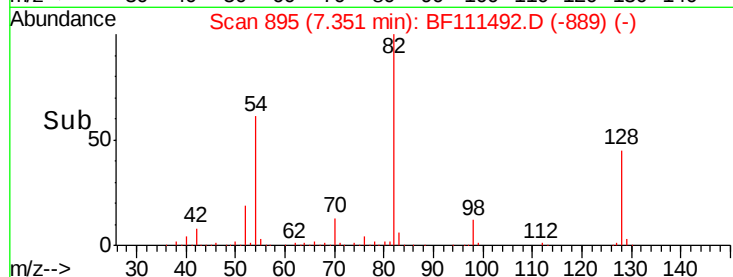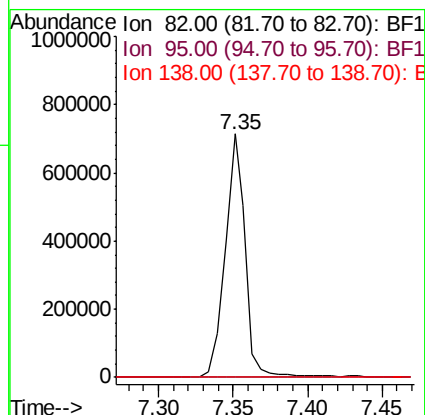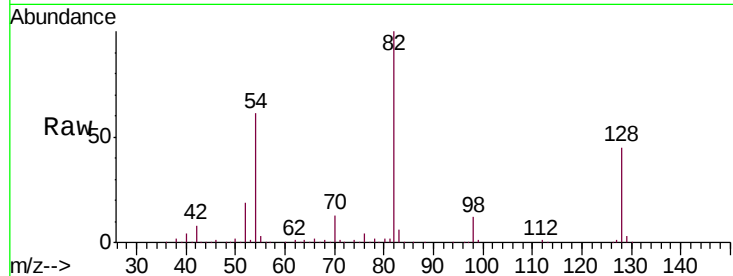

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.83 min Scan# 1316
Delta R.T. -0.01 min
Lab File: BF111492.D
Acq: 16 Dec 2018 3:39

Tgt Ion: 164 Resp: 159672
Ion Ratio Lower Upper
164 100
162 102.4 81.4 122.0
160 43.8 35.7 53.5


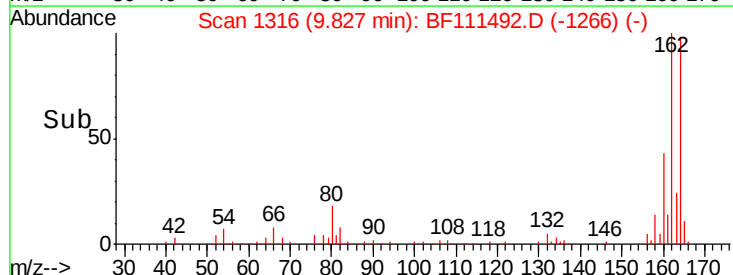
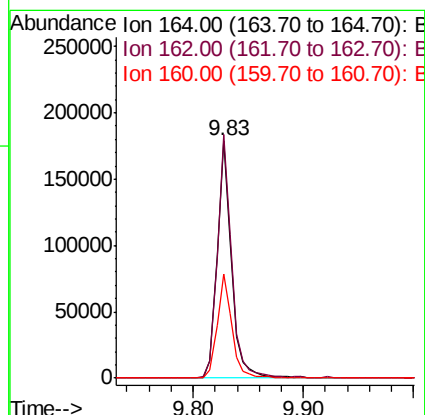
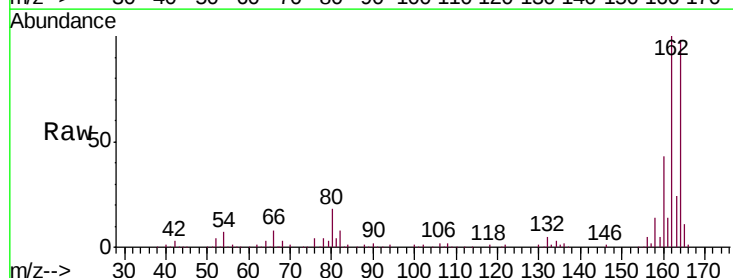


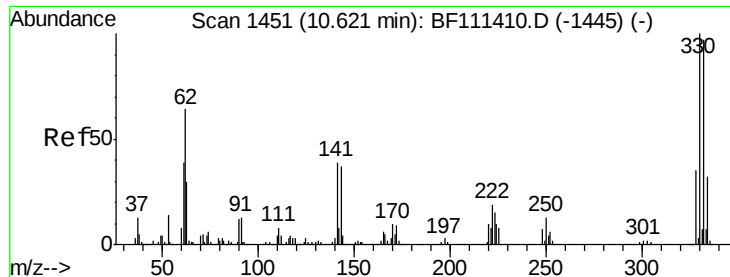

#42
 2,4,6-Tribromophenol
 Concen: 133.626 ng
 RT: 10.62 min Scan# 1450
 Delta R.T. -0.01 min
 Lab File: BF111492.D
 Acq: 16 Dec 2018 3:39




Instrument :
 BNA_F
 ClientSampleId :
 TEST-PIT-2


Tgt Ion:330 Resp: 191128
 Ion Ratio Lower Upper
 330 100
 332 96.3 76.0 114.0
 141 39.6 31.0 46.6

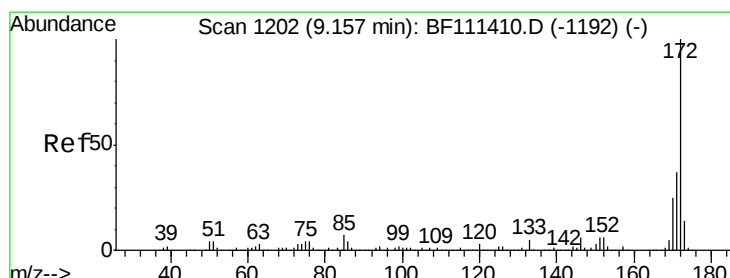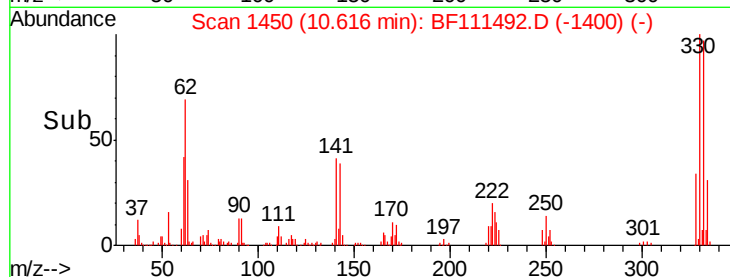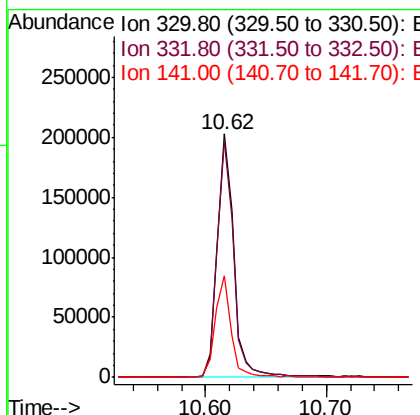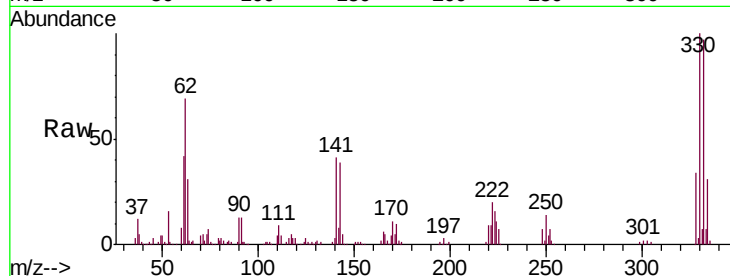

#45
 2-Fluorobiphenyl
 Concen: 114.428 ng
 RT: 9.15 min Scan# 1201
 Delta R.T. -0.01 min
 Lab File: BF111492.D
 Acq: 16 Dec 2018 3:39

Tgt Ion:172 Resp: 1182858
 Ion Ratio Lower Upper
 172 100
 171 34.5 33.0 49.4
 170 23.2 22.3 33.5

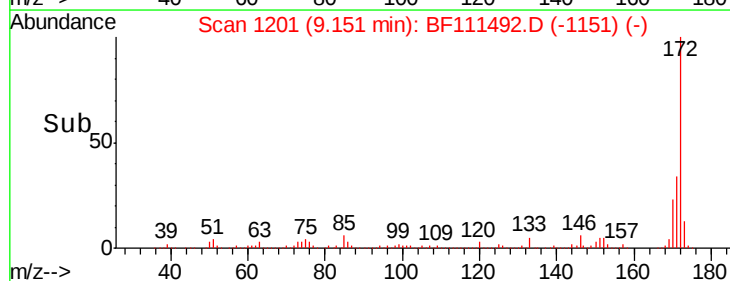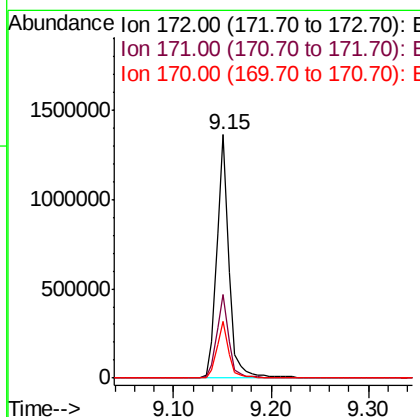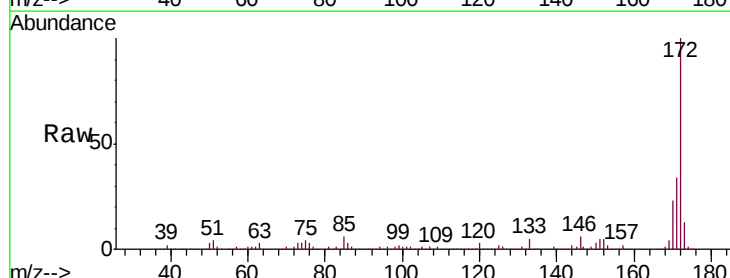

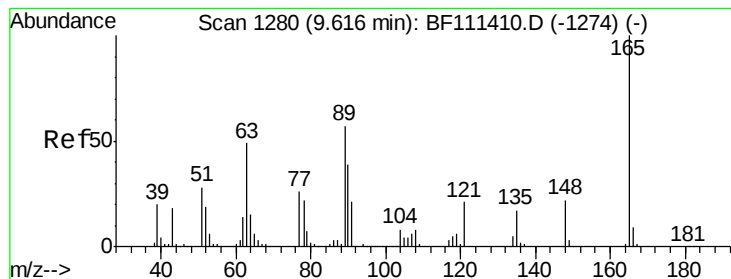

#51

2,6-Dinitrotoluene

Concen: 7.553 ng

RT: 9.83 min Scan# 1316

Delta R.T. 0.21 min

Lab File: BF111492.D

Acq: 16 Dec 2018 3:39

Instrument :

BNA_F

ClientSampled :

TEST-PIT-2


Tgt Ion:165 Resp: 19550

Ion Ratio Lower Upper

165 100

63 2.3 40.5 60.7#




89 1.7 40.0 60.0#

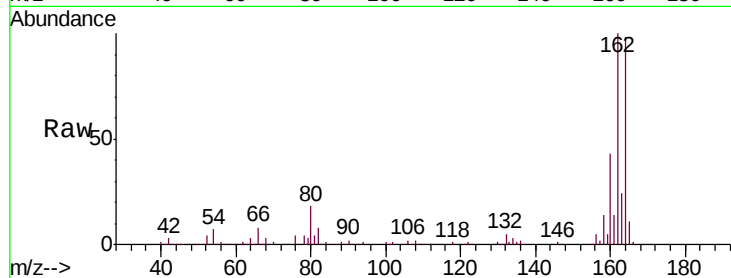

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

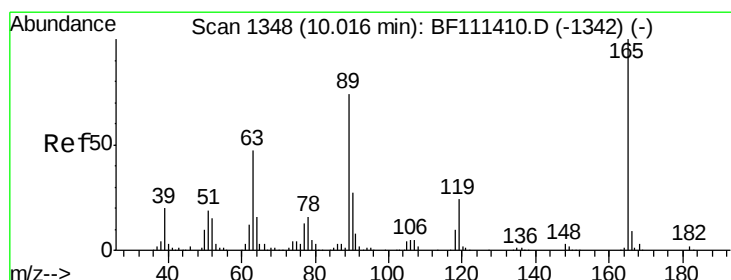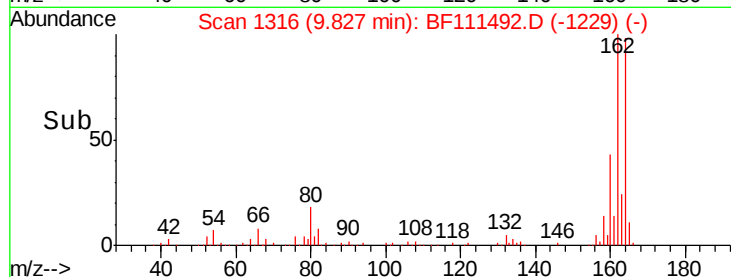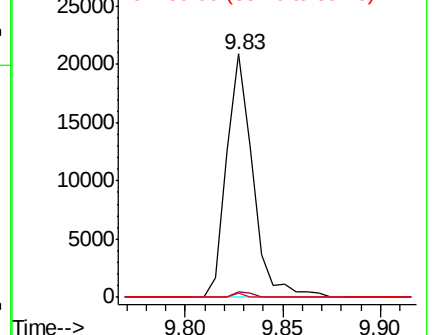

#57

2,4-Dinitrotoluene

Concen: 5.755 ng

RT: 9.83 min Scan# 1316

Delta R.T. -0.19 min

Lab File: BF111492.D

Acq: 16 Dec 2018 3:39

Tgt Ion:165 Resp: 19550


Ion Ratio Lower Upper

165 100

63 2.3 34.6 52.0#

89 1.7 56.2 84.4#

182 0.0 1.8 2.6#


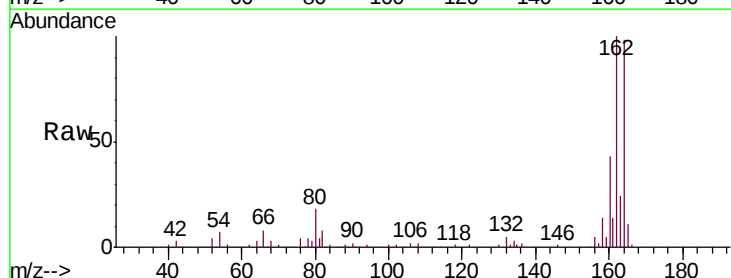



Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

Ion 182.00 (181.70 to 182.70): E

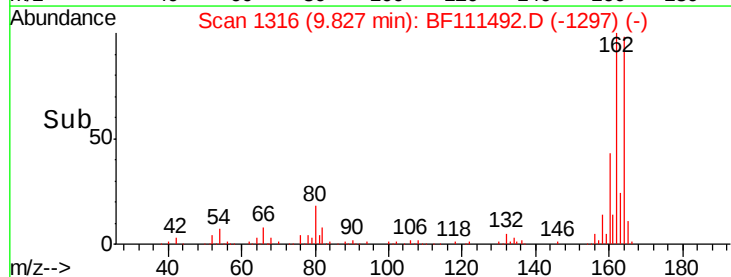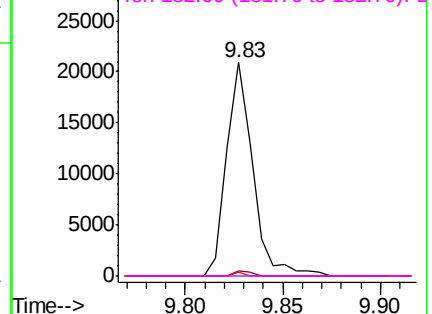


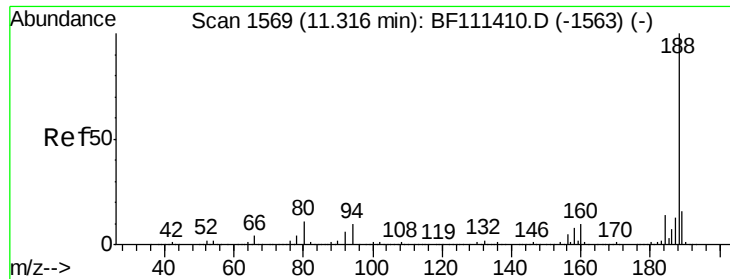




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.31 min Scan# 1568
Delta R.T. -0.01 min
Lab File: BF111492.D
Acq: 16 Dec 2018 3:39

Instrument :
BNA_F
ClientSampleId :
TEST-PIT-2

Tgt Ion:188 Resp: 270918
Ion Ratio Lower Upper
188 100
94 10.1 9.6 14.4
80 11.1 9.8 14.6

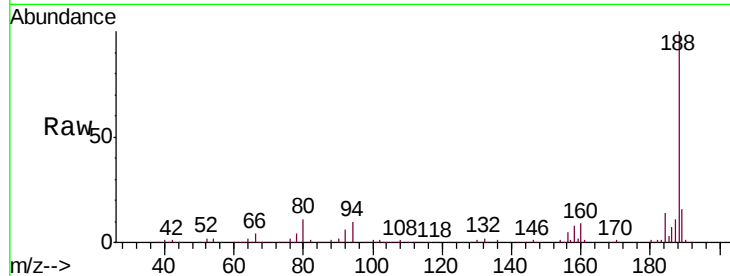


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

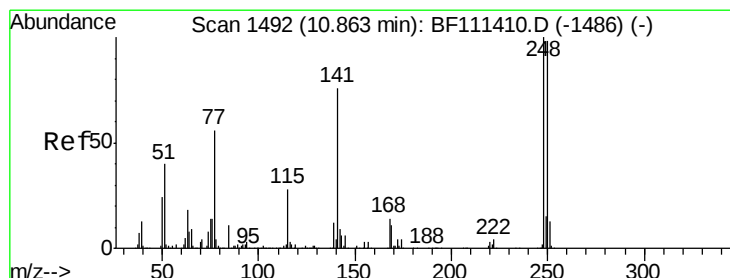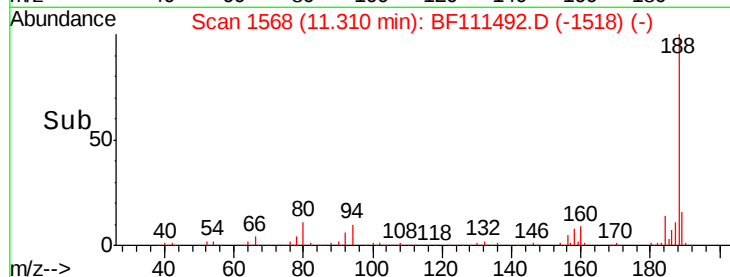
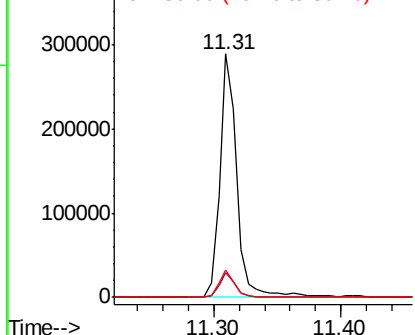



#67
4-Bromophenyl-phenylether
Concen: 4.126 ng
RT: 10.62 min Scan# 1450
Delta R.T. -0.25 min
Lab File: BF111492.D
Acq: 16 Dec 2018 3:39

Tgt Ion:248 Resp: 12048
Ion Ratio Lower Upper
248 100
250 200.5 77.0 115.4#
141 607.2 63.0 94.6#

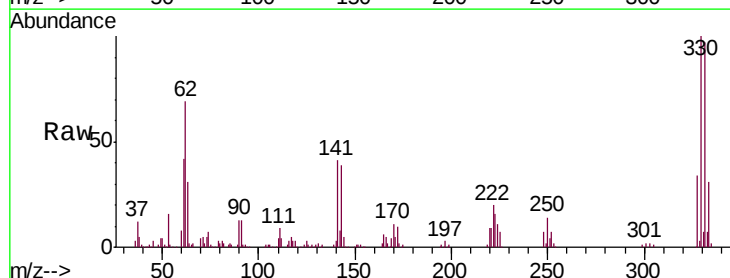

Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E



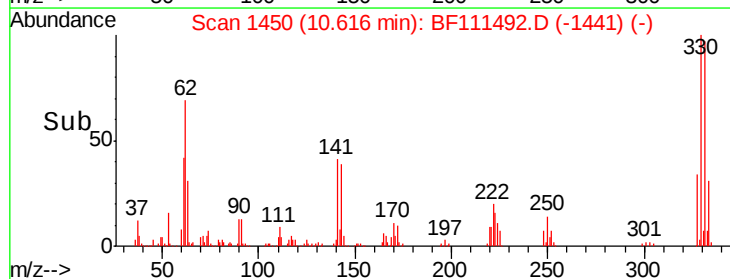
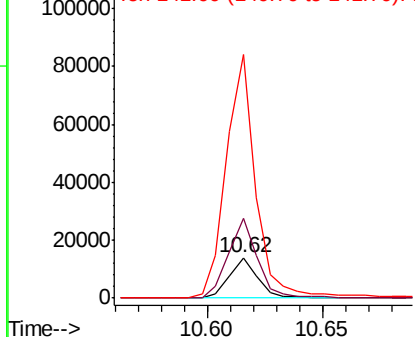


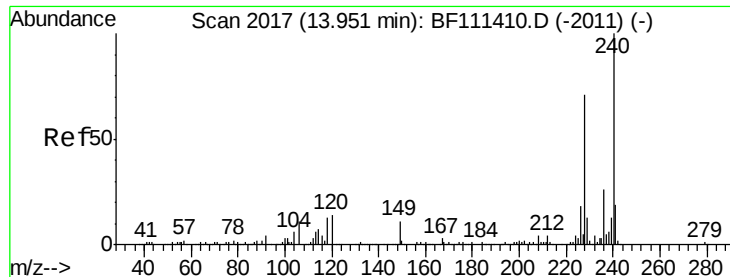

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.95 min Scan# 2017
Delta R.T. -0.00 min
Lab File: BF111492.D
Acq: 16 Dec 2018 3:39




Instrument :
BNA_F
ClientSampleId :
TEST-PIT-2


Tgt Ion:240 Resp: 264118
Ion Ratio Lower Upper
240 100
120 10.9 12.2 18.2#
236 24.2 20.2 30.2

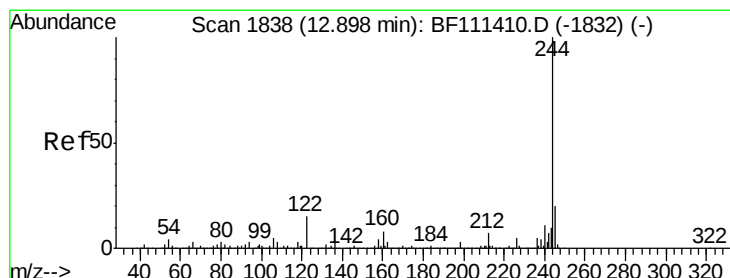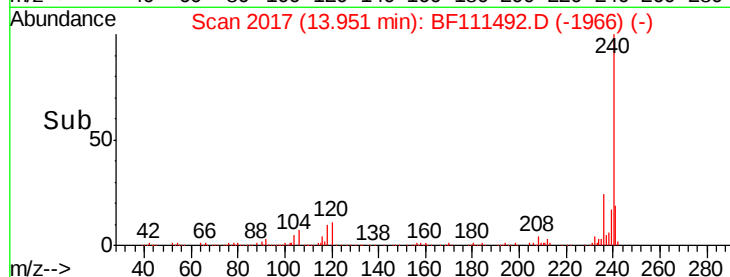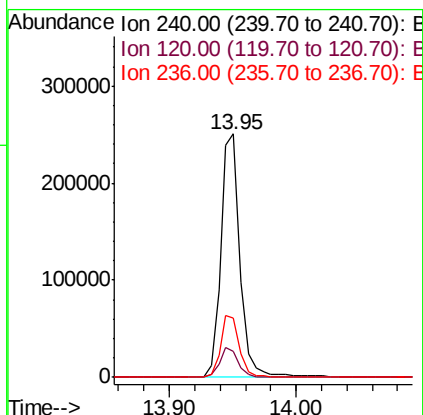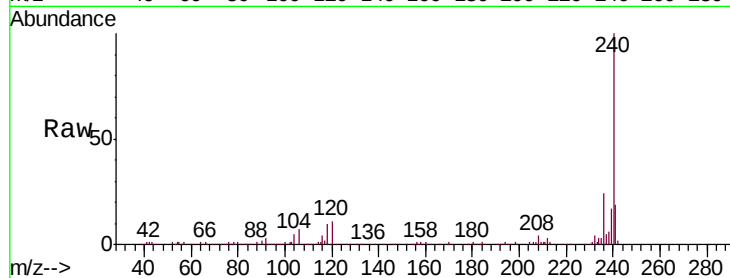

#79
Terphenyl-d14
Concen: 101.179 ng
RT: 12.90 min Scan# 1838
Delta R.T. -0.00 min
Lab File: BF111492.D
Acq: 16 Dec 2018 3:39

Tgt Ion:244 Resp: 1138014
Ion Ratio Lower Upper
244 100
212 6.6 5.7 8.5
122 13.8 13.1 19.7

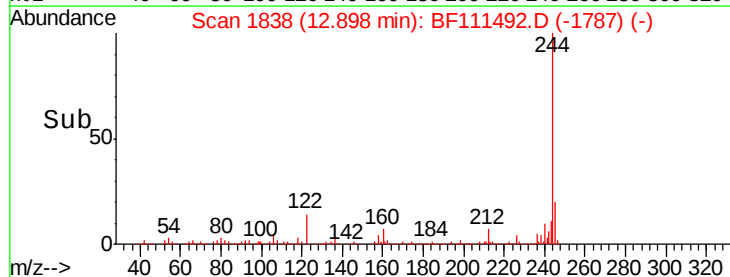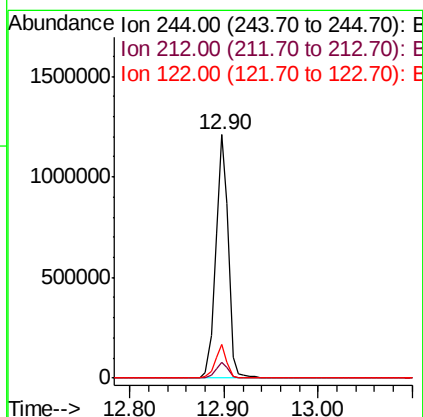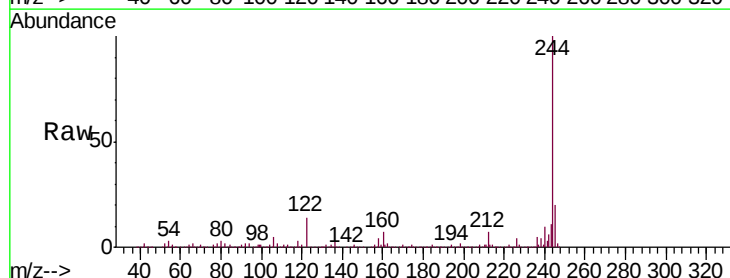

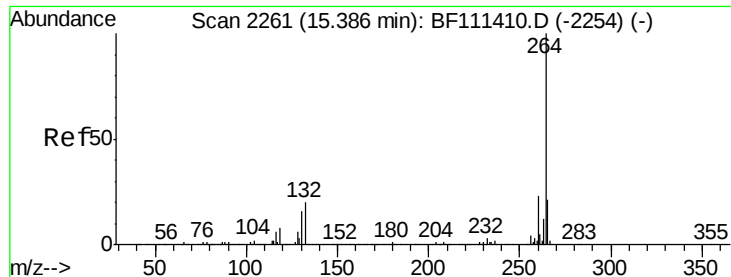

#87
Perylene-d12
Concen: 20.000 ng
RT: 15.39 min Scan# 2261
Delta R.T. -0.00 min
Lab File: BF111492.D
Acq: 16 Dec 2018 3:39

Instrument :
BNA_F
ClientSampleId :
TEST-PIT-2

Tgt Ion:	264	Resp:	174853
Ion	Ratio	Lower	Upper
264	100		
260	22.7	18.3	27.5
265	23.2	17.7	26.5

