


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121518\
 Data File : BF111457.D
 Acq On : 15 Dec 2018 9:55
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 14 13:26:17 2018

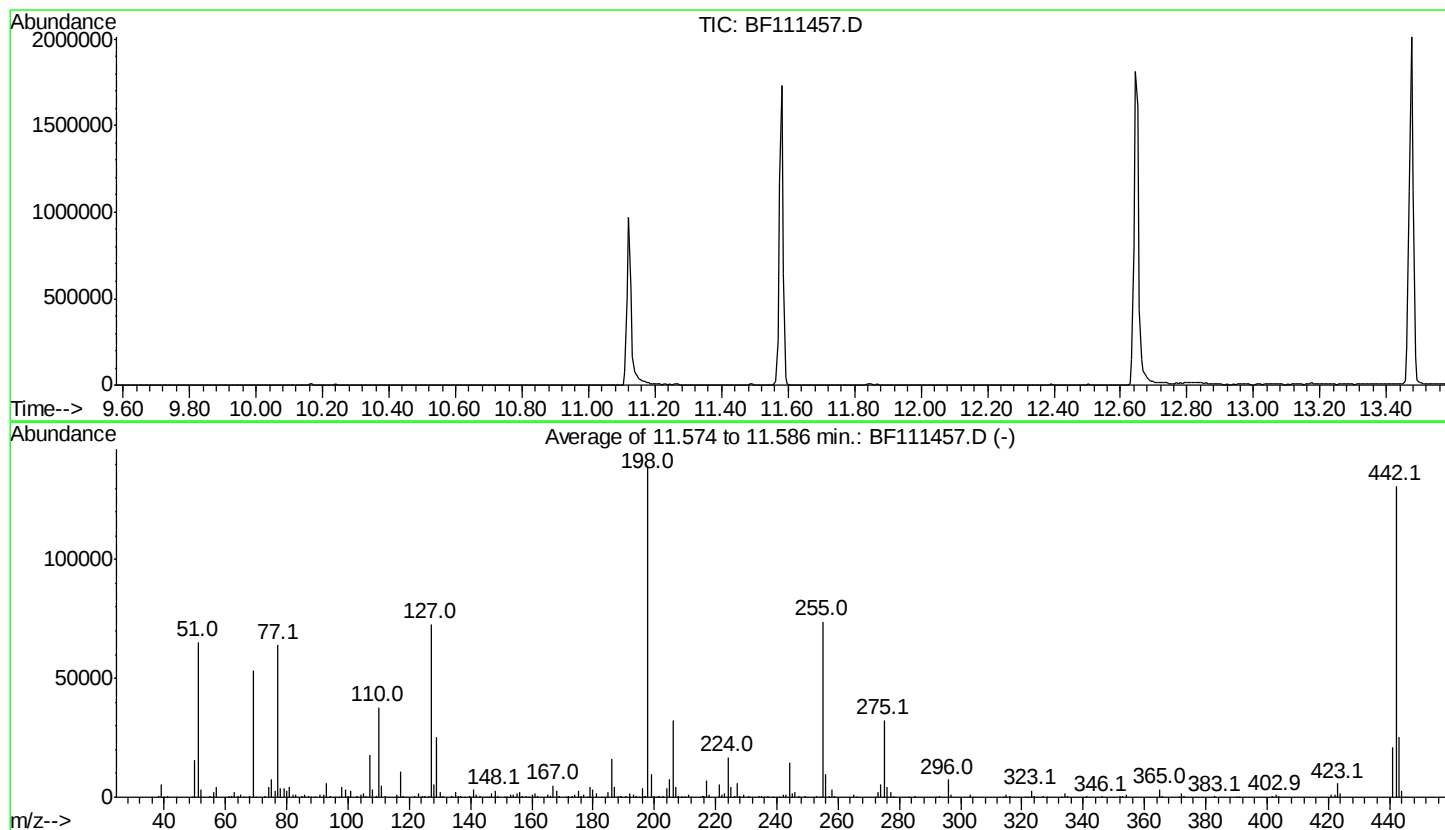

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.8	65306	PASS
68	69	0.00	2	1.4	723	PASS
69	198	0.00	100	38.0	53077	PASS
70	69	0.00	2	0.2	100	PASS
127	198	10	80	52.1	72717	PASS
197	198	0.00	2	0.4	594	PASS
198	198	100	100	100.0	139514	PASS
199	198	5	9	6.8	9536	PASS
275	198	10	60	23.3	32453	PASS
365	198	1	100	2.5	3510	PASS
441	198	0.01	100	15.0	20861	PASS
442	198	50	100	94.0	131157	PASS
443	442	15	24	19.5	25595	PASS