

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121522\
 Data File : BF131648.D
 Acq On : 15 Dec 2022 14:35
 Operator : CG\JU
 Sample : N6038-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RB-30-(6-8)

Quant Time: Dec 16 01:50:45 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 16 01:44:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.881	152	62324	20.000	ng	0.00
21) Naphthalene-d8	8.169	136	224380	20.000	ng	0.00
39) Acenaphthene-d10	9.933	164	132762	20.000	ng	0.00
64) Phenanthrene-d10	11.427	188	268447	20.000	ng	0.00
76) Chrysene-d12	14.080	240	152953	20.000	ng	# 0.00
86) Perylene-d12	15.580	264	135907	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.498	112	419537	112.301	ng	0.00
7) Phenol-d6	6.510	99	548894	112.122	ng	0.00
23) Nitrobenzene-d5	7.445	82	379055	63.869	ng	0.00
42) 2,4,6-Tribromophenol	10.727	330	160536	108.836	ng	0.00
45) 2-Fluorobiphenyl	9.251	172	659962	62.678	ng	0.00
79) Terphenyl-d14	13.021	244	784936	70.379	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121522\
Data File : BF131648.D
Acq On : 15 Dec 2022 14:35
Operator : CG\JU
Sample : N6038-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RB-30-(6-8)

Quant Time: Dec 16 01:50:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 16 01:44:46 2022
Response via : Initial Calibration




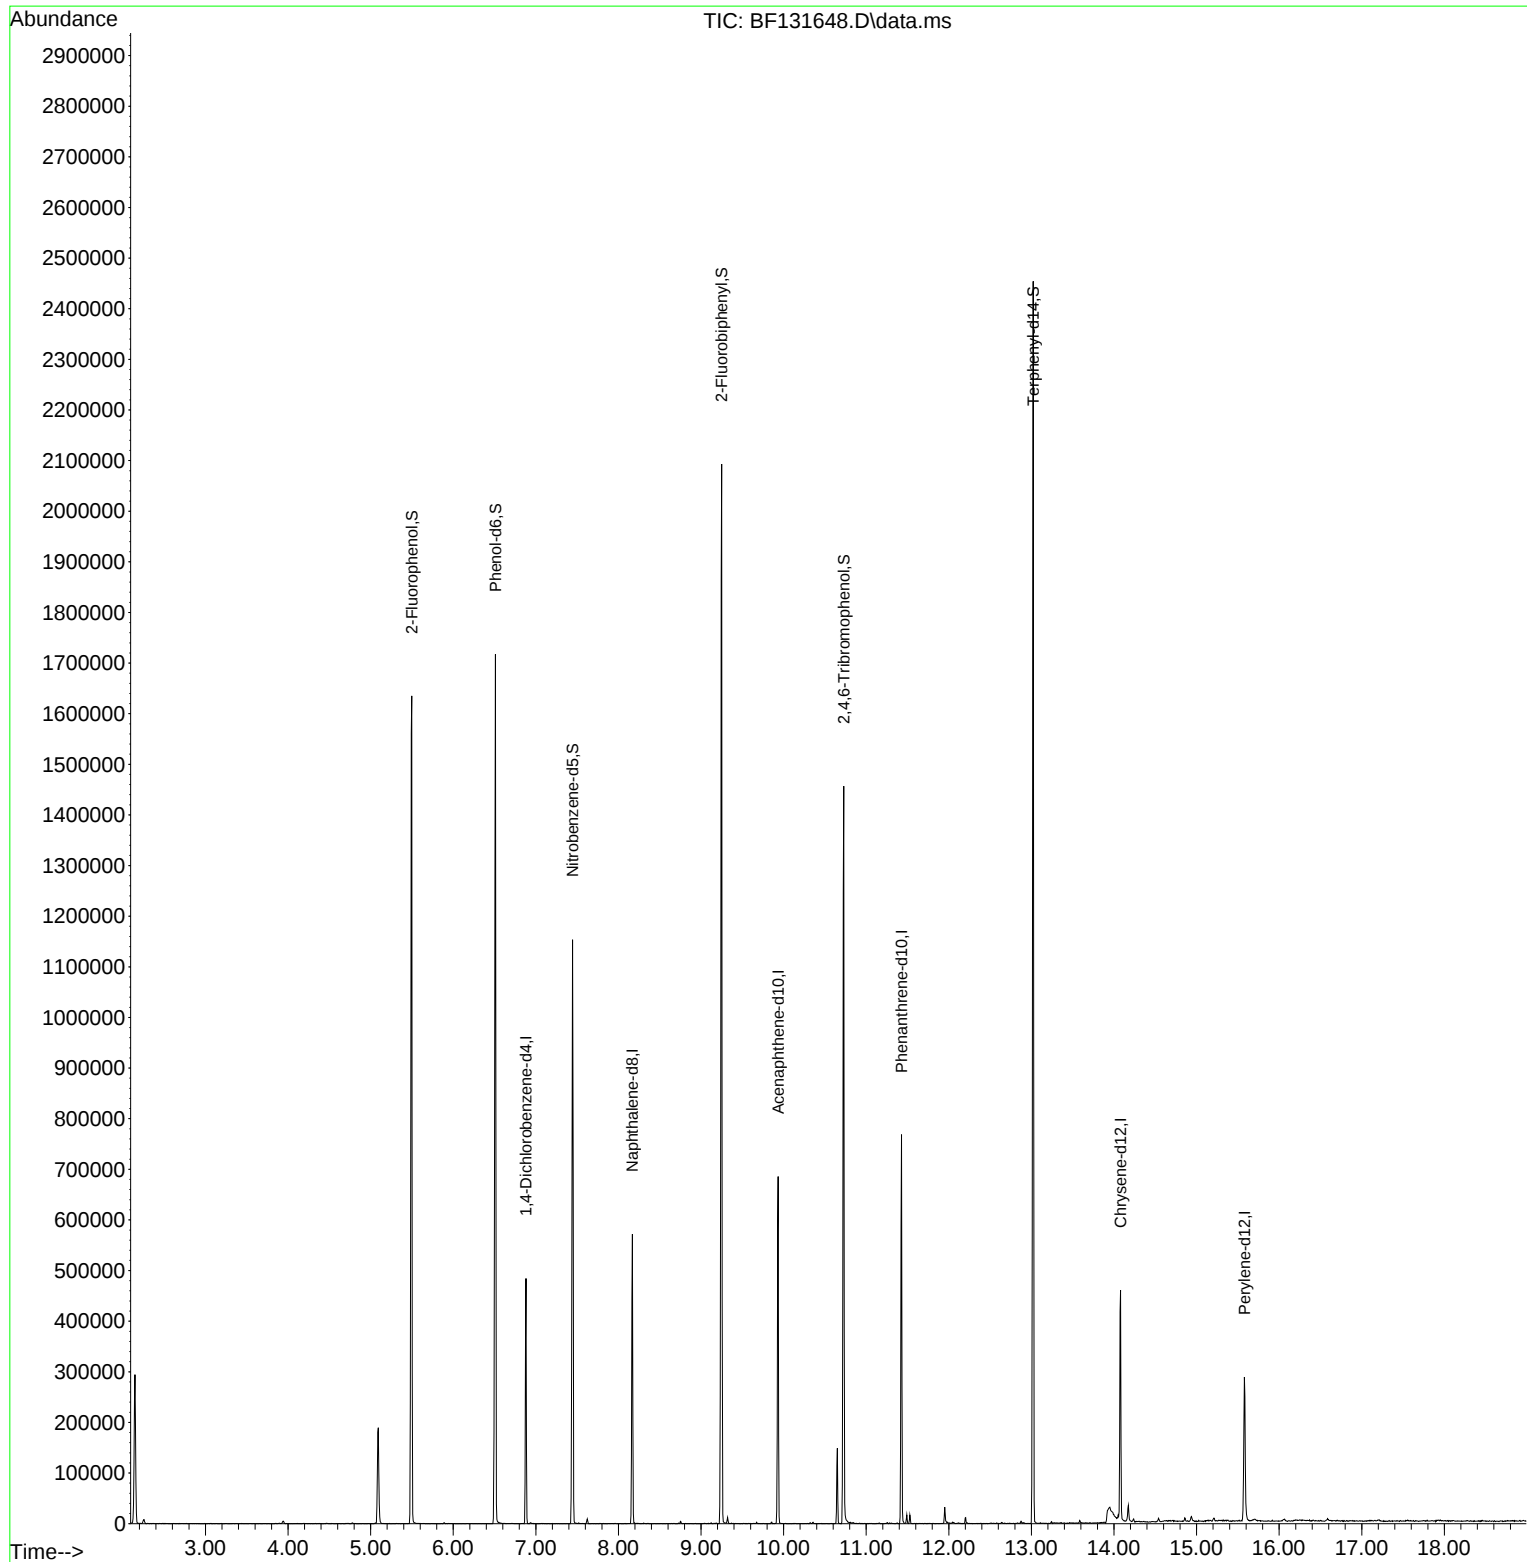




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.881 min Scan# 81
 Delta R.T. -0.000 min
 Lab File: BF131648.D
 Acq: 15 Dec 2022 14:35




Instrument :
 BNA_F
 ClientSampleId :
 RB-30-(6-8)


Tgt Ion:152 Resp: 62324
 Ion Ratio Lower Upper
 152 100
 150 149.5 116.7 175.1
 115 64.9 54.6 82.0

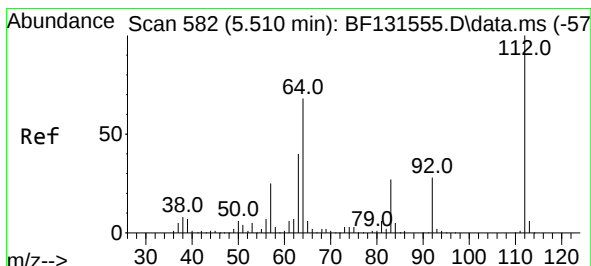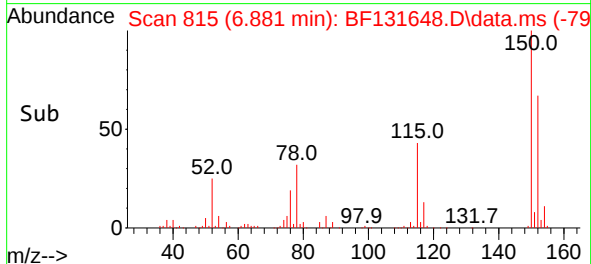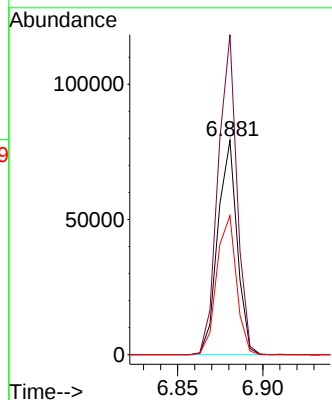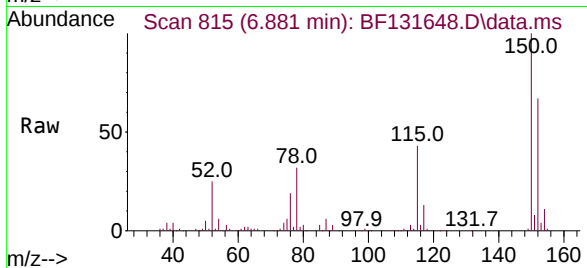

#5
 2-Fluorophenol
 Concen: 112.301 ng
 RT: 5.498 min Scan# 580
 Delta R.T. 0.006 min
 Lab File: BF131648.D
 Acq: 15 Dec 2022 14:35

Tgt Ion:112 Resp: 419537
 Ion Ratio Lower Upper
 112 100
 64 61.9 54.5 81.7
 63 35.3 31.9 47.9


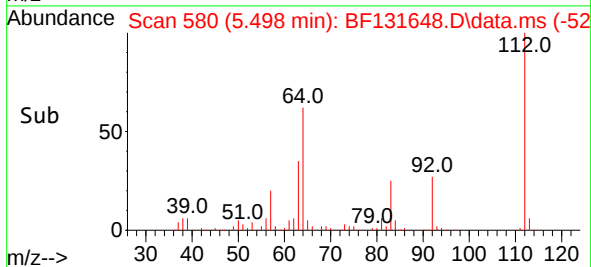
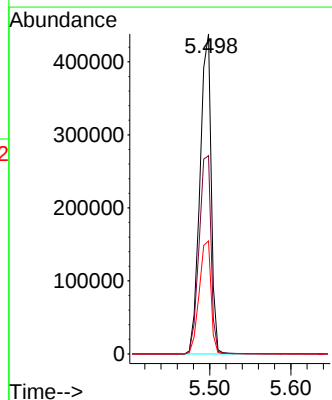
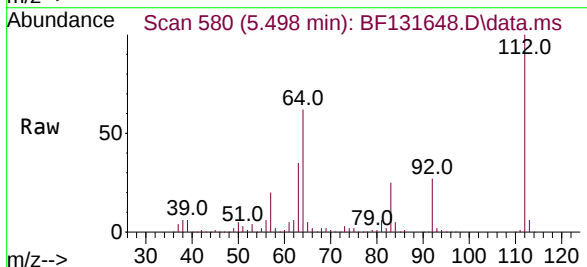


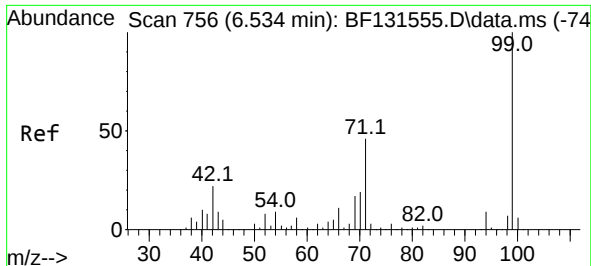

#7
Phenol-d6
Concen: 112.122 ng
RT: 6.510 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF131648.D
Acq: 15 Dec 2022 14:35




Instrument :
BNA_F
ClientSampleId :
RB-30-(6-8)

Tgt Ion: 99 Resp: 548894
Ion Ratio Lower Upper
99 100
42 19.5 17.9 26.9
71 42.6 37.2 55.8

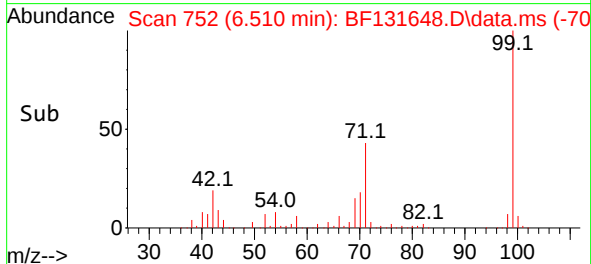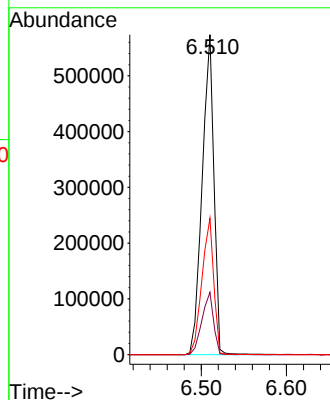

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.169 min Scan# 1034
Delta R.T. -0.006 min
Lab File: BF131648.D
Acq: 15 Dec 2022 14:35

Tgt Ion: 136 Resp: 224380
Ion Ratio Lower Upper
136 100
137 10.4 8.1 12.1
54 8.1 6.0 9.0
68 5.6 3.8 5.8


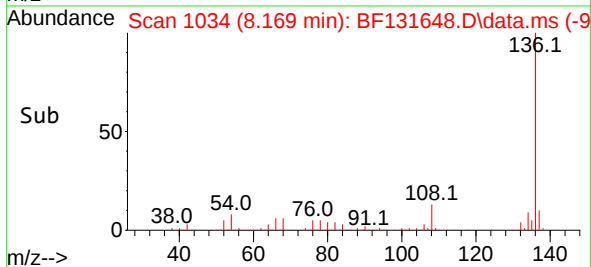
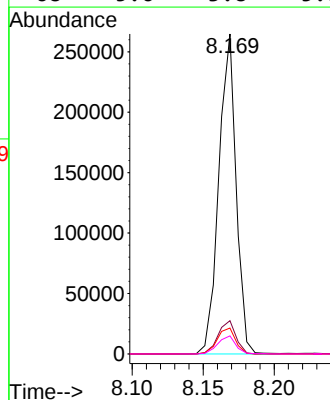
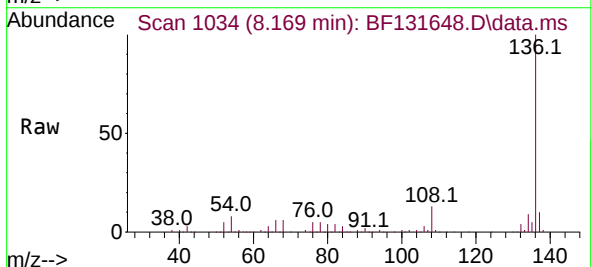




#23
Nitrobenzene-d5
Concen: 63.869 ng
RT: 7.445 min Scan# 911
Delta R.T. -0.006 min
Lab File: BF131648.D
Acq: 15 Dec 2022 14:35




Instrument :
BNA_F
ClientSampleId :
RB-30-(6-8)


Tgt Ion: 82 Resp: 379055
Ion Ratio Lower Upper
82 100
128 33.5 26.1 39.1
54 48.4 40.6 60.8

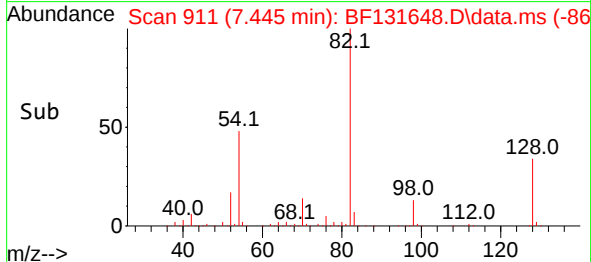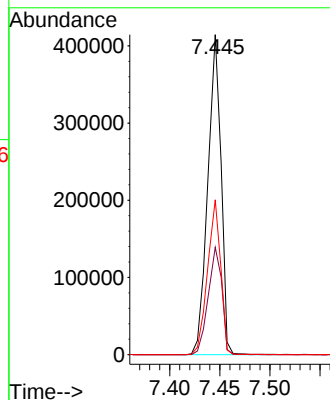

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.933 min Scan# 1334
Delta R.T. -0.006 min
Lab File: BF131648.D
Acq: 15 Dec 2022 14:35

Tgt Ion:164 Resp: 132762
Ion Ratio Lower Upper
164 100
162 101.3 81.0 121.6
160 44.8 35.0 52.6

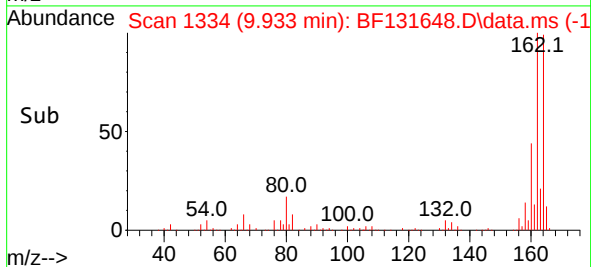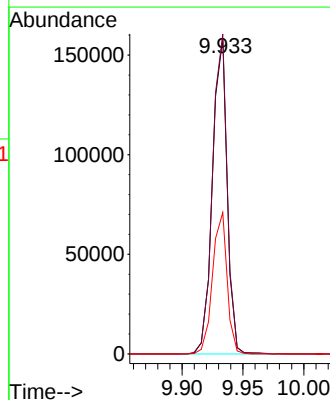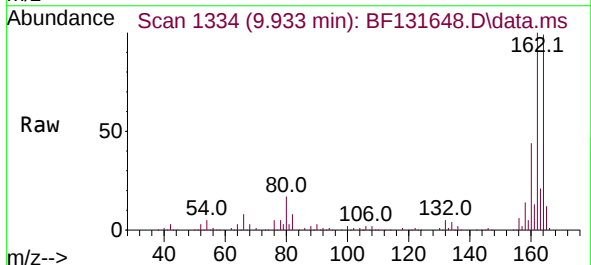

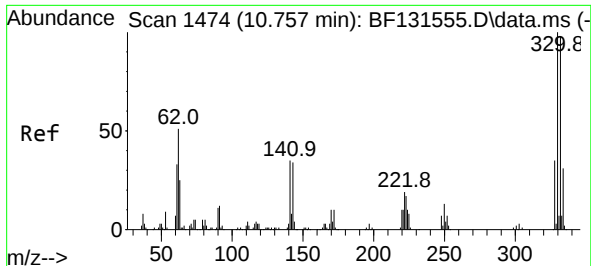

#42

2,4,6-Tribromophenol

Concen: 108.836 ng

RT: 10.727 min Scan# 1474

Delta R.T. -0.006 min

Lab File: BF131648.D

Acq: 15 Dec 2022 14:35

Instrument :

BNA_F

ClientSampleId :

RB-30-(6-8)





Tgt Ion:330 Resp: 160536

Ion Ratio Lower Upper

330 100

332 93.3 78.3 117.5

141 38.6 32.6 49.0

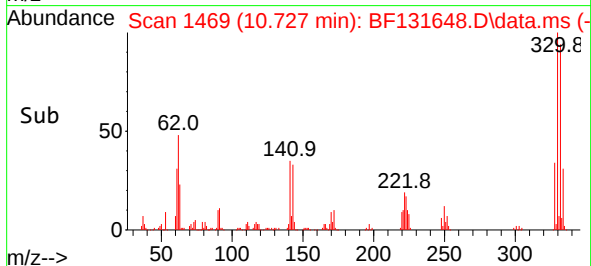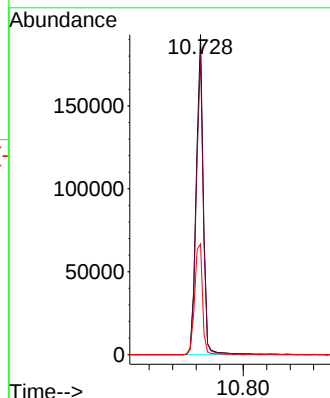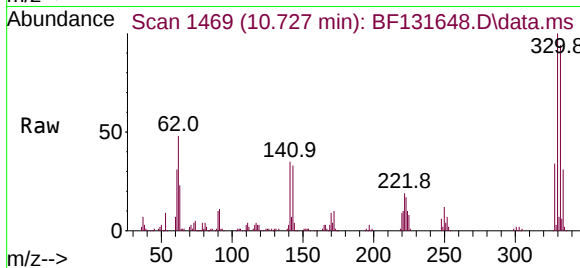

#45

2-Fluorobiphenyl

Concen: 62.678 ng

RT: 9.251 min Scan# 1218

Delta R.T. 0.000 min

Lab File: BF131648.D

Acq: 15 Dec 2022 14:35




Tgt Ion:172 Resp: 659962


Ion Ratio Lower Upper

172 100

171 35.2 28.3 42.5

170 23.7 19.3 28.9

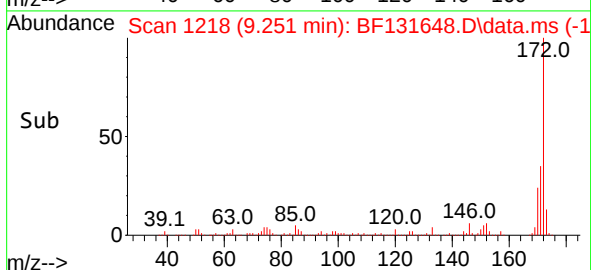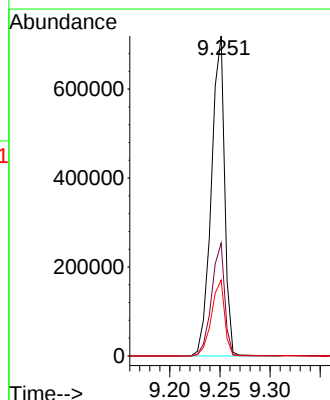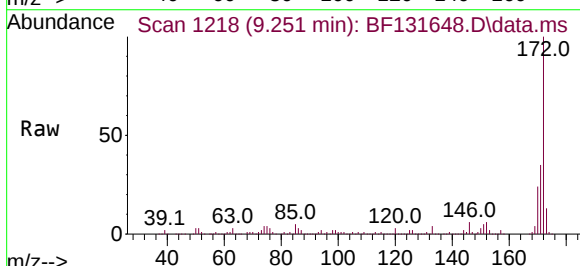



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.427 min Scan# 11

Delta R.T. 0.000 min

Lab File: BF131648.D

Acq: 15 Dec 2022 14:35

Instrument :

BNA_F

ClientSampleId :

RB-30-(6-8)





Tgt Ion:188 Resp: 268447

Ion Ratio Lower Upper

188 100

94 7.0 5.5 8.3

80 8.1 6.6 10.0

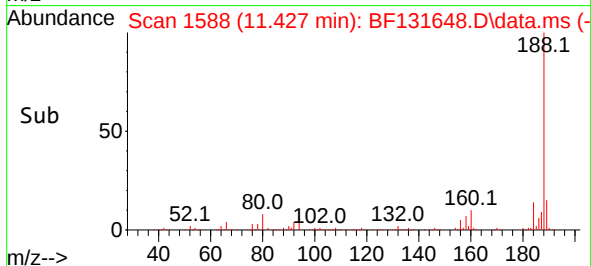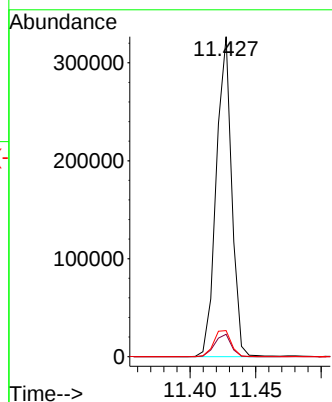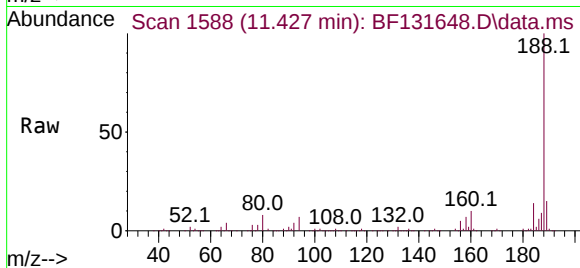

#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.080 min Scan# 2039

Delta R.T. 0.000 min

Lab File: BF131648.D

Acq: 15 Dec 2022 14:35




Tgt Ion:240 Resp: 152953


Ion Ratio Lower Upper

240 100

120 7.0 4.6 7.0#

236 26.4 20.2 30.2


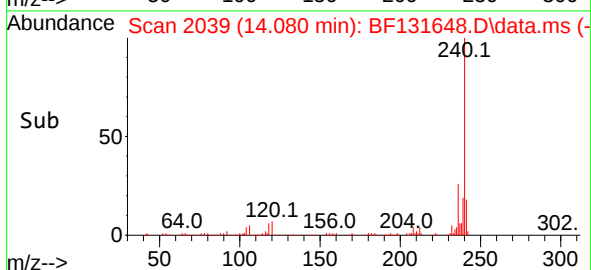
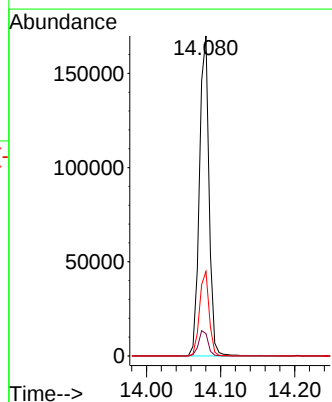
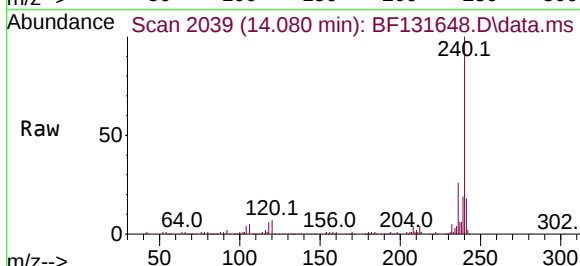


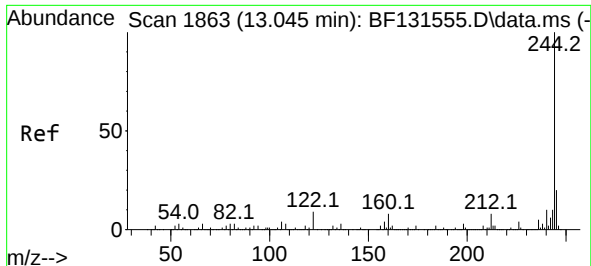

#79
 Terphenyl-d14
 Concen: 70.379 ng
 RT: 13.021 min Scan# 1863
 Delta R.T. 0.000 min
 Lab File: BF131648.D
 Acq: 15 Dec 2022 14:35

Instrument :
 BNA_F
 ClientSampleId :
 RB-30-(6-8)

Tgt Ion:244 Resp: 784936
 Ion Ratio Lower Upper
 244 100
 212 8.1 6.5 9.7
 122 8.3 7.1 10.7

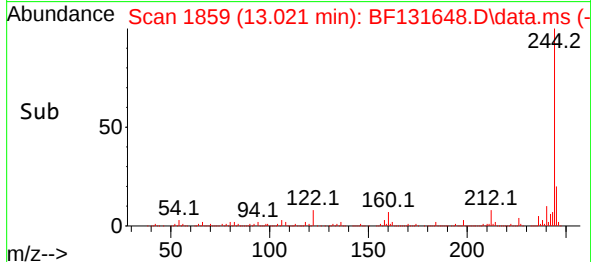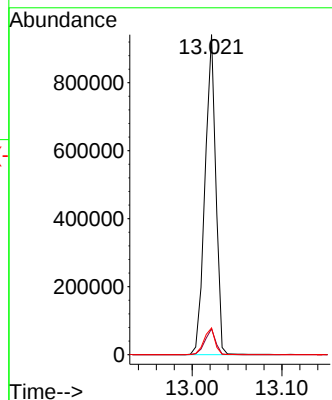

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.580 min Scan# 2294
 Delta R.T. 0.000 min
 Lab File: BF131648.D
 Acq: 15 Dec 2022 14:35

Tgt Ion:264 Resp: 135907
 Ion Ratio Lower Upper
 264 100
 260 23.3 20.6 30.8
 265 21.2 16.8 25.2

